

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD120622AR\
Data File : FD044605.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2022 15:37
Operator : YP/AJ
Sample : N5863-01D
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 07 04:01:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 112922.M
Quant Title : GC Extractables
QLast Update : Tue Nov 29 00:29:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	18.056	47235	0.371 ug/ml
20) T	Dibenz[a,h]anthracene...	18.056	47235	0.375 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD120622AR\
Data File : FD044605.D
Signal(s) : FID2B.ch
Acq On : 06 Dec 2022 15:37
Operator : YP/AJ
Sample : N5863-01D
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 07 04:01:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 112922.M
Quant Title : GC Extractables
QLast Update : Tue Nov 29 00:29:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

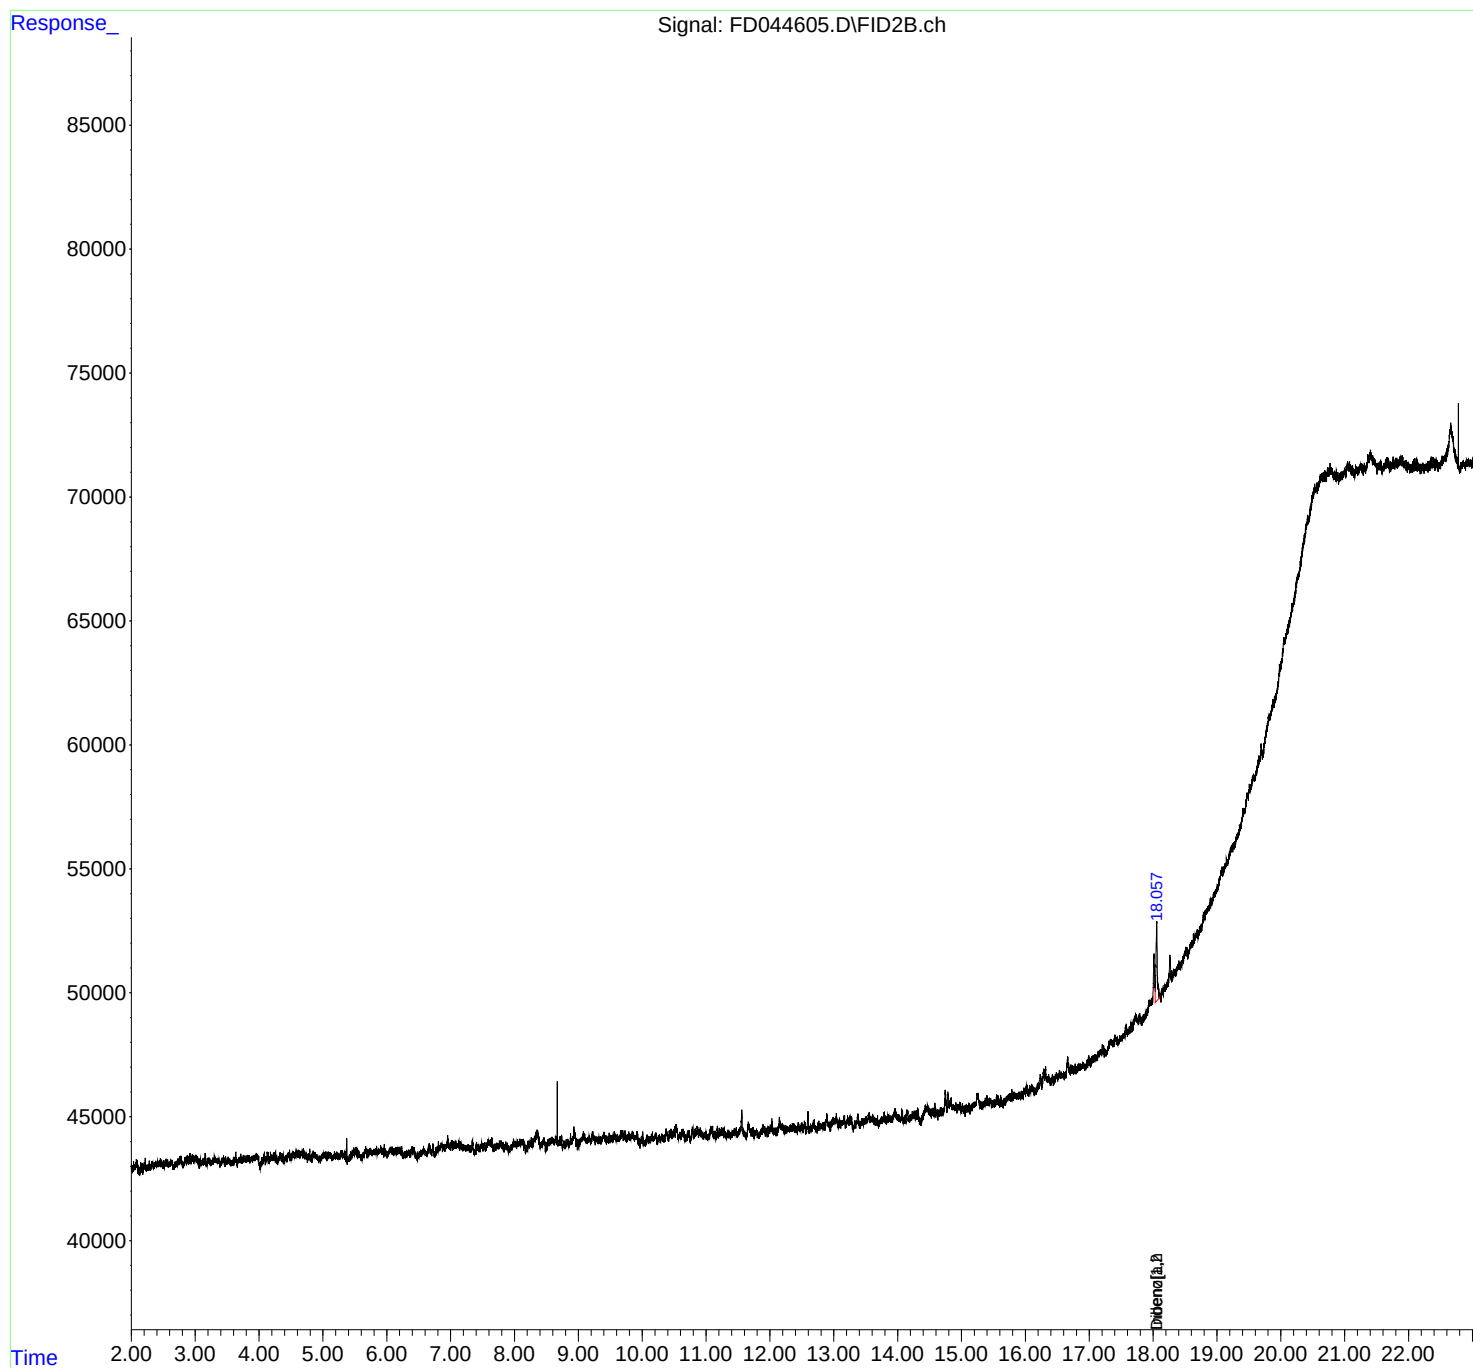


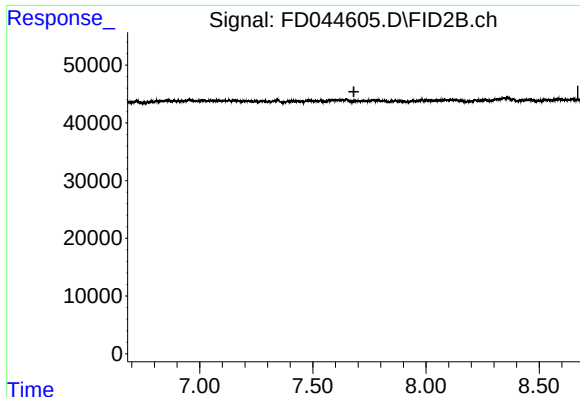

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T.: 7.682 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

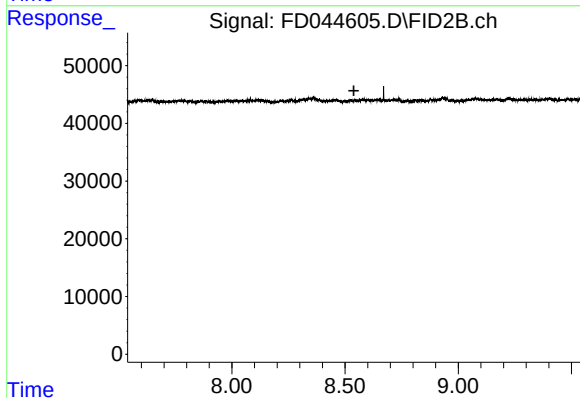


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 8.539 min
Response: 0
Conc: N.D.

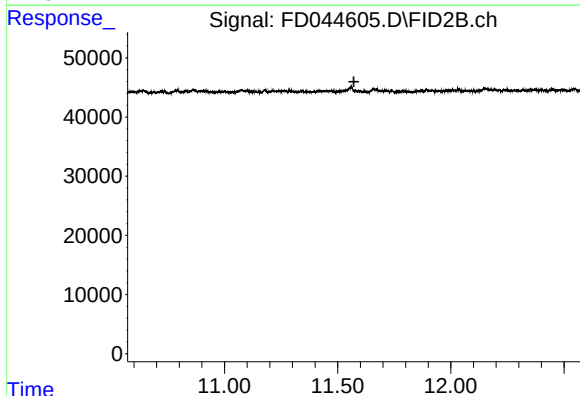


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.572 min
Response: 0
Conc: N.D.

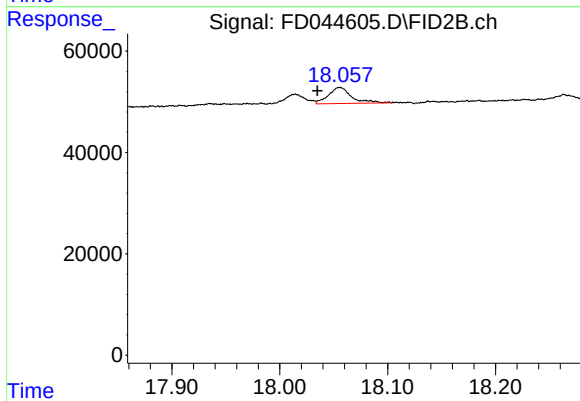

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.056 min
Delta R.T.: 0.021 min
Response: 47235
Conc: 0.37 ug/ml

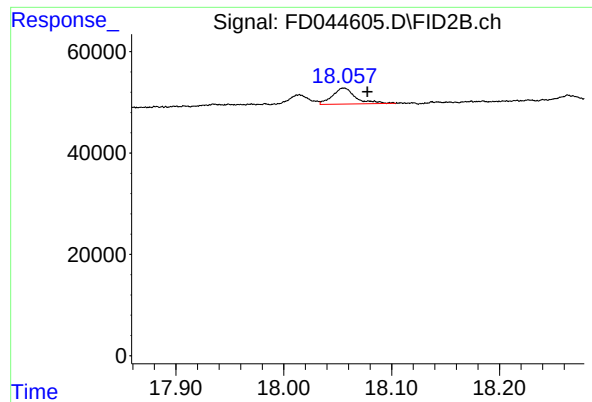

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.056 min
Delta R.T.: -0.022 min
Response: 47235
Conc: 0.38 ug/ml

Instrument :

FID_D

ClientSampleId :