

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD121521AL\
 Data File : FD039926.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2021 19:07
 Operator : AJ\MA
 Sample : M5022-56DL 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 TP15-E6DL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/16/2021
 Supervised By :Yogesh Patel 12/16/2021

Integration File: sample.E
 Quant Time: Dec 16 01:25:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 121521.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 15 16:44:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.835	6619676	42.167 ug/mlm
Spiked Amount 50.000		Recovery =	84.33%
12) S 1-chlorooctadecane (S...	12.269	2598208	21.039 ug/mlm
Spiked Amount 50.000		Recovery =	42.08%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD121521AL\
Data File : FD039926.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2021 19:07
Operator : AJ\MA
Sample : M5022-56DL 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
TP15-E6DL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/16/2021
Supervised By :Yogesh Patel 12/16/2021

Integration File: sample.E
Quant Time: Dec 16 01:25:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 121521.M
Quant Title : GC Extractables
QLast Update : Wed Dec 15 16:44:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

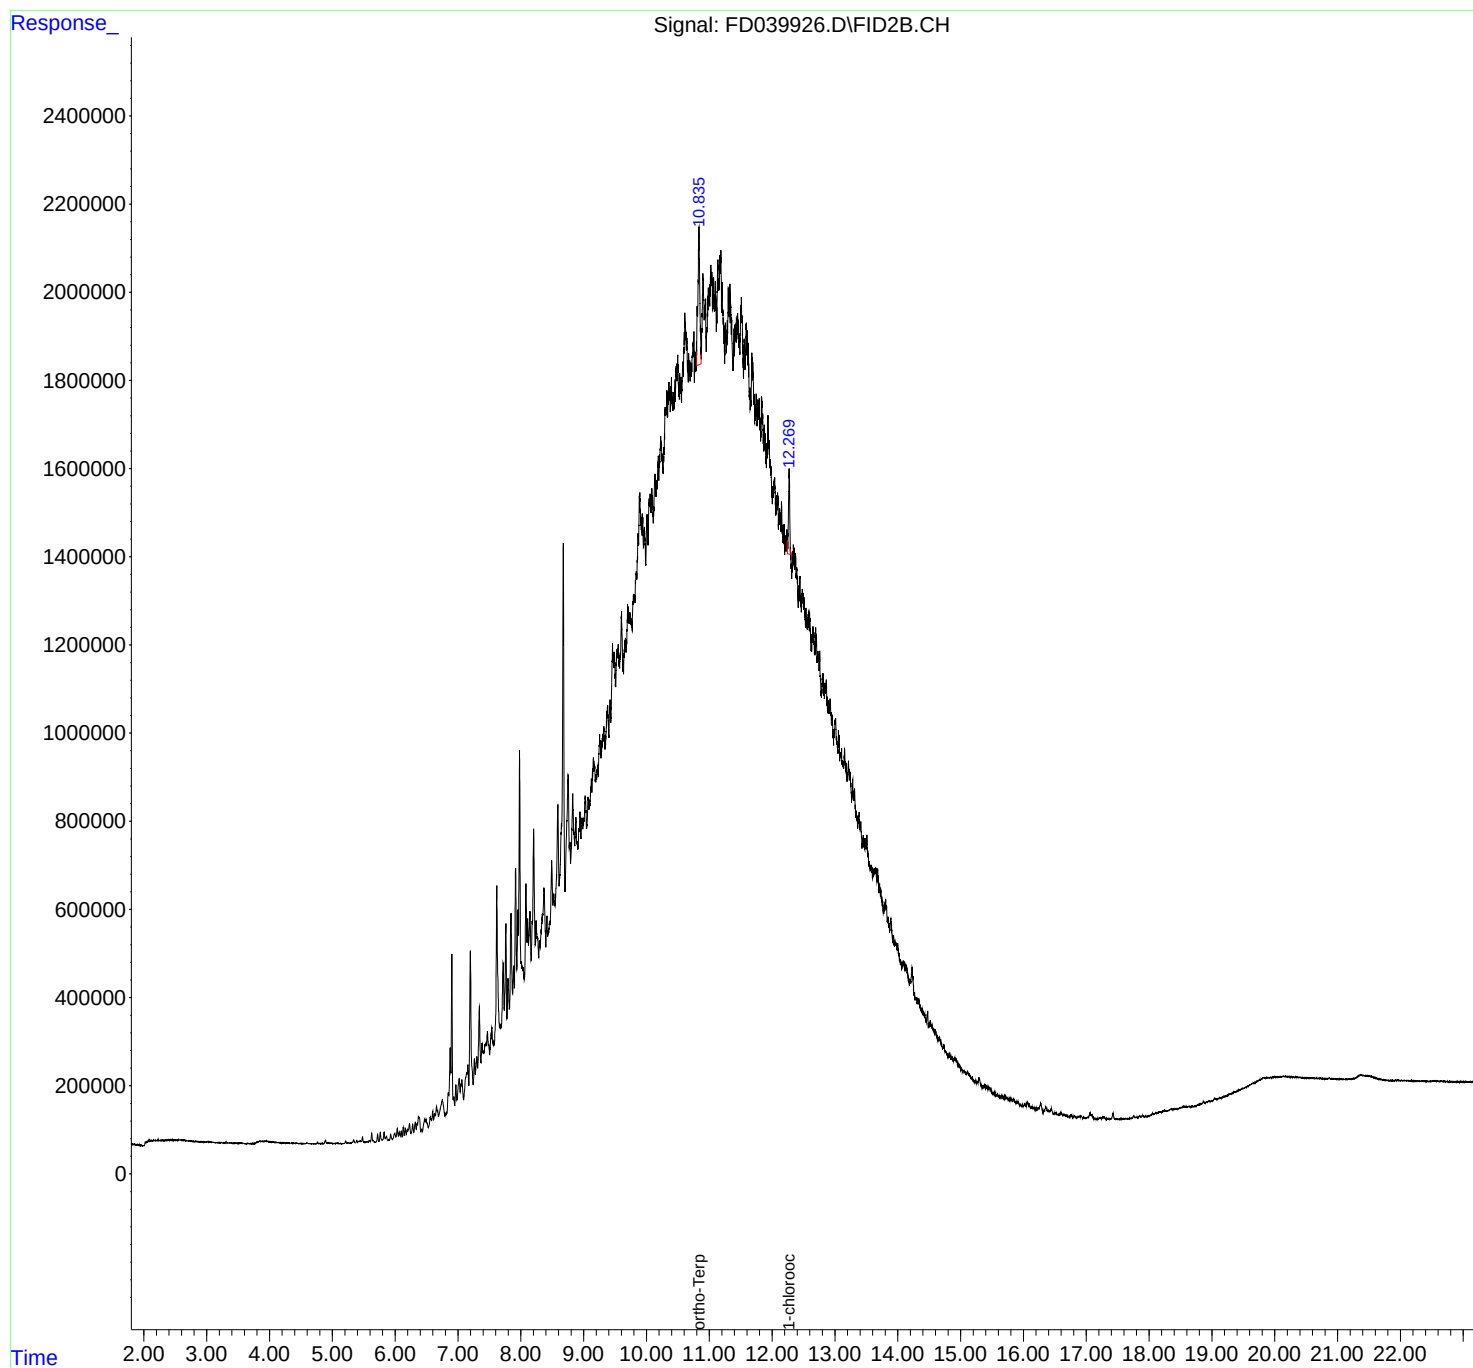

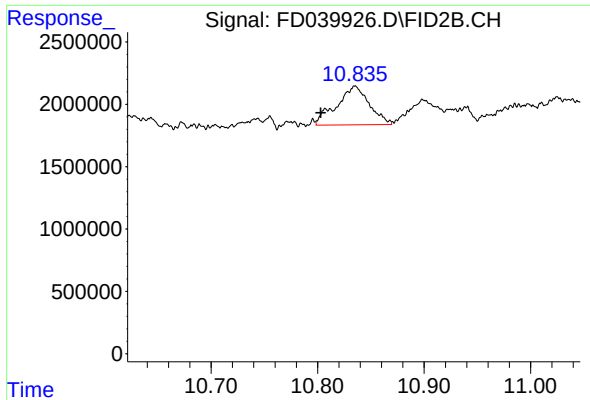


#9 ortho-Terphenyl (SURR)

R.T.: 10.835 min
Delta R.T.: 0.032 min
Response: 6619676
Conc: 42.17 ug/ml

Instrument :
FID_D
ClientSampleId :
TP15-E6DL

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/16/2021
Supervised By :Yogesh Patel 12/16/2021

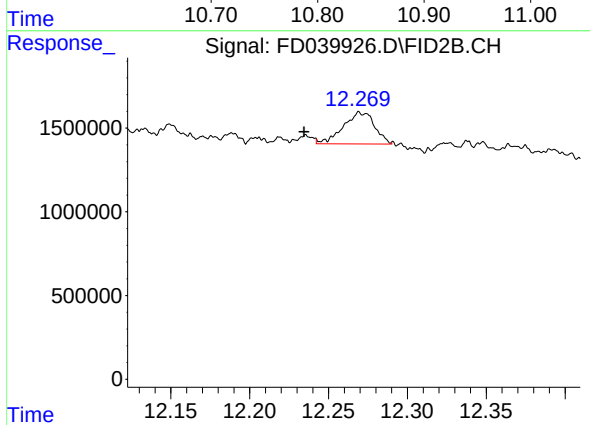

#12 1-chlorooctadecane (SURR)

R.T.: 12.269 min
Delta R.T.: 0.034 min
Response: 2598208
Conc: 21.04 ug/ml m