

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD123021AL\
 Data File : FD040340.D
 Signal(s) : FID2B.CH
 Acq On : 31 Dec 2021 13:43
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 31 21:36:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 122821.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 29 02:26:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	13.971	43777	0.312 ug/ml
15) T n-Hexacosane (C26)	14.986	49451	0.360 ug/ml
16) T n-Octacosane (C28)	15.931	63156	0.464 ug/ml
17) T n-Tricontane (C30)	16.812	66508	0.497 ug/ml
18) T n-Dotriacontane (C32)	17.678	26080	0.201 ug/ml
19) T n-Tetratriacontane (C34)	18.421	23551	0.194 ug/ml
20) T n-Hexatriacontane (C36)	19.226	85092	0.798 ug/ml
21) T n-Octatriacontane (C38)	19.858f	315023	3.411 ug/ml
22) T n-Tetracontane (C40)	20.759	164907	2.118 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD123021AL\
Data File : FD040340.D
Signal(s) : FID2B.CH
Acq On : 31 Dec 2021 13:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 31 21:36:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 122821.M
Quant Title : GC Extractables
QLast Update : Wed Dec 29 02:26:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

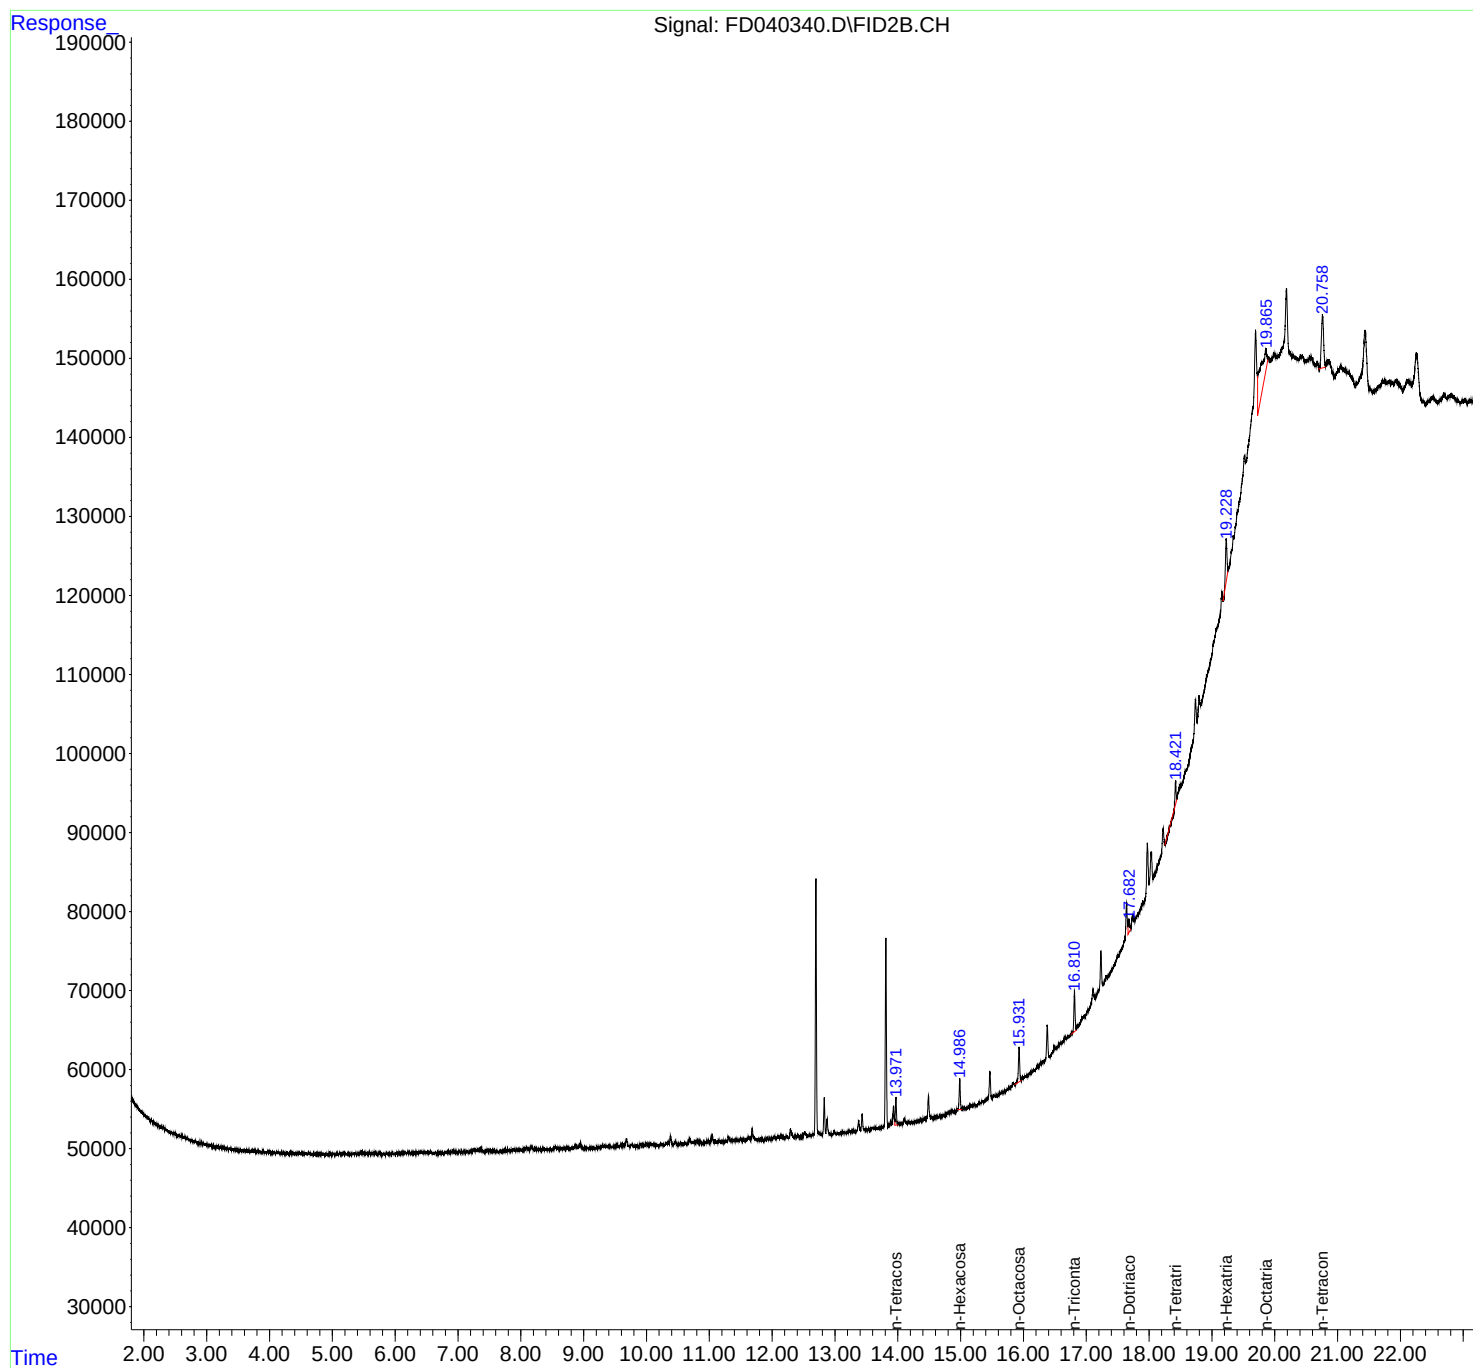


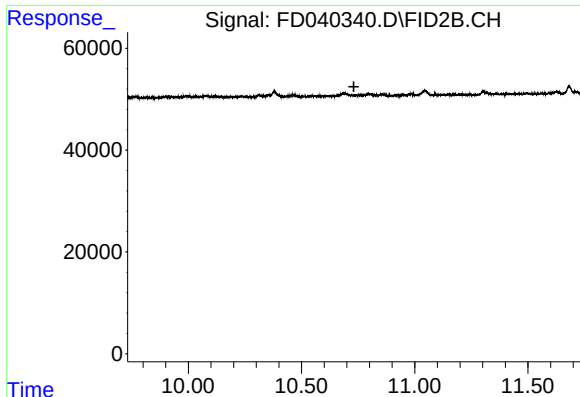

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.731 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

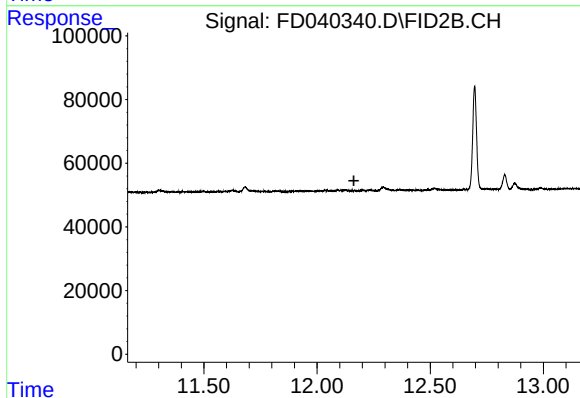


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.163 min
Response: 0
Conc: N.D.

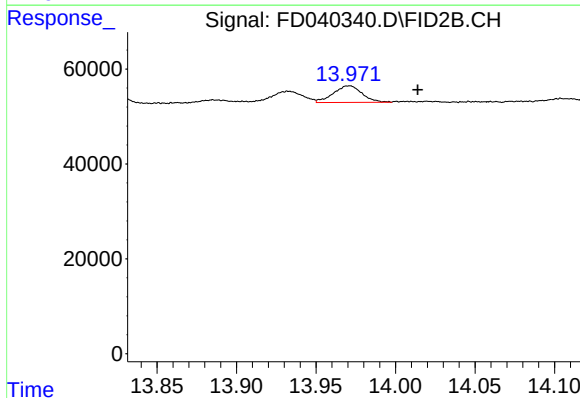


#14 n-Tetracosane (C24)

R.T.: 13.971 min
Delta R.T.: -0.043 min
Response: 43777
Conc: 0.31 ug/ml

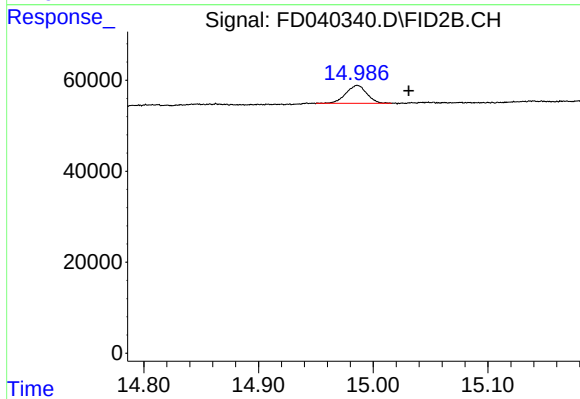

#15 n-Hexacosane (C26)


R.T.: 14.986 min
Delta R.T.: -0.045 min
Response: 49451
Conc: 0.36 ug/ml

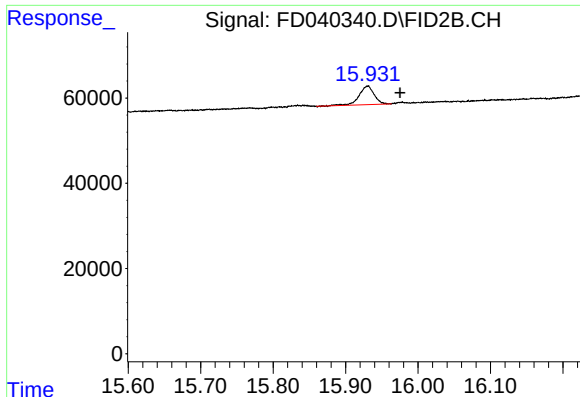

#16 n-Octacosane (C28)


R.T.: 15.931 min
Delta R.T.: -0.044 min
Response: 63156
Conc: 0.46 ug/ml

Instrument :
FID_D
ClientSampleId :

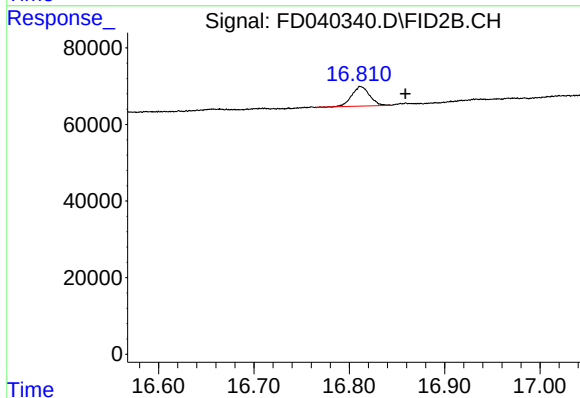


#17 n-Tricontane (C30)

R.T.: 16.812 min
Delta R.T.: -0.047 min
Response: 66508
Conc: 0.50 ug/ml

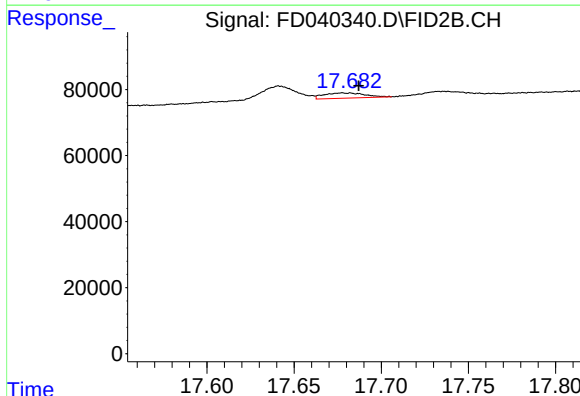


#18 n-Dotriacontane (C32)

R.T.: 17.678 min
Delta R.T.: -0.009 min
Response: 26080
Conc: 0.20 ug/ml

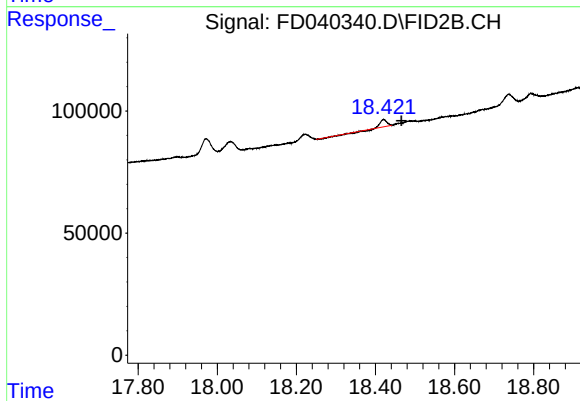

#19 n-Tetratriacontane (C34)


R.T.: 18.421 min
Delta R.T.: -0.045 min
Response: 23551
Conc: 0.19 ug/ml

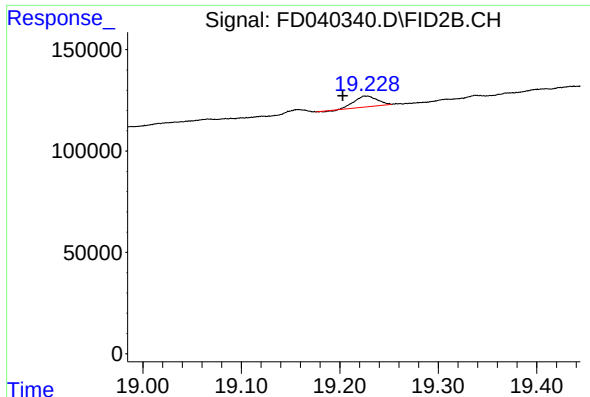

#20 n-Hexatriacontane (C36)


R.T.: 19.226 min
Delta R.T.: 0.023 min
Response: 85092
Conc: 0.80 ug/ml

Instrument :
FID_D
ClientSampleId :

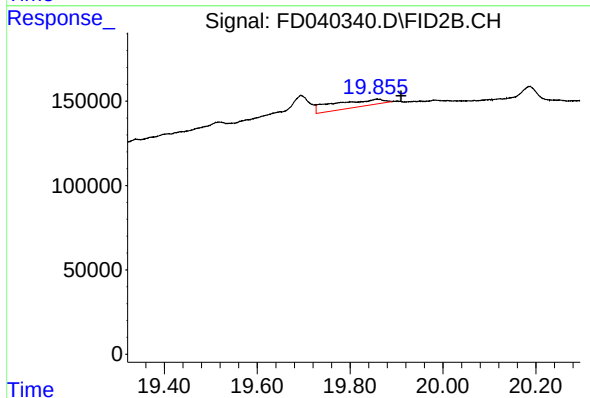

#21 n-Octatriacontane (C38)

R.T.: 19.858 min
Delta R.T.: -0.051 min
Response: 315023
Conc: 3.41 ug/ml

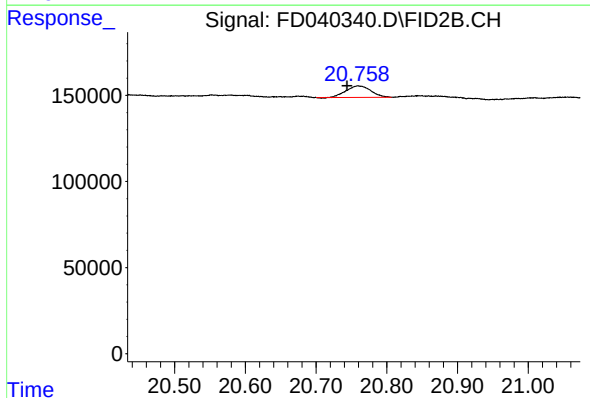

#22 n-Tetracontane (C40)

R.T.: 20.759 min
Delta R.T.: 0.015 min
Response: 164907
Conc: 2.12 ug/ml