

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD123021AL\
 Data File : FD040334.D
 Signal(s) : FID2B.CH
 Acq On : 31 Dec 2021 10:21
 Operator : AJ\MA
 Sample : M5253-01
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 SA-1-122921

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/03/2022
 Supervised By :Ankita Jodhani 01/03/2022

Integration File: autoint1.e
 Quant Time: Dec 31 21:34:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 122821.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 29 02:26:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.693	5658807	36.324 ug/mlm
Spiked Amount	50.000	Recovery	= 72.65%
12) S 1-chlorooctadecane (S...	12.126	11907383	98.736 ug/mlm
Spiked Amount	50.000	Recovery	= 197.47%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD123021AL\
Data File : FD040334.D
Signal(s) : FID2B.CH
Acq On : 31 Dec 2021 10:21
Operator : AJ\MA
Sample : M5253-01
Misc :
ALS Vial : 76 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
SA-1-122921


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/03/2022
Supervised By :Ankita Jodhani 01/03/2022

Integration File: autoint1.e
Quant Time: Dec 31 21:34:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 122821.M
Quant Title : GC Extractables
QLast Update : Wed Dec 29 02:26:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

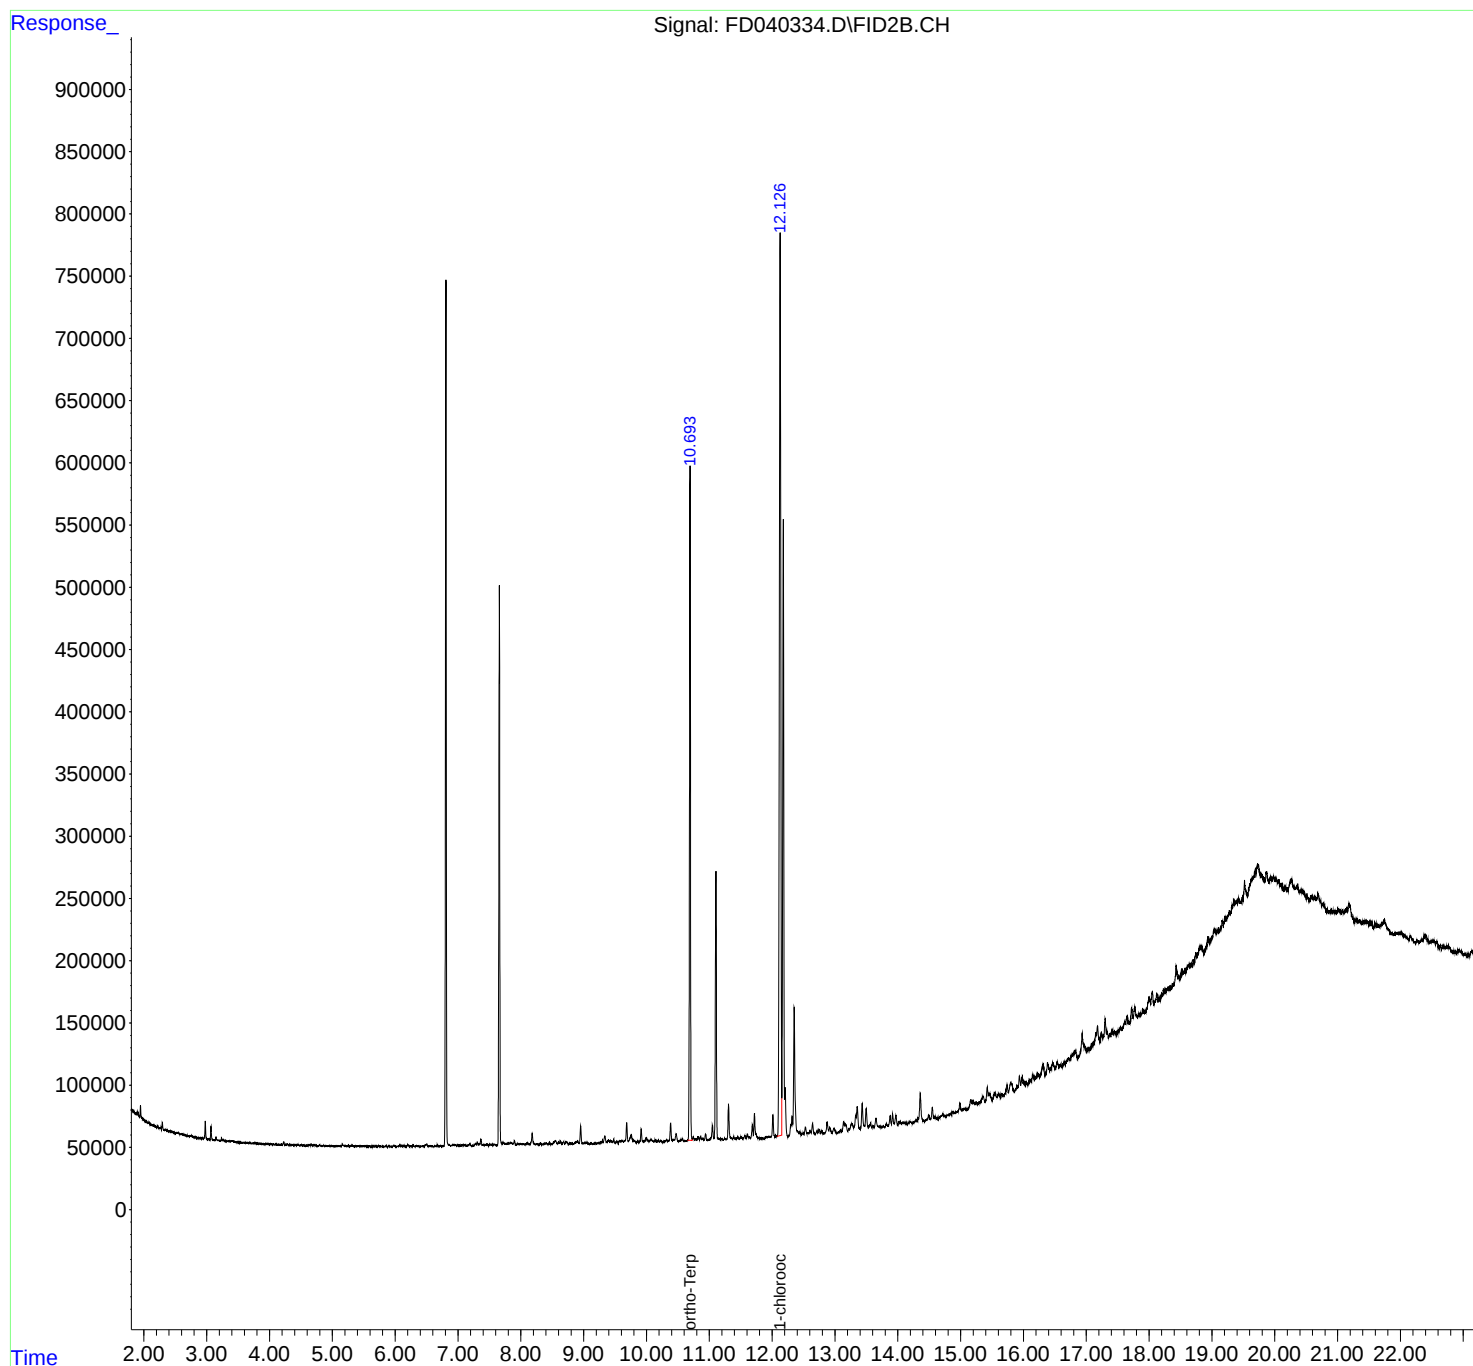

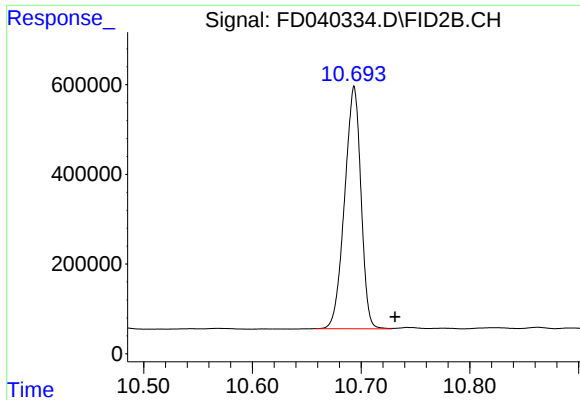


#9 ortho-Terphenyl (SURR)

R.T.: 10.693 min
Delta R.T.: -0.038 min
Response: 5658807
Conc: 36.32 ug/ml

Instrument :
FID_D
ClientSampleId :
SA-1-122921

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/03/2022
Supervised By :Ankita Jodhani 01/03/2022

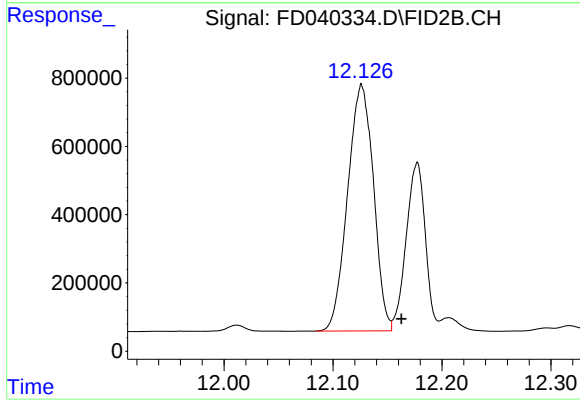

#12 1-chlorooctadecane (SURR)

R.T.: 12.126 min
Delta R.T.: -0.037 min
Response: 11907383
Conc: 98.74 ug/ml m