

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD123021AR\
Data File : FD040296.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2021 12:25
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 30 16:53:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 123021.M
Quant Title : GC Extractables
QLast Update : Thu Dec 30 16:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T Benzo[a]anthracene (C...	13.823f	243993	2.088 ug/ml
20) T Dibenz[a,h]anthracene...	17.247	54012	0.475 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD123021AR\
Data File : FD040296.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2021 12:25
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 30 16:53:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 123021.M
Quant Title : GC Extractables
QLast Update : Thu Dec 30 16:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

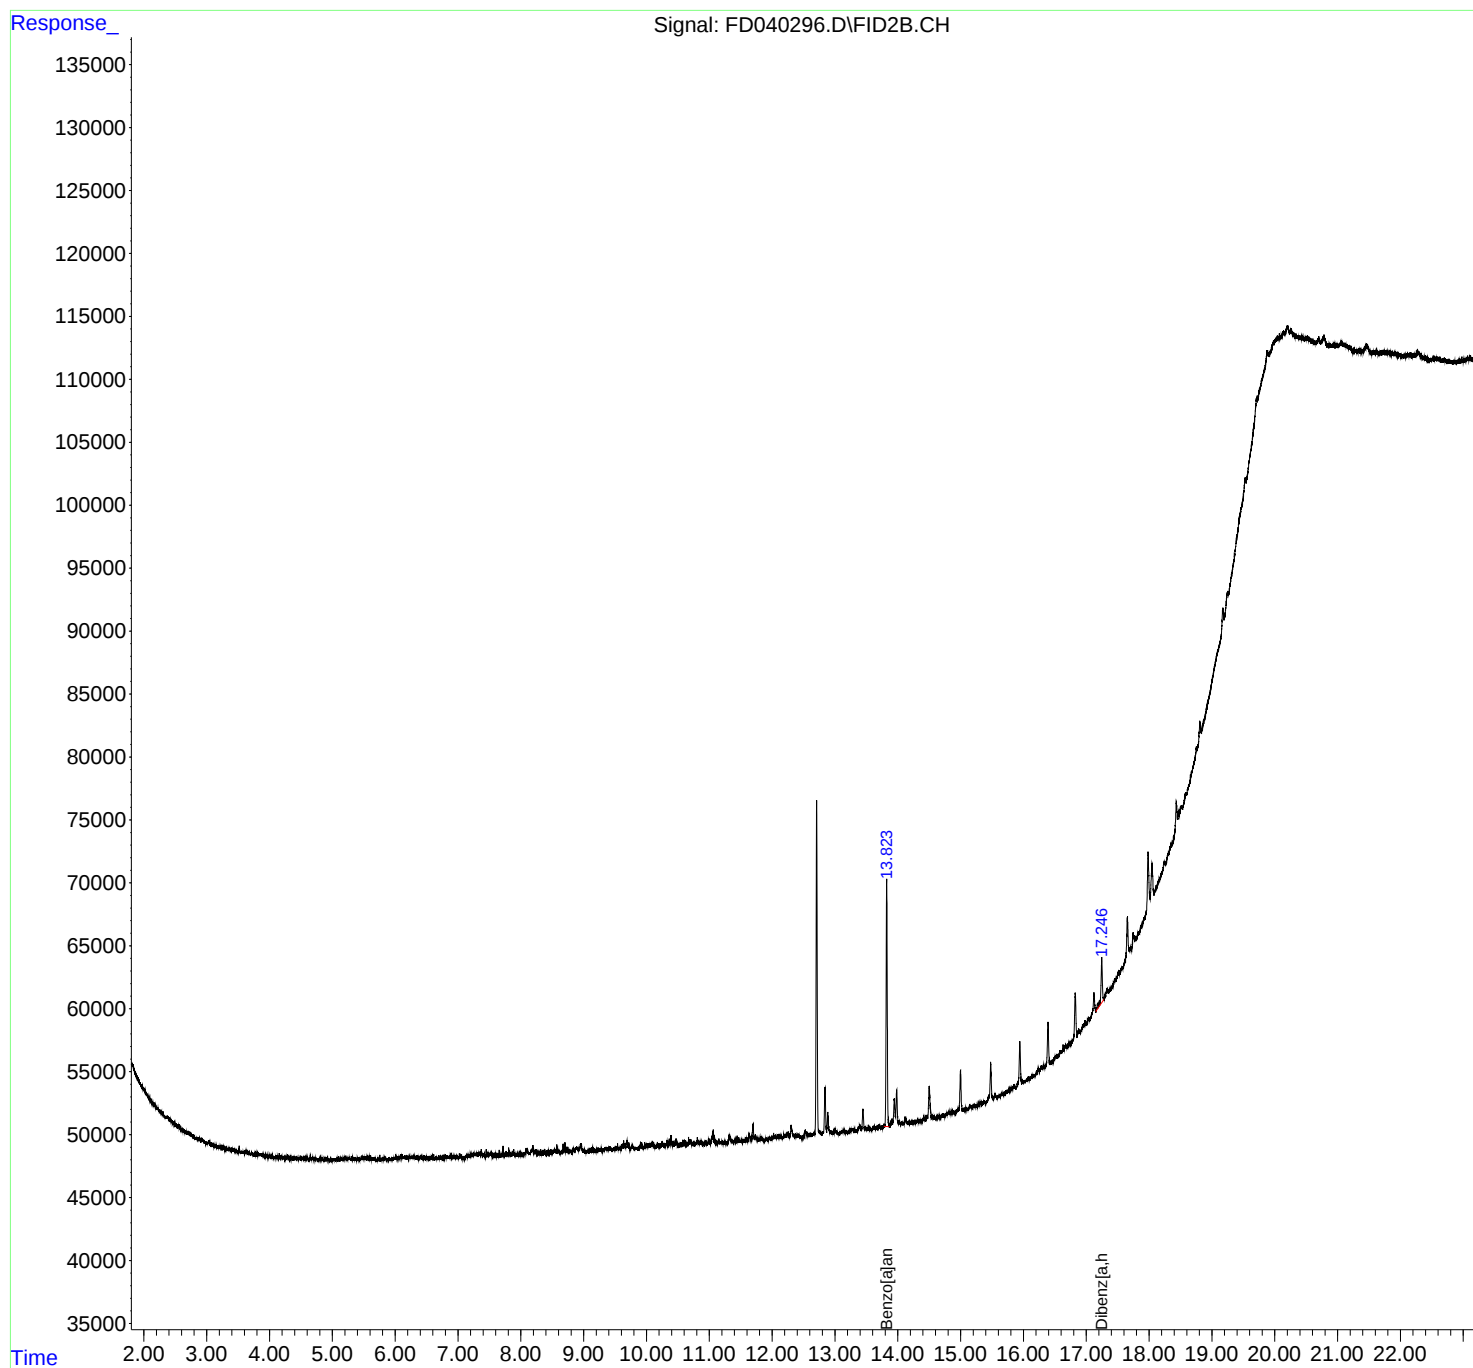


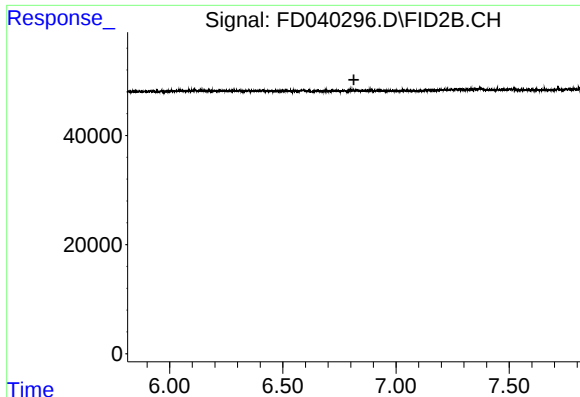

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

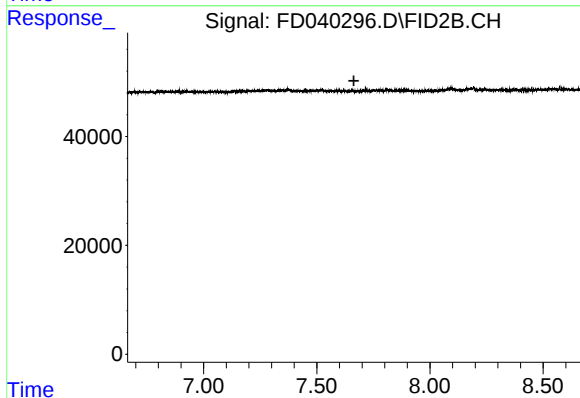


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 7.664 min
Response: 0
Conc: N.D.

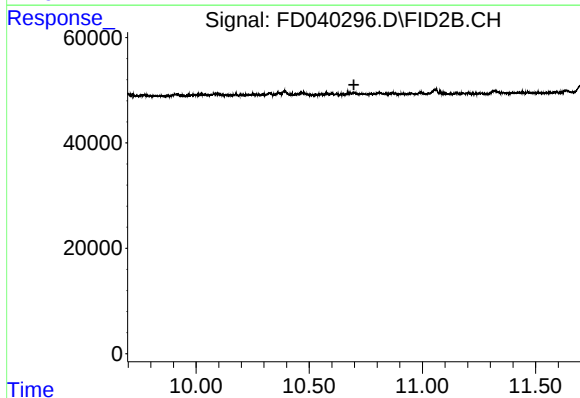


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 10.697 min
Response: 0
Conc: N.D.

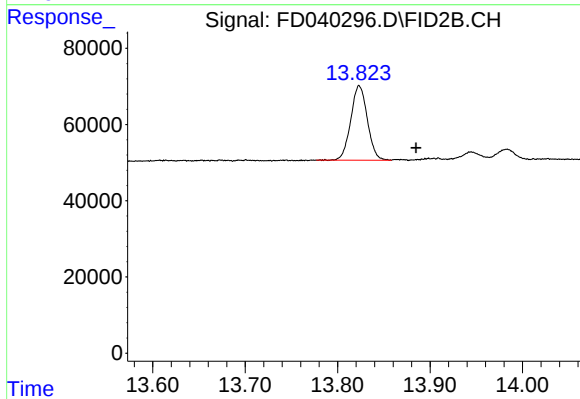

#14 Benzo[a]anthracene (C26.37)

R.T.: 13.823 min
Delta R.T.: -0.062 min
Response: 243993
Conc: 2.09 ug/ml

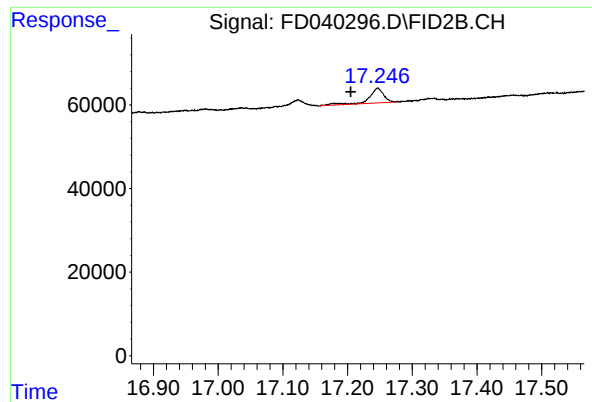

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.247 min
Delta R.T.: 0.042 min
Response: 54012
Conc: 0.48 ug/ml

Instrument :
FID_D
ClientSampleId :