

Data Path : P:\HPCHEM1\FID D\Data\FD030518AR\
Data File : FD022367.D
Signal(s) : FID2B.CH
Acq On : 06 Mar 2018 14:57
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 20:15:11 2018
Quant Method : P:\HPCHEM1\FID_D\methods\Aromatic EPH 022018.M
Quant Title : GC Extractables
QLast Update : Wed Feb 21 04:46:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	Indeno[1,2,3-cd]pyren...	17.799	9447	0.099 ug/ml
20) T	Dibenz[a,h]anthracene...	17.799	9447	0.083 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID D\Data\FD030518AR\
Data File : FD022367.D
Signal(s) : FID2B.CH
Acq On : 06 Mar 2018 14:57
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 20:15:11 2018
Quant Method : P:\HPCHEM1\FID_D\methods\Aromatic EPH 022018.M
Quant Title : GC Extractables
QLast Update : Wed Feb 21 04:46:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

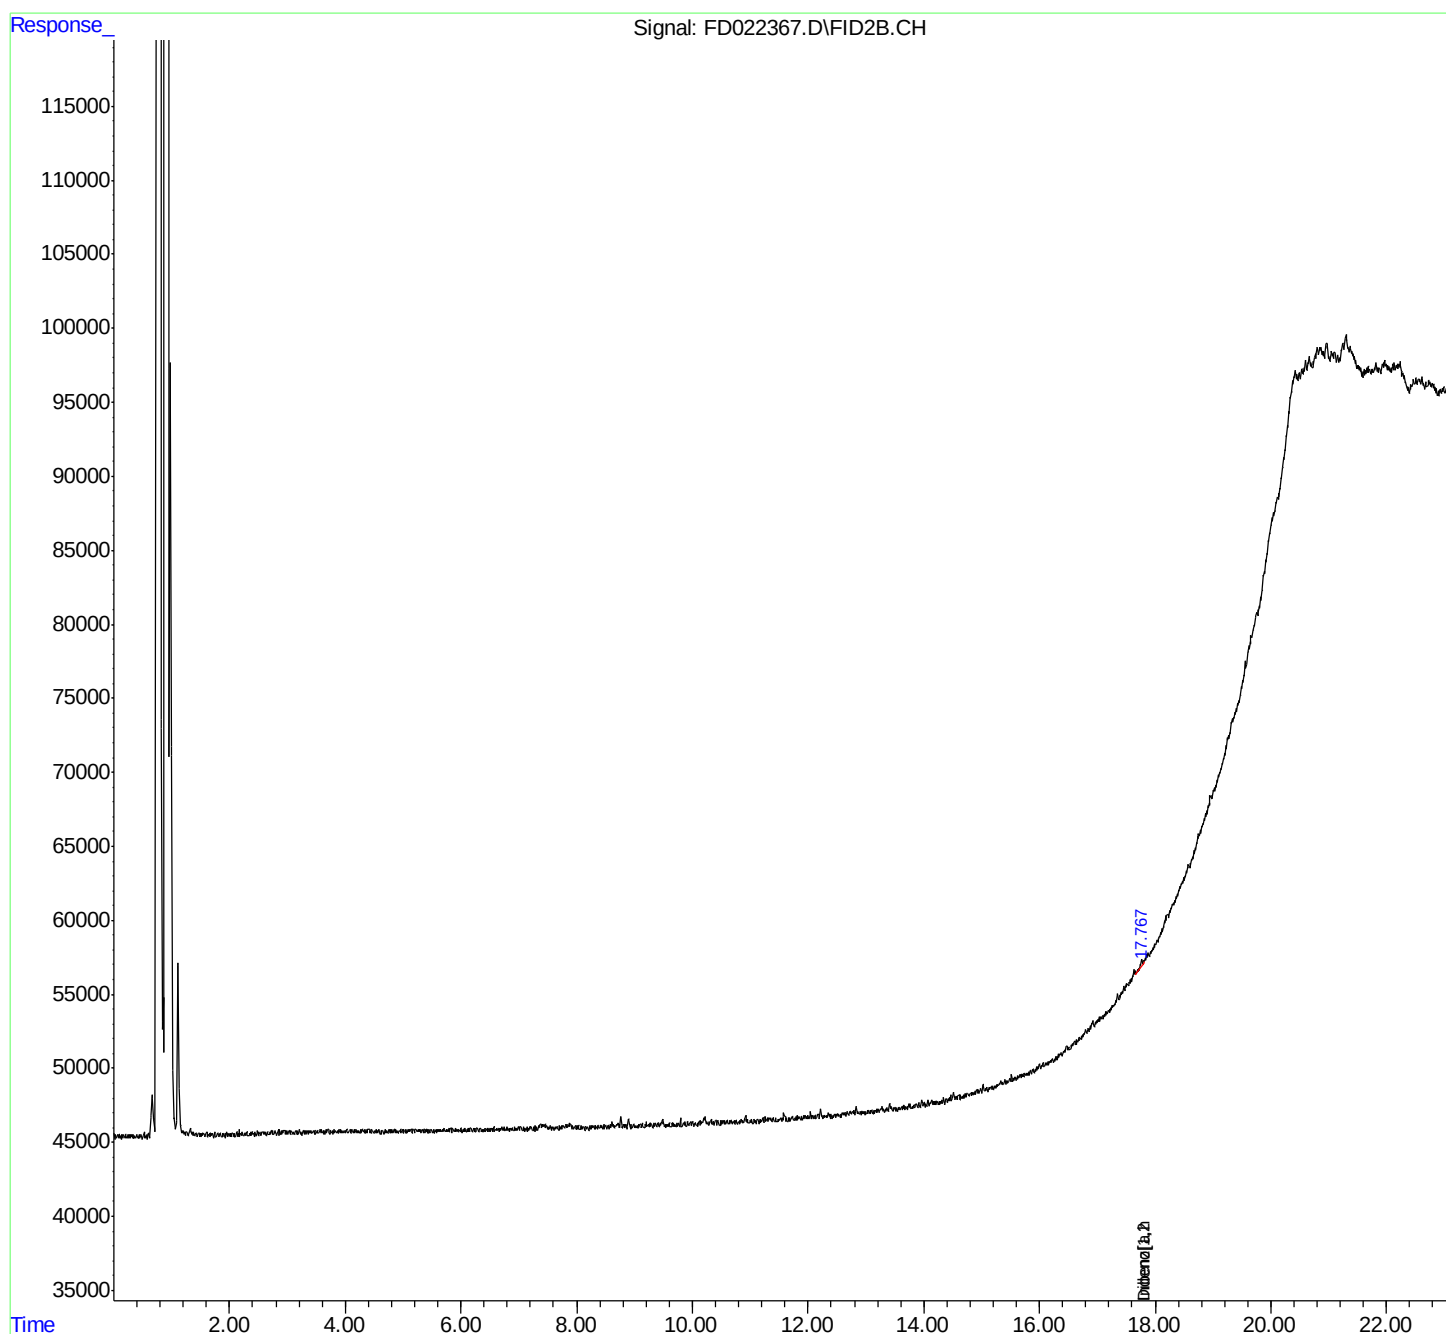


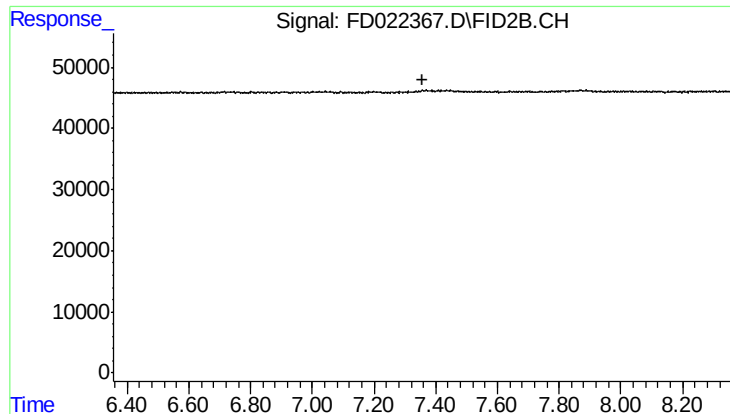

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T.: 7.355 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

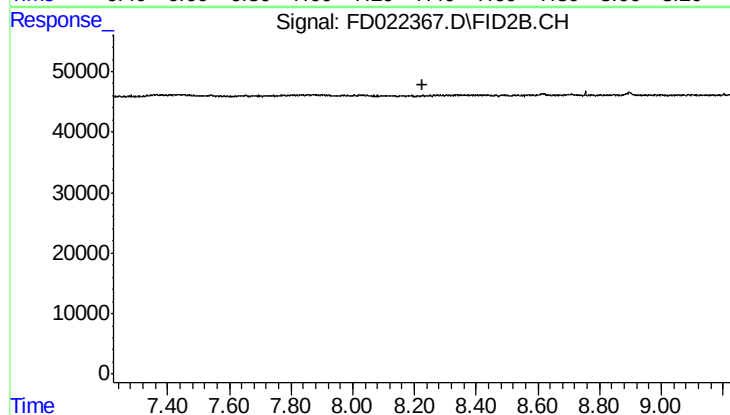


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 8.225 min
Response: 0
Conc: N.D.

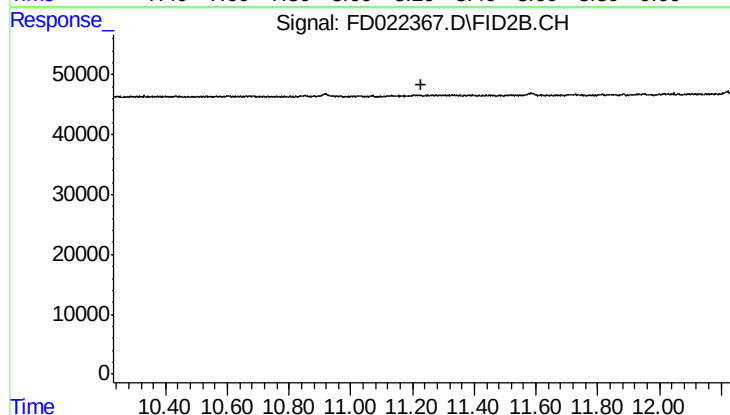


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.230 min
Response: 0
Conc: N.D.

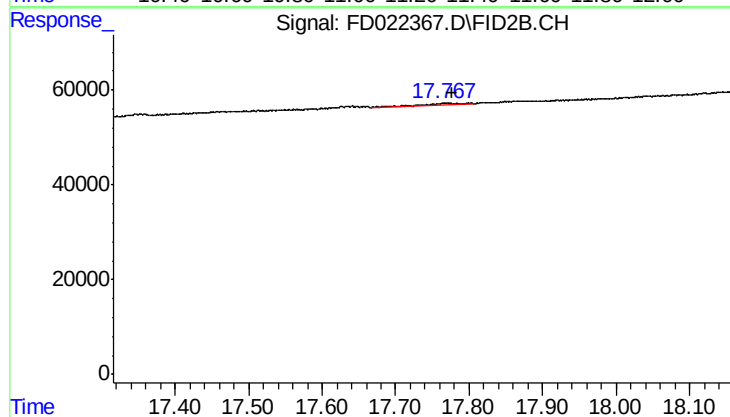

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.799 min
Delta R.T.: 0.022 min
Response: 9447
Conc: 0.10 ug/ml

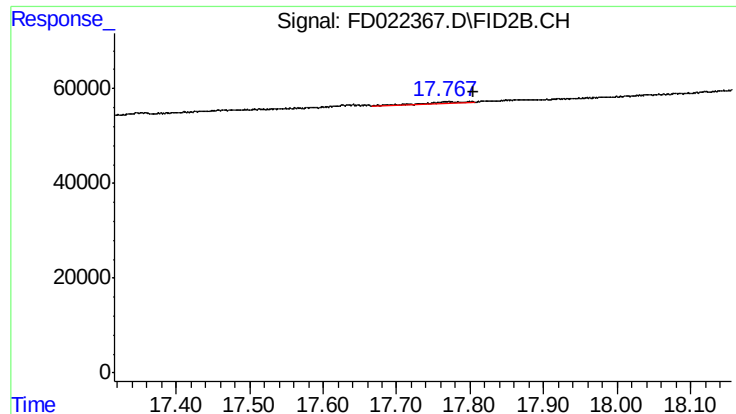

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.799 min
Delta R.T.: -0.006 min
Response: 9447
Conc: 0.08 ug/ml

Instrument :
FID_D
ClientSampleId :