

Data Path : P:\HPCHEM1\FID D\Data\FD040618AL\
Data File : FD022871.D
Signal(s) : FID2B.CH
Acq On : 07 Apr 2018 4:37
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 07 06:40:36 2018
Quant Method : P:\HPCHEM1\FID_D\methods\Alaphatic EPH 031618.M
Quant Title : GC Extractables
QLast Update : Mon Mar 19 11:51:27 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
20) T	n-Hexatriacontane (C36)	19.664	77246	0.905 ug/ml
21) T	n-Octatriacontane (C38)	20.360	175693	2.121 ug/ml
22) T	n-Tetracontane (C40)	21.125	304615	3.911 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID D\Data\FD040618AL\
Data File : FD022871.D
Signal(s) : FID2B.CH
Acq On : 07 Apr 2018 4:37
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 07 06:40:36 2018
Quant Method : P:\HPCHEM1\FID_D\methods\Alaphatic EPH 031618.M
Quant Title : GC Extractables
QLast Update : Mon Mar 19 11:51:27 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

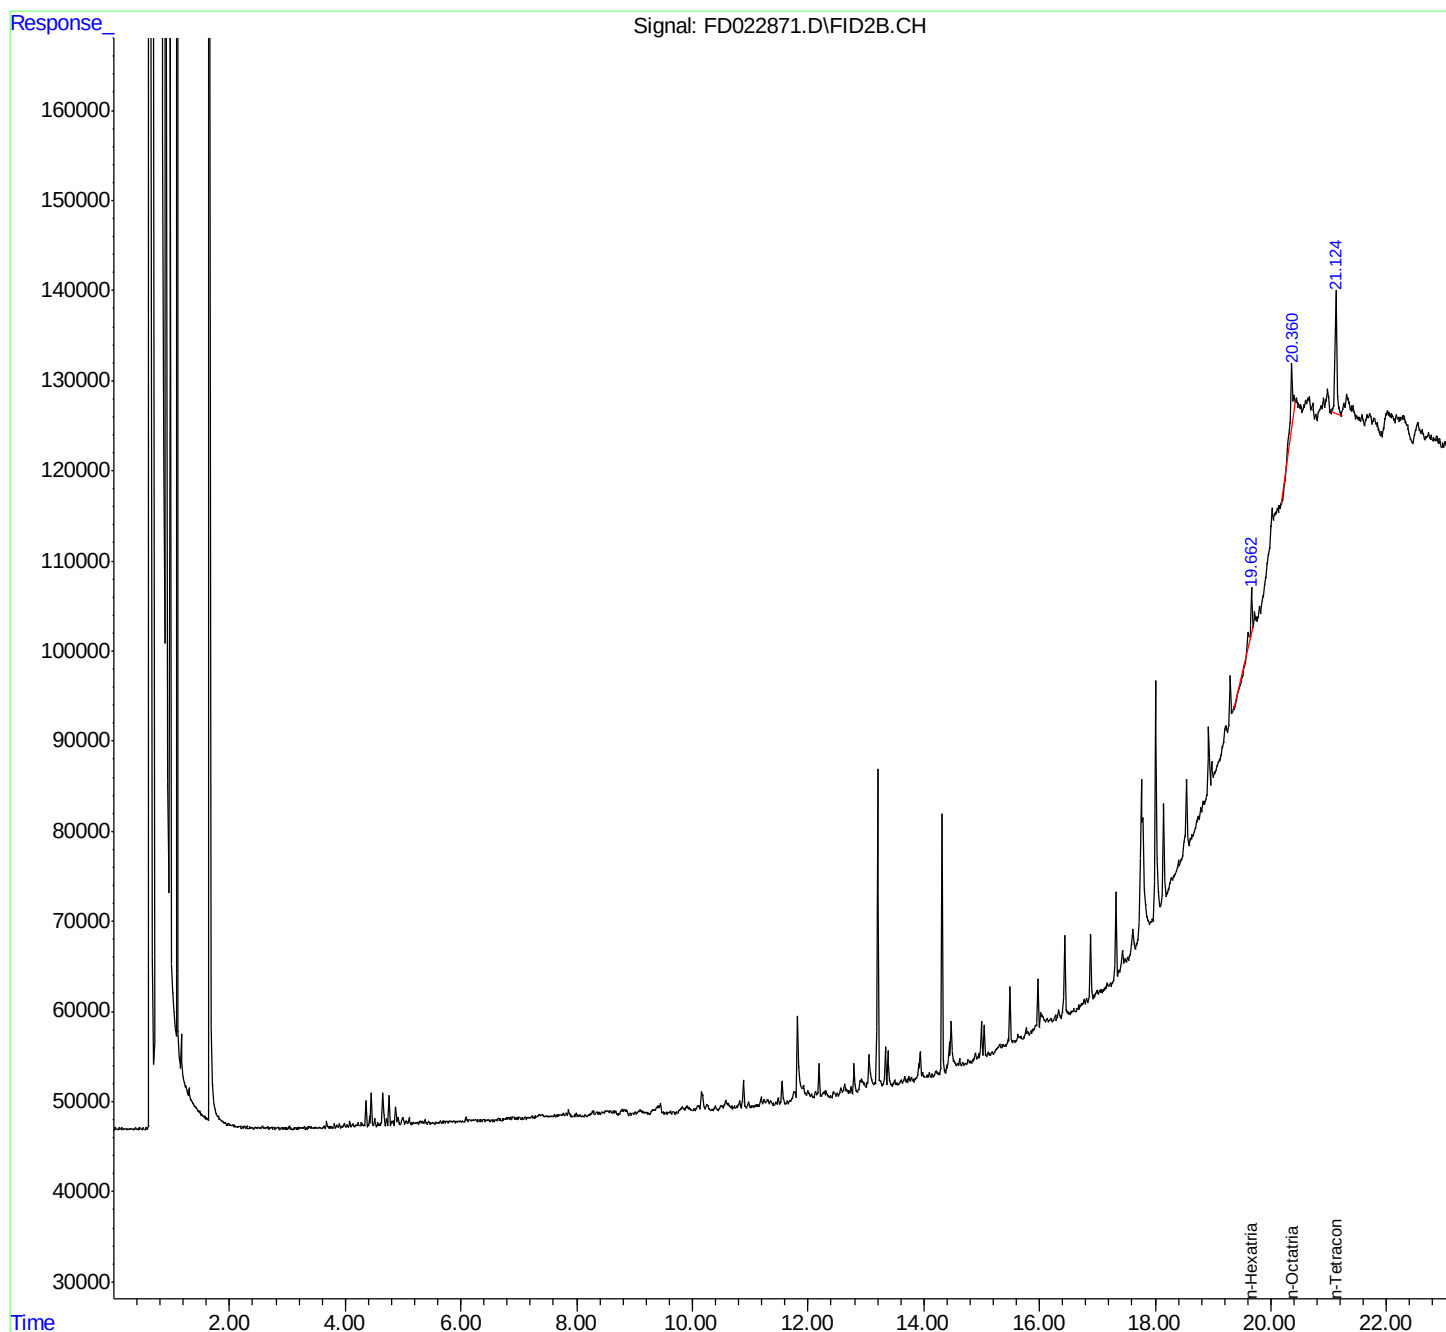

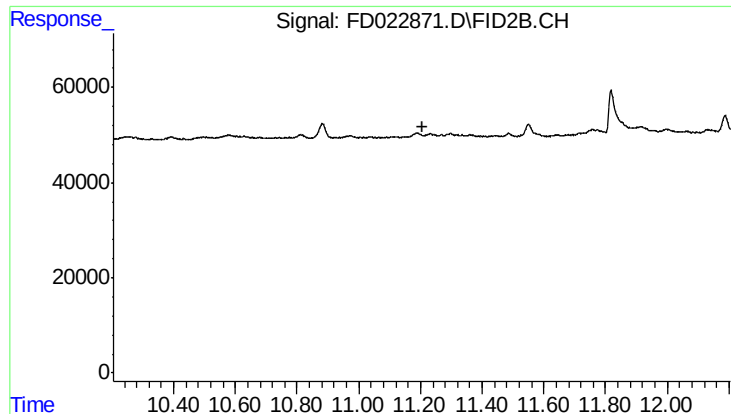


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.205 min
Response: 0
Conc: N.D.

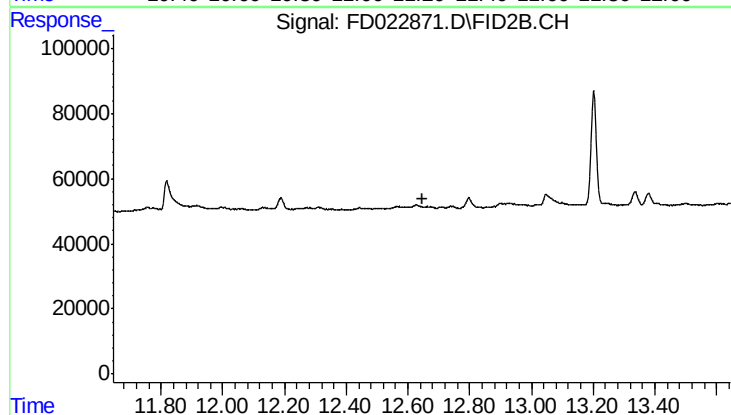


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.645 min
Response: 0
Conc: N.D.

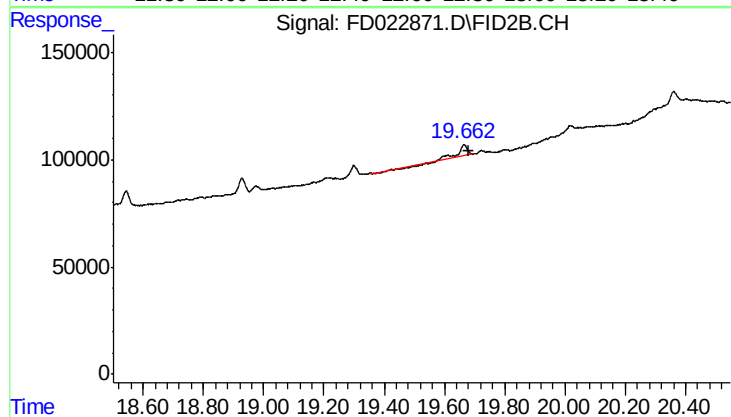


#20 n-Hexatriacontane (C36)

R.T.: 19.664 min
Delta R.T.: -0.014 min
Response: 77246
Conc: 0.90 ug/ml

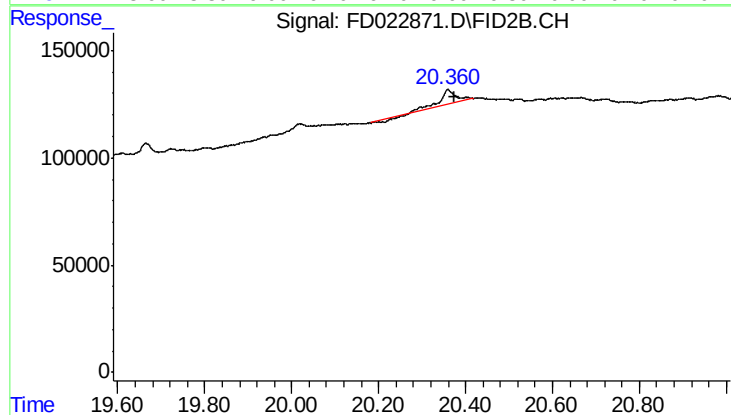

#21 n-Octatriacontane (C38)

R.T.: 20.360 min
Delta R.T.: -0.015 min
Response: 175693
Conc: 2.12 ug/ml

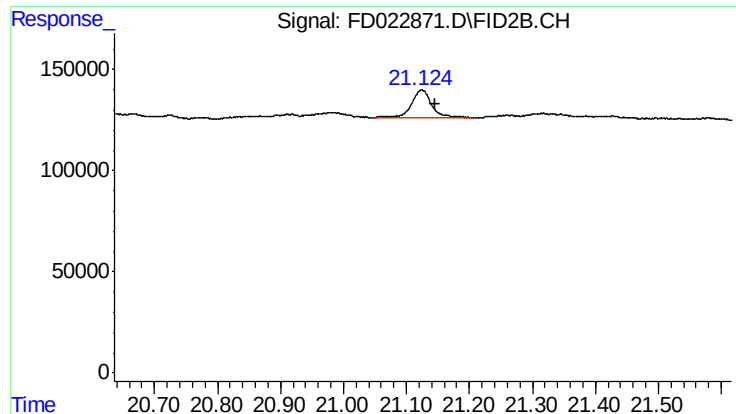

#22 n-Tetracontane (C40)

R.T.: 21.125 min
Delta R.T.: -0.022 min
Response: 304615
Conc: 3.91 ug/ml