

Data Path : P:\HPCHEM1\FID E\Data\FE011218\
Data File : FE025519.D
Signal(s) : FID1B.CH
Acq On : 12 Jan 2018 19:04
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 13 00:47:42 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.862	3557913	19.561 ug/ml
Target Compounds				
6)	N-OCTADECANE	11.448	79643	0.360 ug/ml
13)	N-TRIACONTANE	17.921	49335	0.312 ug/ml
14)	N-DOTRIACONTANE	18.753	93469	0.576 ug/ml
15)	N-TETRATRIACONTANE	19.534	90846	0.585 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID E\Data\FE011218\
Data File : FE025519.D
Signal(s) : FID1B.CH
Acq On : 12 Jan 2018 19:04
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 13 00:47:42 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

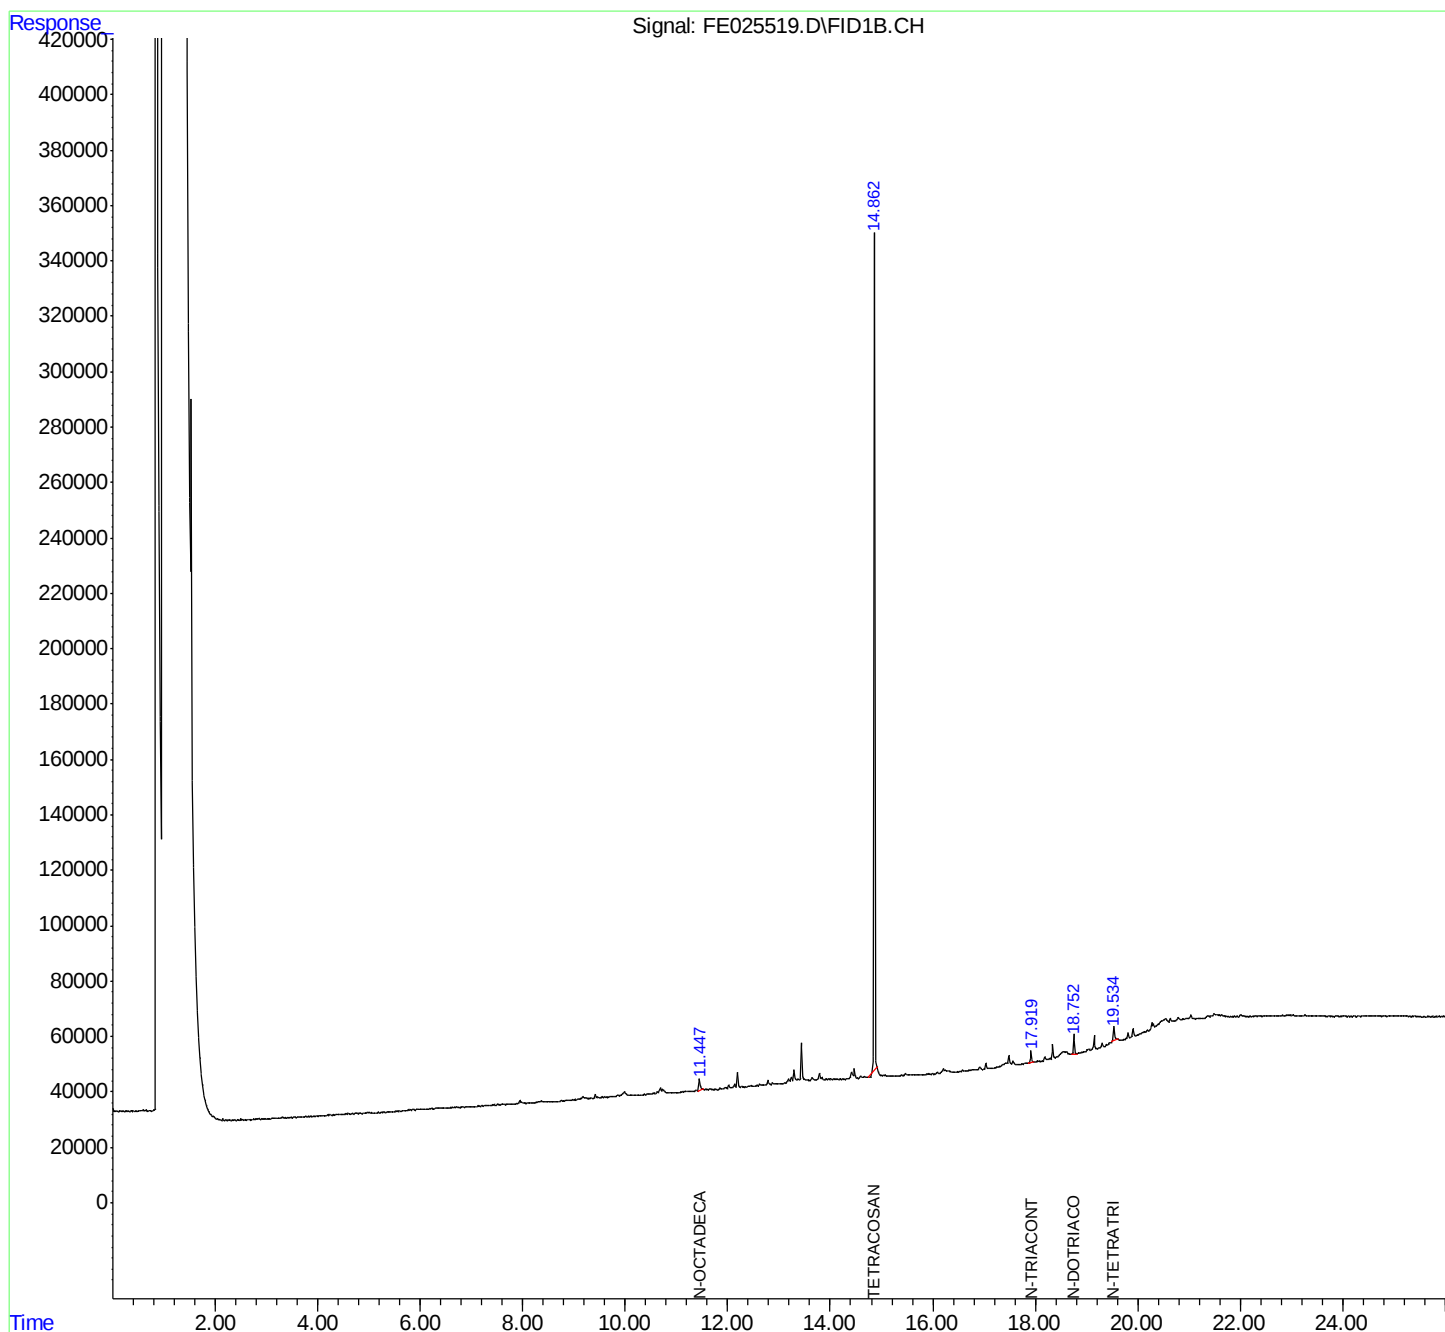

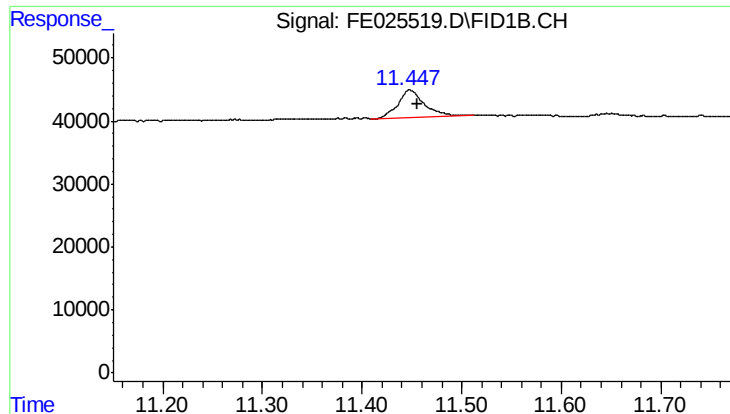


#6 N-OCTADECANE

R.T.: 11.448 min
Delta R.T.: -0.008 min
Response: 79643
Conc: 0.36 ug/ml

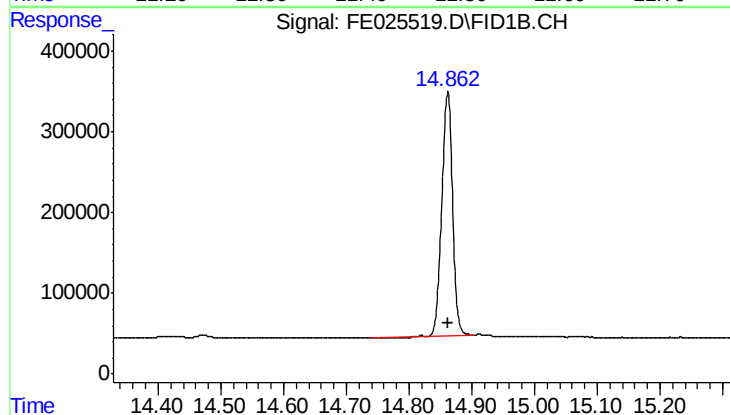


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.862 min
Delta R.T.: 0.000 min
Response: 3557913
Conc: 19.56 ug/ml

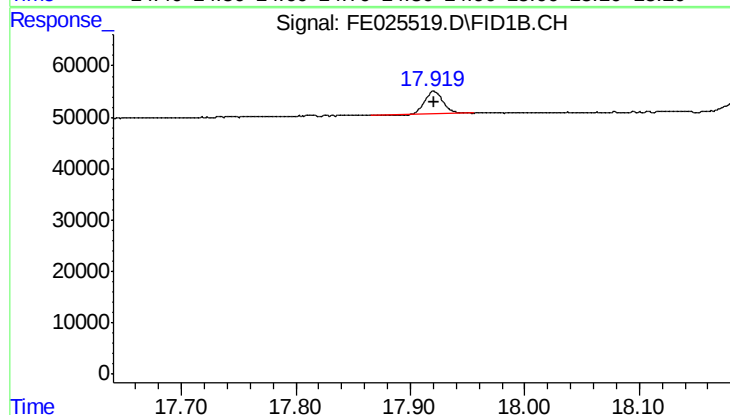


#13 N-TRIACONTANE

R.T.: 17.921 min
Delta R.T.: 0.000 min
Response: 49335
Conc: 0.31 ug/ml

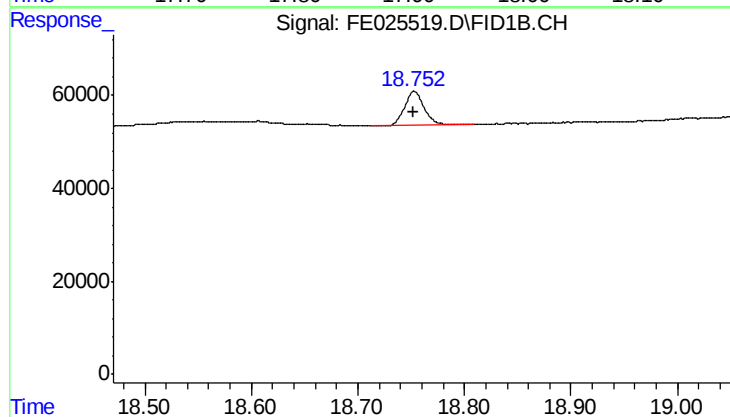

#14 N-DOTRIACONTANE

R.T.: 18.753 min
Delta R.T.: 0.000 min
Response: 93469
Conc: 0.58 ug/ml

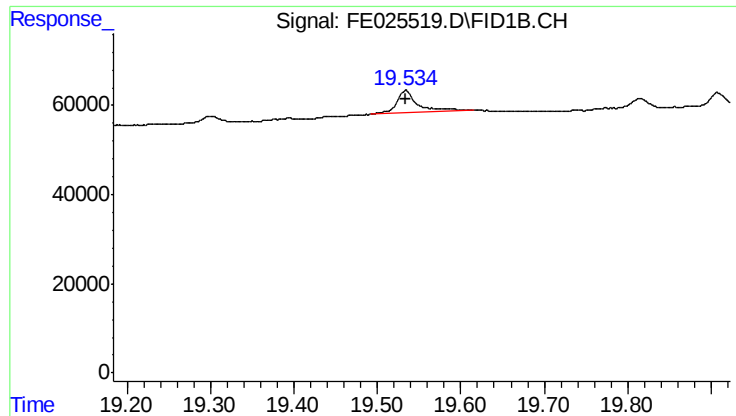

#15 N-TETRATRIACONTANE

R.T.: 19.534 min
Delta R.T.: 0.000 min
Response: 90846
Conc: 0.58 ug/ml