

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010224\  
 Data File : FE046053.D  
 Signal(s) : FID1B.ch  
 Acq On : 02 Jan 2024 09:55  
 Operator : YP\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jan 03 00:39:24 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE121423.M  
 Quant Title :  
 QLast Update : Thu Dec 14 11:27:22 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20m x 0.18mm x 0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 5) N-DODECANE               | 6.639  | 2292051  | 16.455 ug/ml |
| 11) N-OCTACOSANE            | 17.113 | 2358570  | 19.992 ug/ml |
| 12) N-DOTRIACONTANE         | 18.839 | 148952   | 1.255 ug/ml  |
| 14) N-HEXATRIACONTANE       | 20.369 | 159446   | 1.400 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010224\  
Data File : FE046053.D  
Signal(s) : FID1B.ch  
Acq On : 02 Jan 2024 09:55  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jan 03 00:39:24 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE121423.M  
Quant Title :  
QLast Update : Thu Dec 14 11:27:22 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

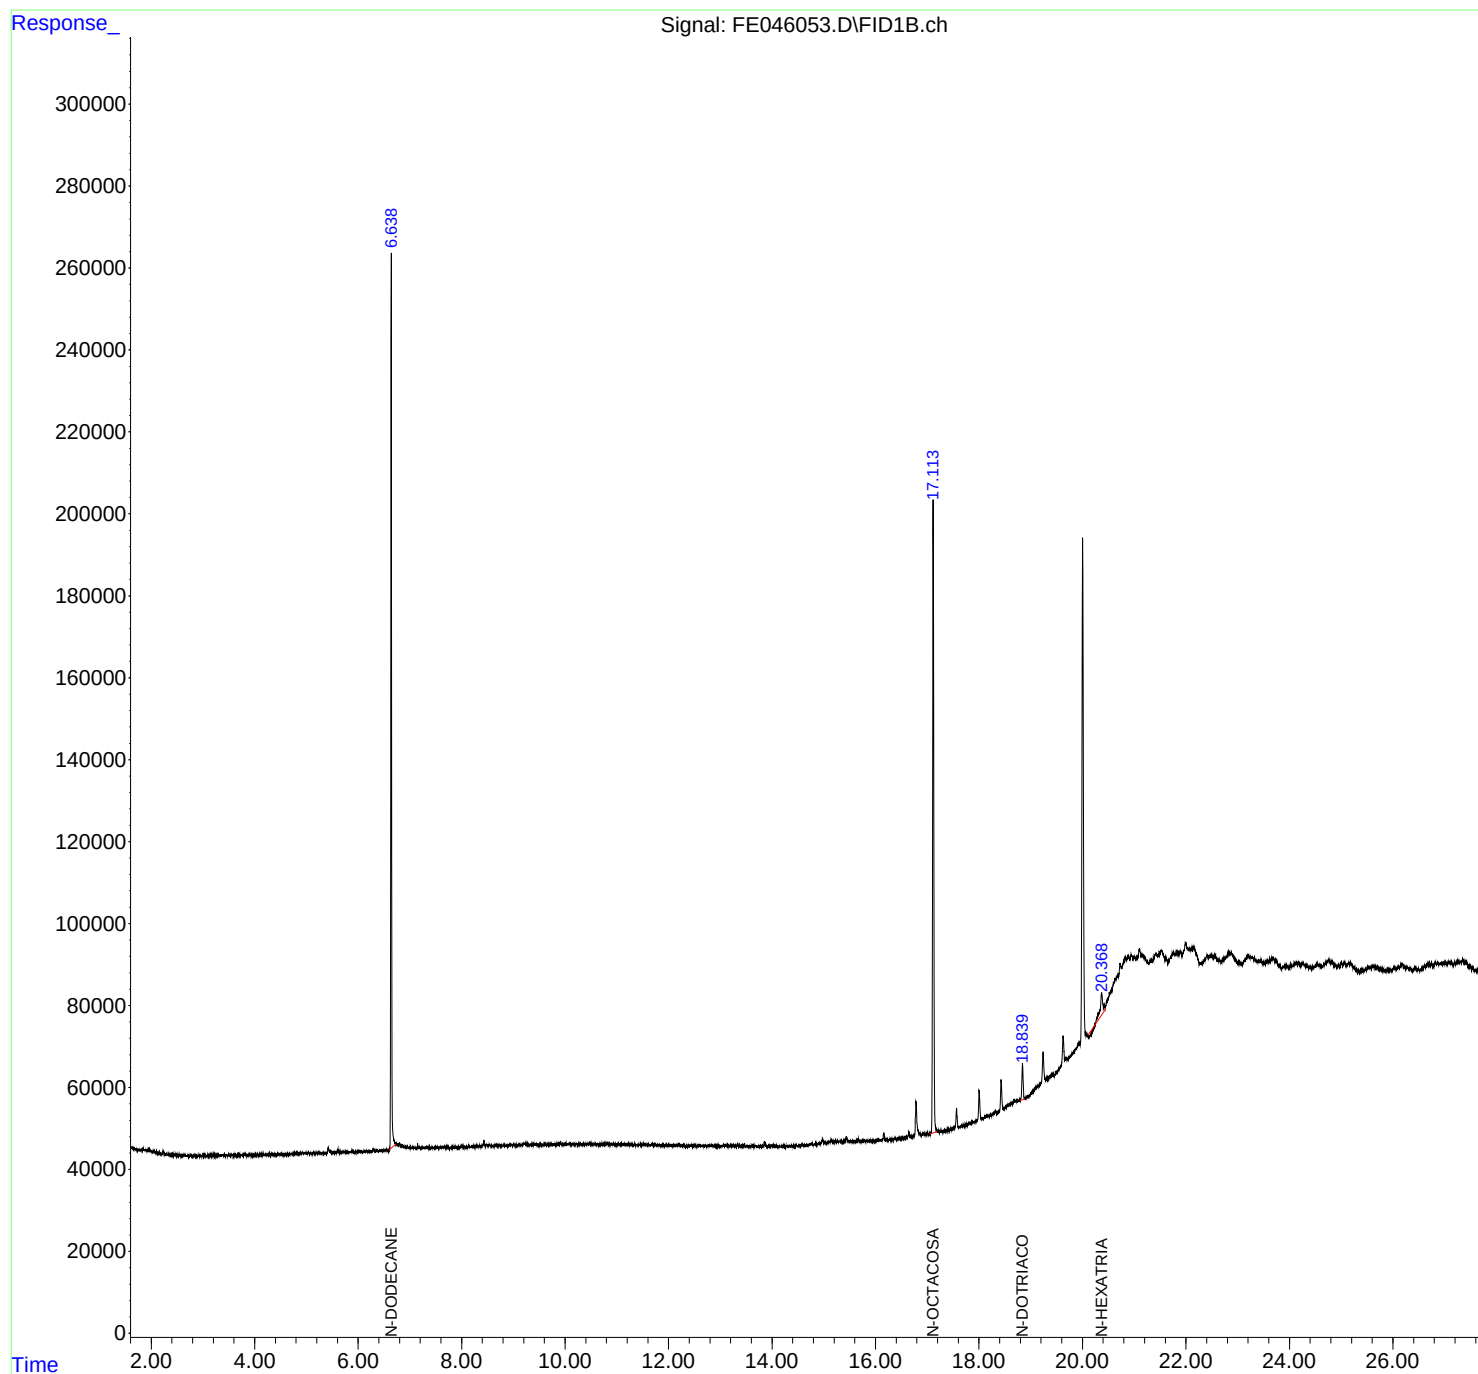

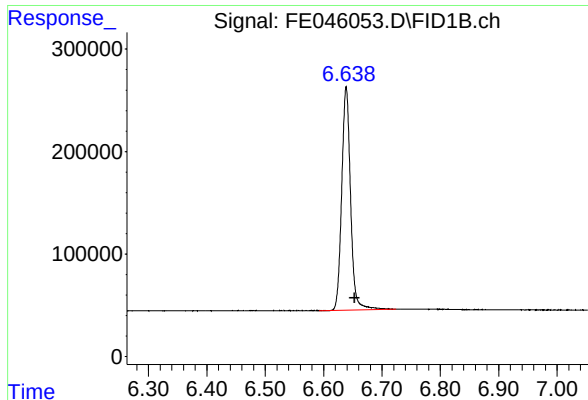


#5 N-DODECANE

R.T.: 6.639 min  
Delta R.T.: -0.014 min  
Response: 2292051  
Conc: 16.45 ug/ml

Instrument :


FID\_E

ClientSampleId :

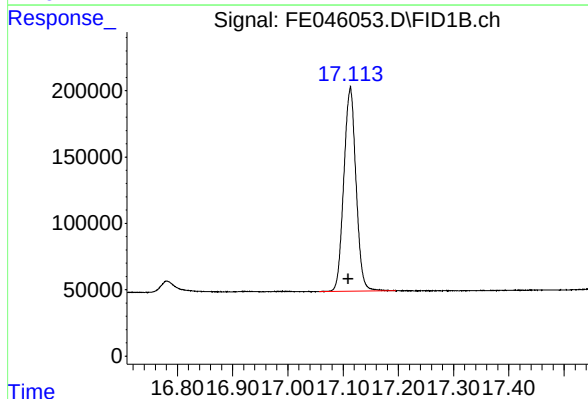


#11 N-OCTACOSANE

R.T.: 17.113 min  
Delta R.T.: 0.004 min  
Response: 2358570  
Conc: 19.99 ug/ml

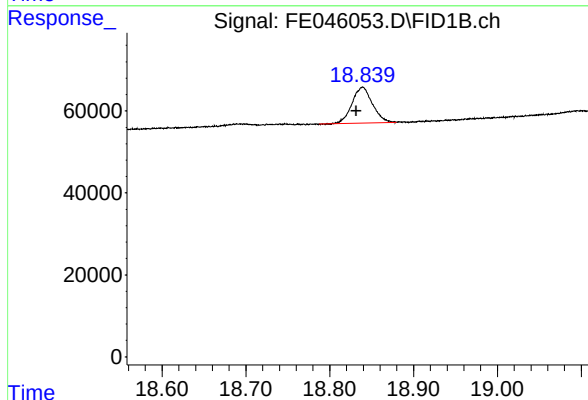


#12 N-DOTRIACONTANE

R.T.: 18.839 min  
Delta R.T.: 0.008 min  
Response: 148952  
Conc: 1.26 ug/ml

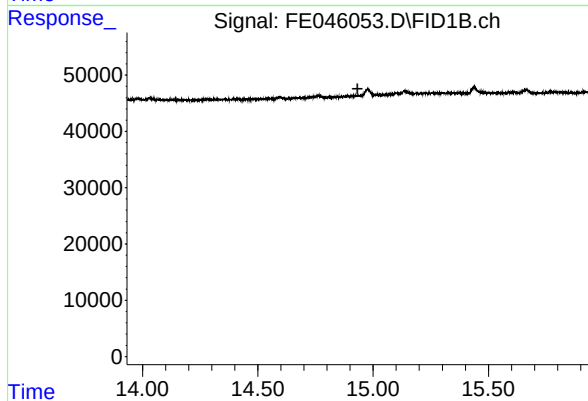

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.932 min  
Response: 0  
Conc: N.D.

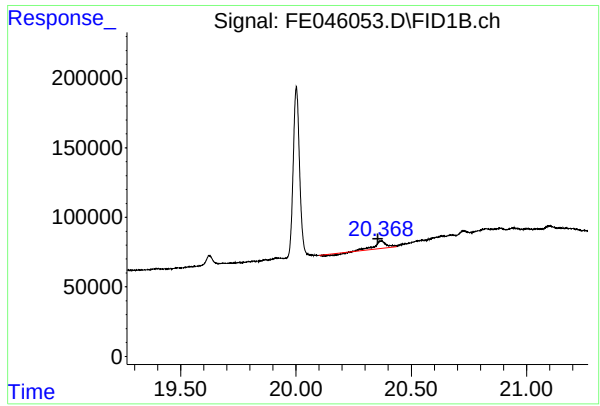

#14 N-HEXATRIACONTANE

R.T.: 20.369 min  
Delta R.T.: 0.014 min  
Response: 159446  
Conc: 1.40 ug/ml

Instrument :

FID\_E

ClientSampleId :