

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010224\
Data File : FE046055.D
Signal(s) : FID1B.ch
Acq On : 02 Jan 2024 11:39
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jan 03 00:39:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE121423.M
Quant Title :
QLast Update : Thu Dec 14 11:27:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.931	2131851	17.073 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010224\
Data File : FE046055.D
Signal(s) : FID1B.ch
Acq On : 02 Jan 2024 11:39
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jan 03 00:39:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE121423.M
Quant Title :
QLast Update : Thu Dec 14 11:27:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

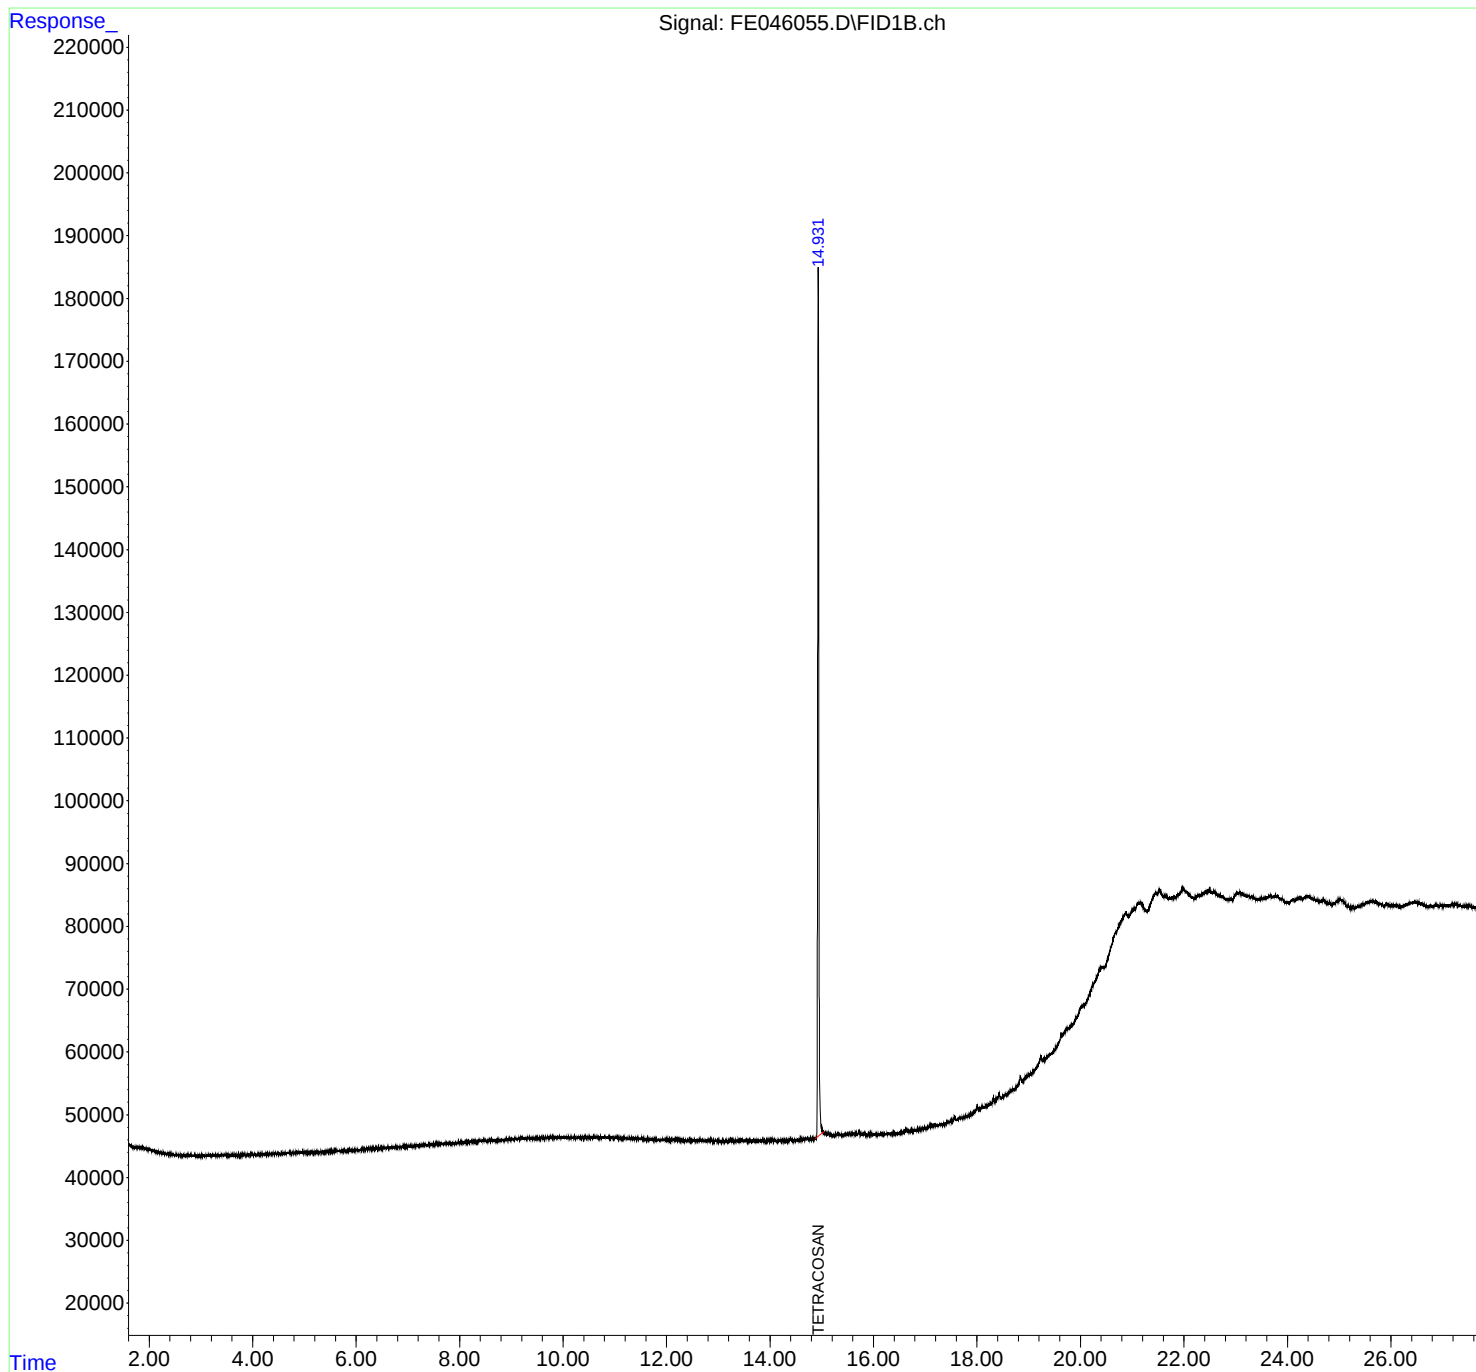

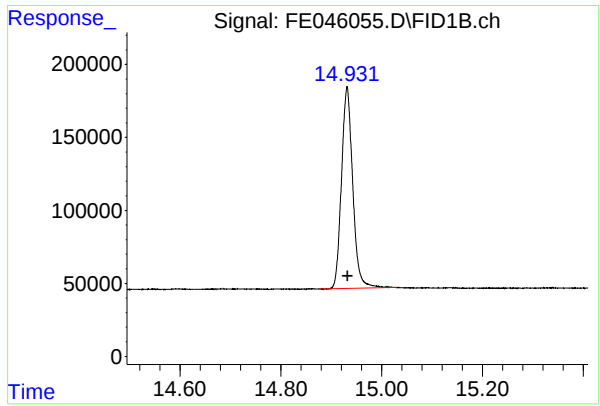

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.931 min
Delta R.T.: 0.000 min
Response: 2131851
Conc: 17.07 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK