

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010323AL\
 Data File : FE039602.D
 Signal(s) : FID1B.ch
 Acq On : 03 Jan 2023 09:03
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 03 17:27:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 17 15:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.925	60179	0.465 ug/ml
19) T n-Tetratriacontane (C34)	19.730	40137	0.318 ug/ml
20) T n-Hexatriacontane (C36)	20.453	36285	0.300 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010323AL\
Data File : FE039602.D
Signal(s) : FID1B.ch
Acq On : 03 Jan 2023 09:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 03 17:27:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 121722.M
Quant Title : GC Extractables
QLast Update : Sat Dec 17 15:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

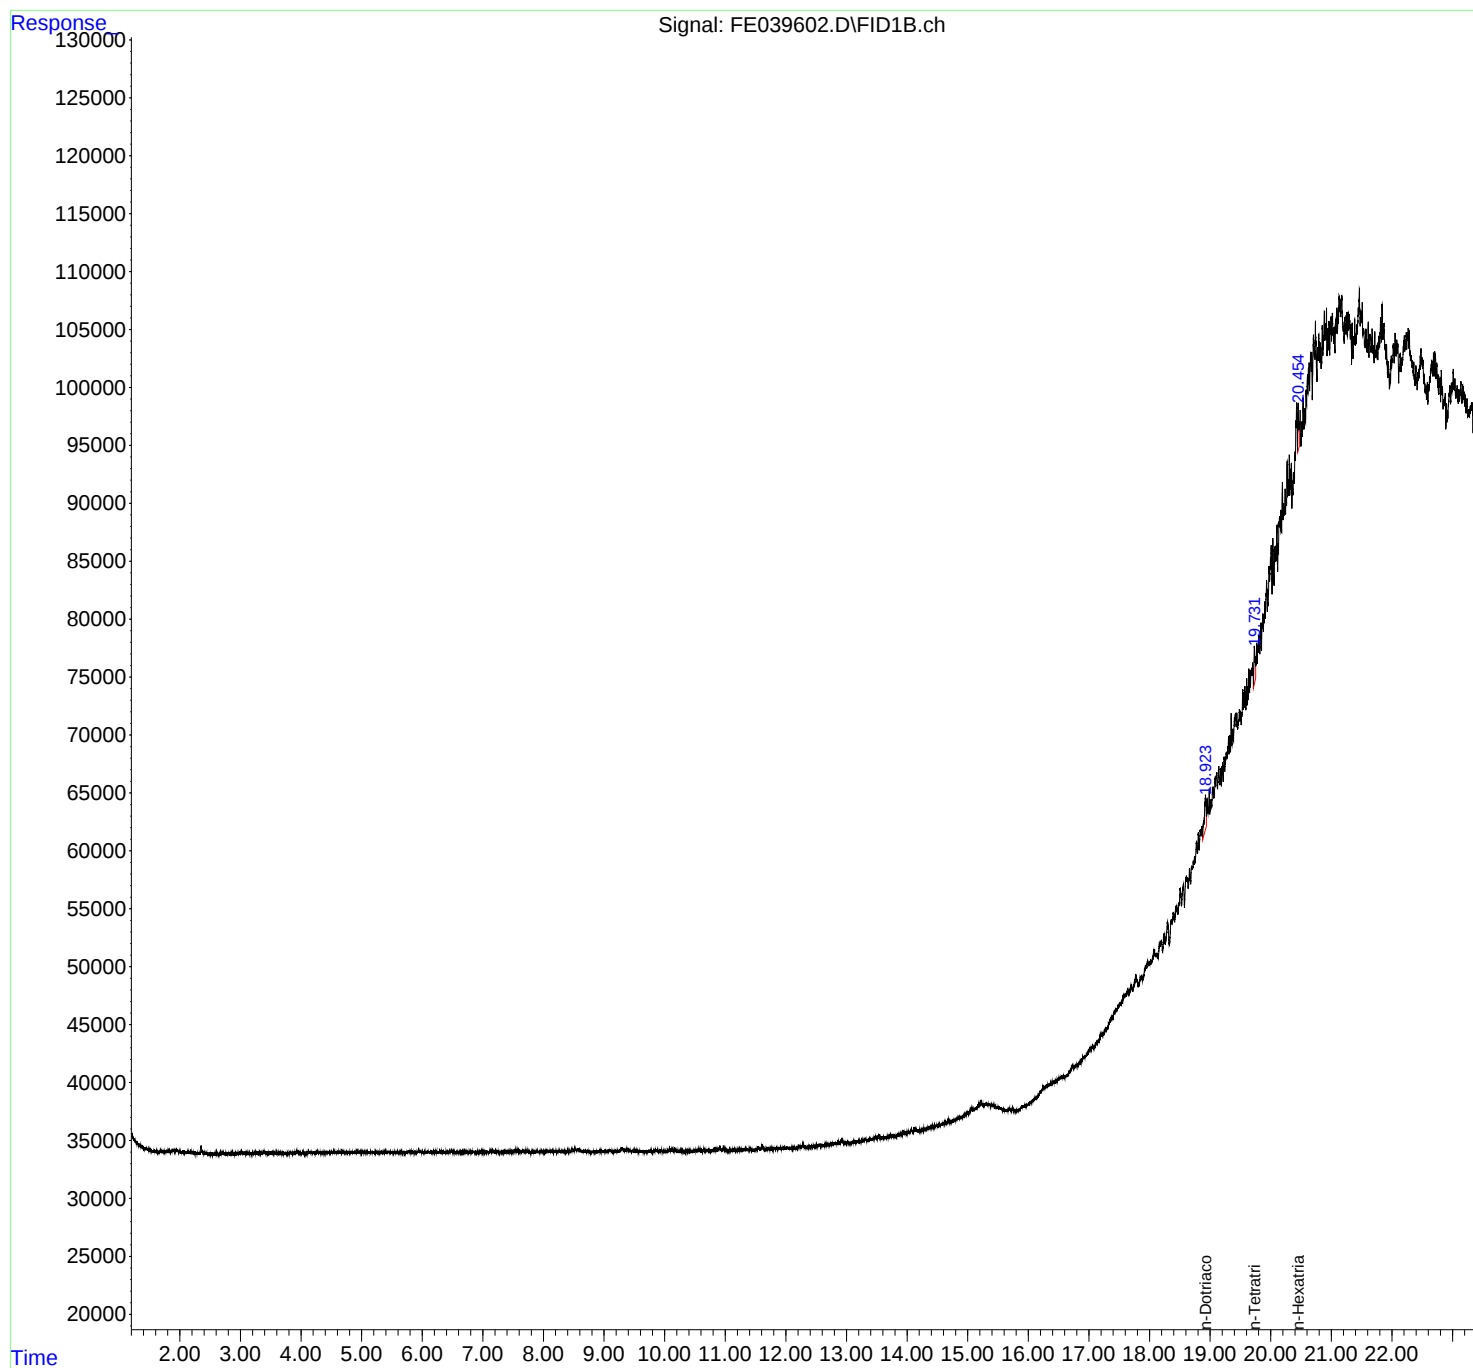


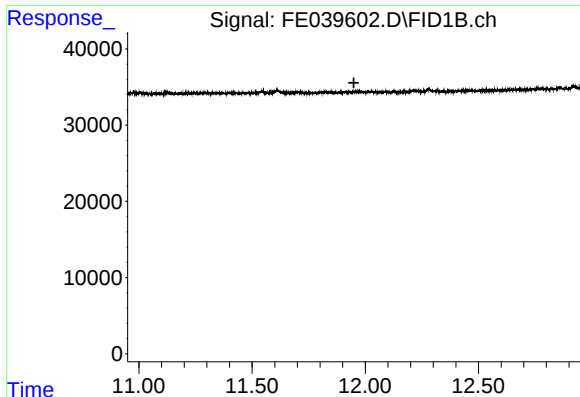

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.950 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

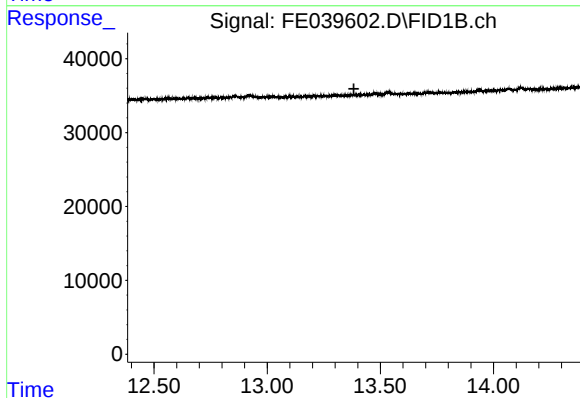


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.383 min
Response: 0
Conc: N.D.

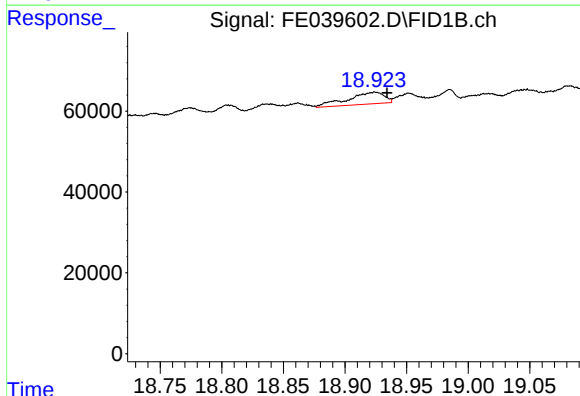


#18 n-Dotriacontane (C32)

R.T.: 18.925 min
Delta R.T.: -0.009 min
Response: 60179
Conc: 0.46 ug/ml

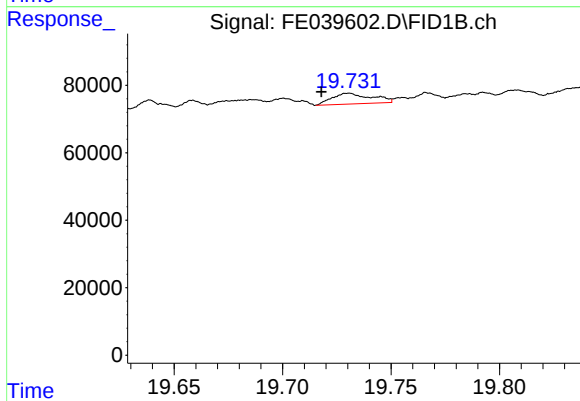

#19 n-Tetratriacontane (C34)

R.T.: 19.730 min
Delta R.T.: 0.012 min
Response: 40137
Conc: 0.32 ug/ml

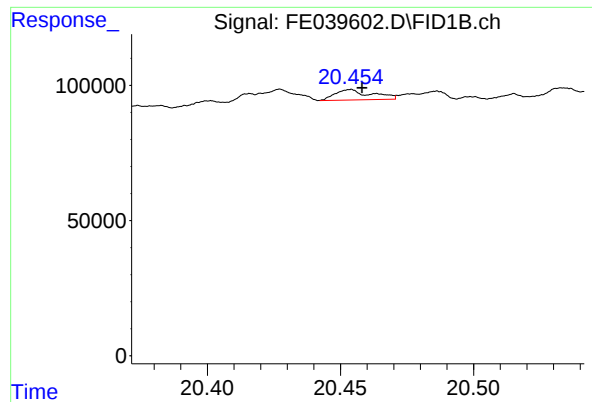

#20 n-Hexatriacontane (C36)

R.T.: 20.453 min
Delta R.T.: -0.005 min
Response: 36285
Conc: 0.30 ug/ml

Instrument :

FID_E

ClientSampleId :