

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010623AL\  
 Data File : FE039675.D  
 Signal(s) : FID1B.ch  
 Acq On : 06 Jan 2023 16:50  
 Operator : YP\AJ  
 Sample : 01043-01D  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 TP-203

Integration File: autoint1.e  
 Quant Time: Jan 09 02:39:18 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121722.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 17 15:09:52 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.921 | 3959243    | 26.531 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 53.06%       |
| 12) S 1-chlorooctadecane (S... | 13.358 | 3136783    | 27.253 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 54.51%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010623AL\  
Data File : FE039675.D  
Signal(s) : FID1B.ch  
Acq On : 06 Jan 2023 16:50  
Operator : YP\AJ  
Sample : 01043-01D  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
TP-203

Integration File: autoint1.e  
Quant Time: Jan 09 02:39:18 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 121722.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 17 15:09:52 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

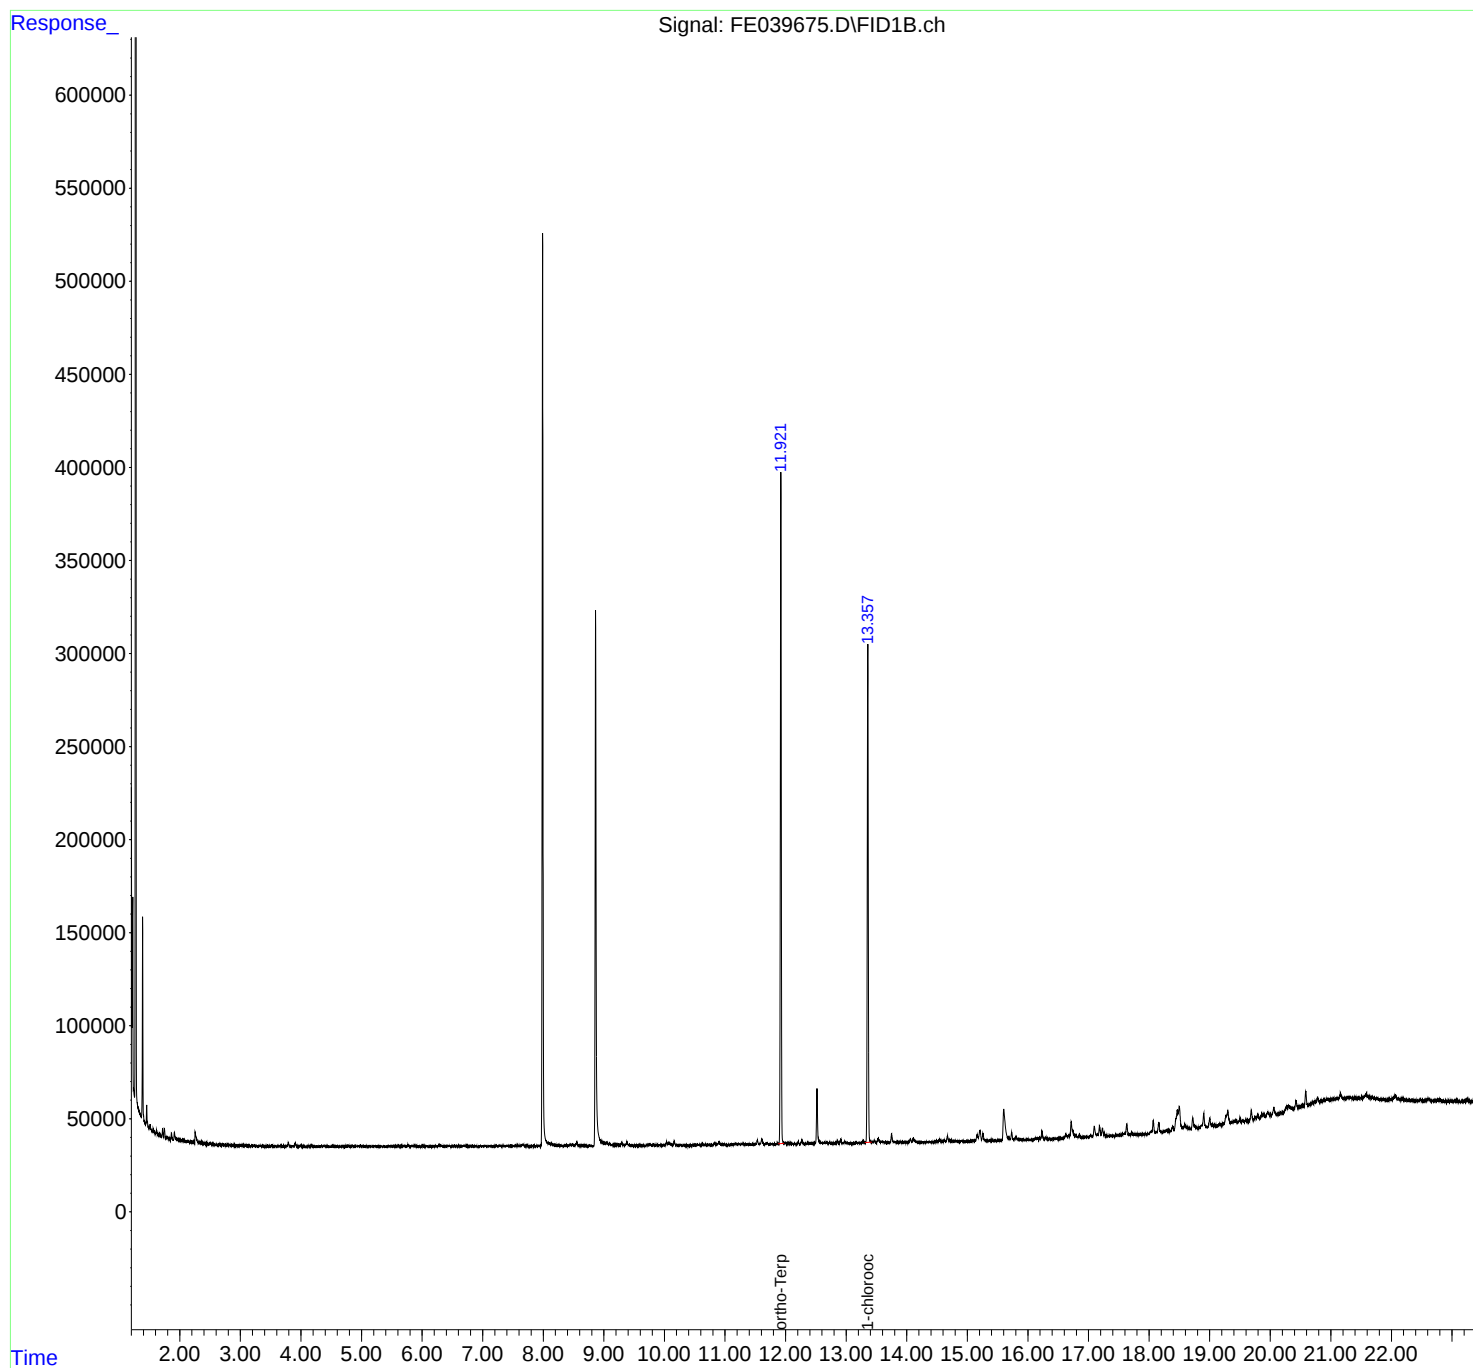


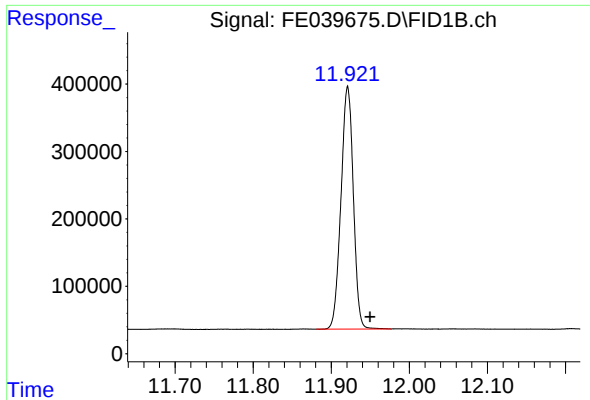

#9 ortho-Terphenyl (SURR)

R.T.: 11.921 min  
Delta R.T.: -0.029 min  
Response: 3959243  
Conc: 26.53 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
TP-203

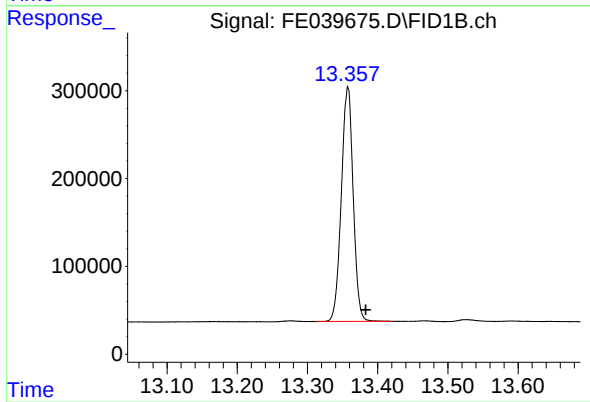

#12 1-chlorooctadecane (SURR)

R.T.: 13.358 min  
Delta R.T.: -0.025 min  
Response: 3136783  
Conc: 27.25 ug/ml