

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010820\  
Data File : FE031060.D  
Signal(s) : FID1B.CH  
Acq On : 08 Jan 2020 11:28  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jan 09 00:50:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE010420.M  
Quant Title :  
QLast Update : Mon Jan 06 08:13:00 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.373  | 7003032  | 19.842 ug/ml |
| 12) N-OCTACOSANE            | 16.802 | 7845474  | 20.408 ug/ml |
| 14) N-DOTRIACONTANE         | 18.525 | 231842   | 0.641 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010820\  
Data File : FE031060.D  
Signal(s) : FID1B.CH  
Acq On : 08 Jan 2020 11:28  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jan 09 00:50:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE010420.M  
Quant Title :  
QLast Update : Mon Jan 06 08:13:00 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

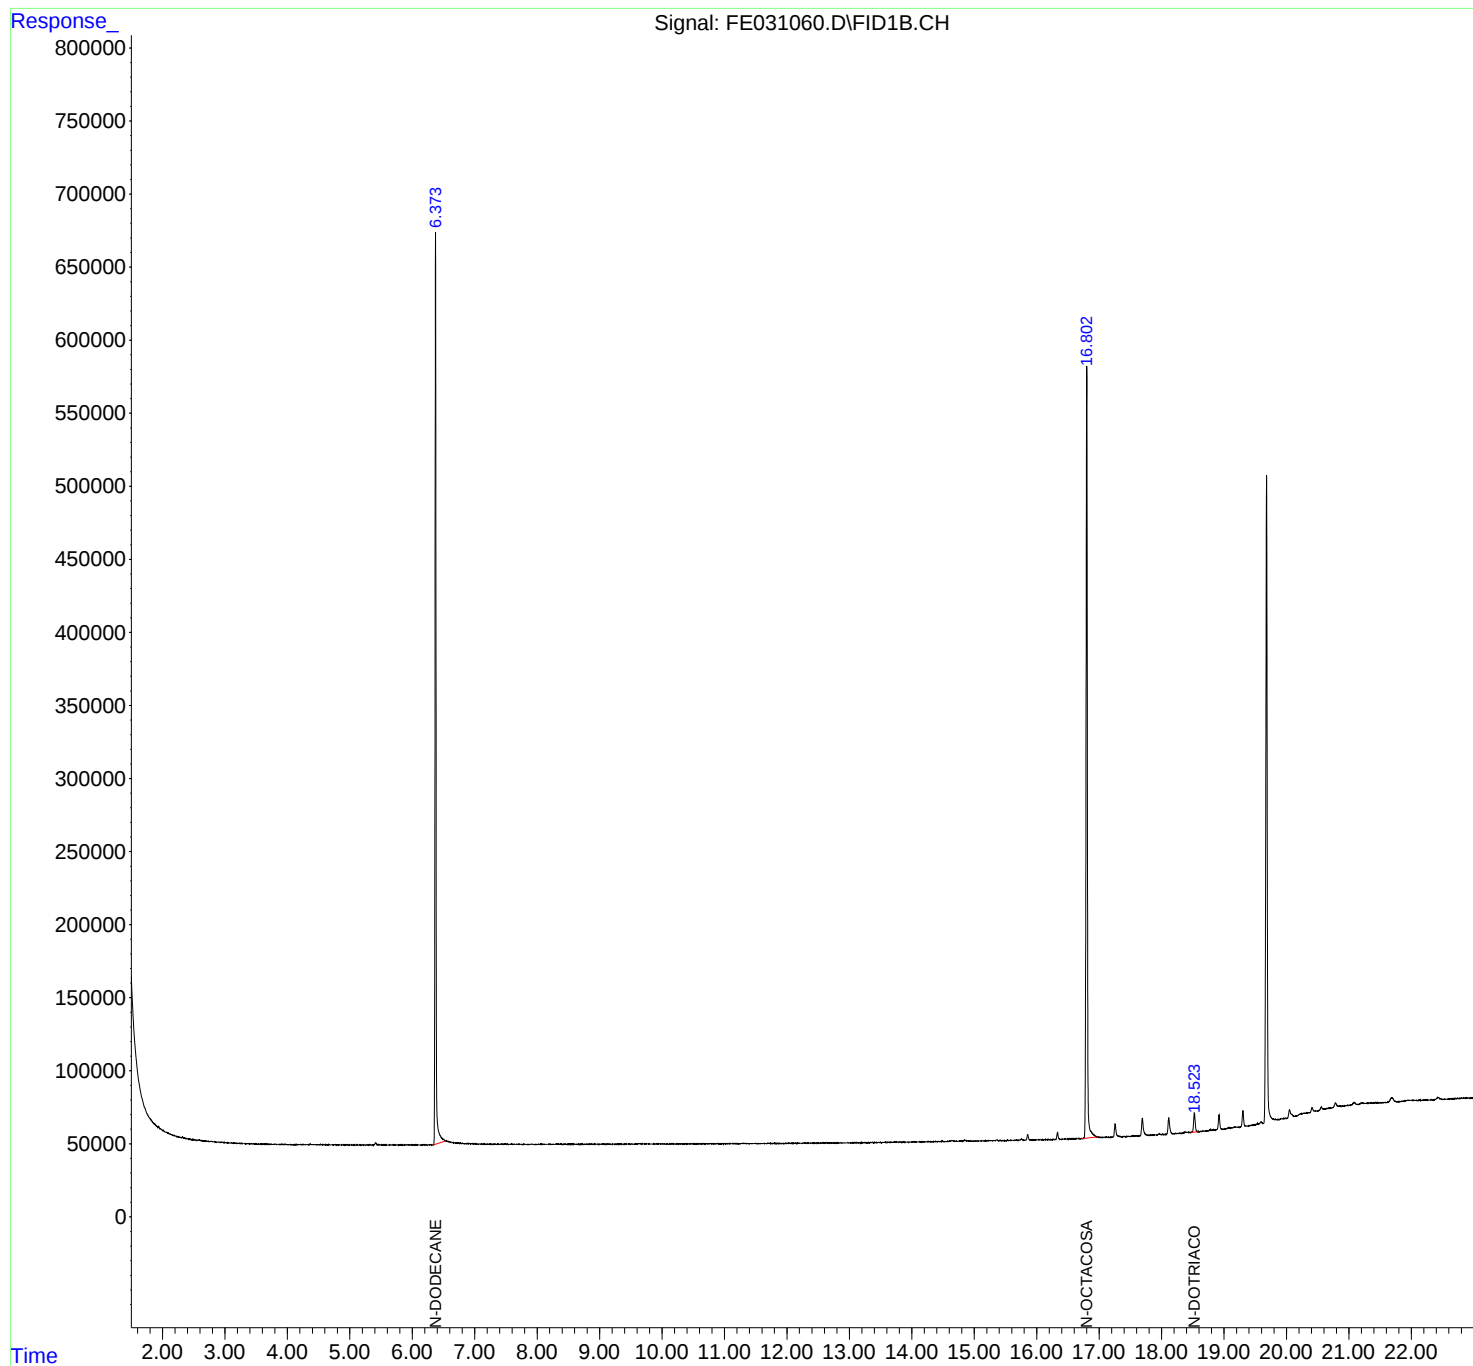


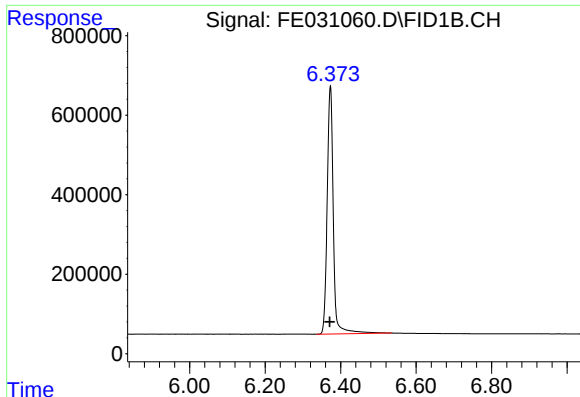

#3 N-DODECANE


R.T.: 6.373 min  
Delta R.T.: 0.001 min  
Response: 7003032  
Conc: 19.84 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

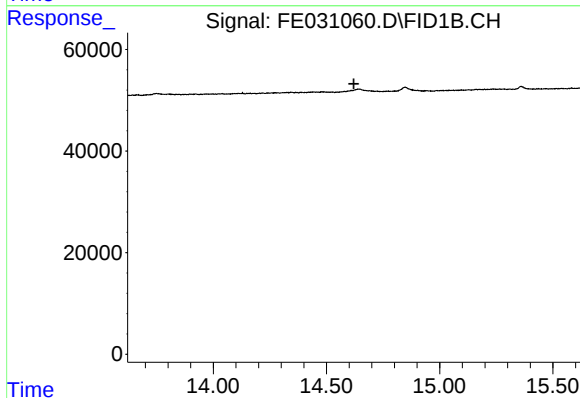


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.621 min  
Response: 0  
Conc: N.D.

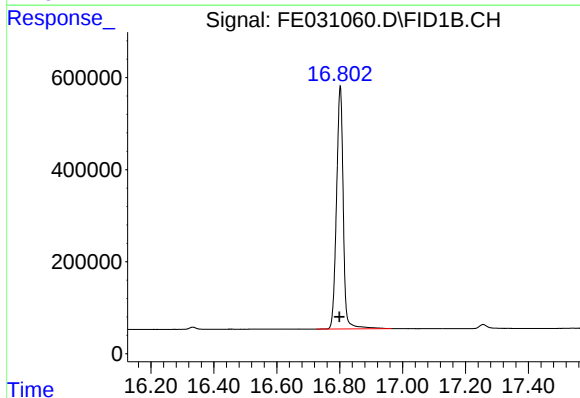

#12 N-OCTACOSANE

R.T.: 16.802 min  
Delta R.T.: 0.003 min  
Response: 7845474  
Conc: 20.41 ug/ml

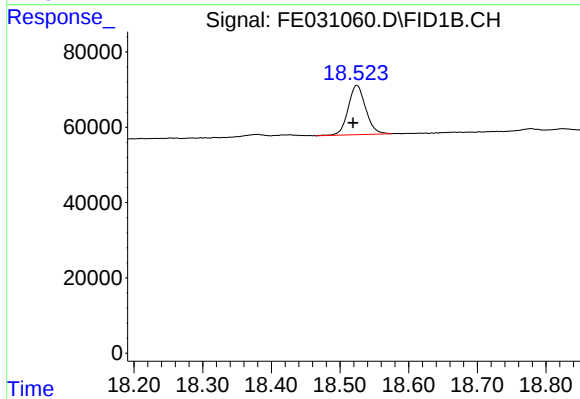

#14 N-DOTRIACONTANE

R.T.: 18.525 min  
Delta R.T.: 0.005 min  
Response: 231842  
Conc: 0.64 ug/ml