

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010820\
 Data File : FE031065.D
 Signal(s) : FID1B.CH
 Acq On : 08 Jan 2020 16:06
 Operator : DD\AJ
 Sample : L1051-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SB-3F-(8.5-10.5)

Integration File: autoint1.e
 Quant Time: Jan 09 00:51:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	5723643	17.153 ug/ml
Target Compounds			
4) N-TETRADECANE	8.228f	875063	2.289 ug/ml
10) N-TETRACOSANE	14.774f	146467	0.382 ug/ml
11) N-HEXACOSANE	15.849	201667	0.527 ug/ml
12) N-OCTACOSANE	16.799	398975	1.038 ug/ml
13) N-TRIACONTANE	17.689	455196	1.187 ug/ml
14) N-DOTRIACONTANE	18.517	639430	1.768 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010820\
Data File : FE031065.D
Signal(s) : FID1B.CH
Acq On : 08 Jan 2020 16:06
Operator : DD\AJ
Sample : L1051-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SB-3F-(8.5-10.5)

Integration File: autoint1.e
Quant Time: Jan 09 00:51:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

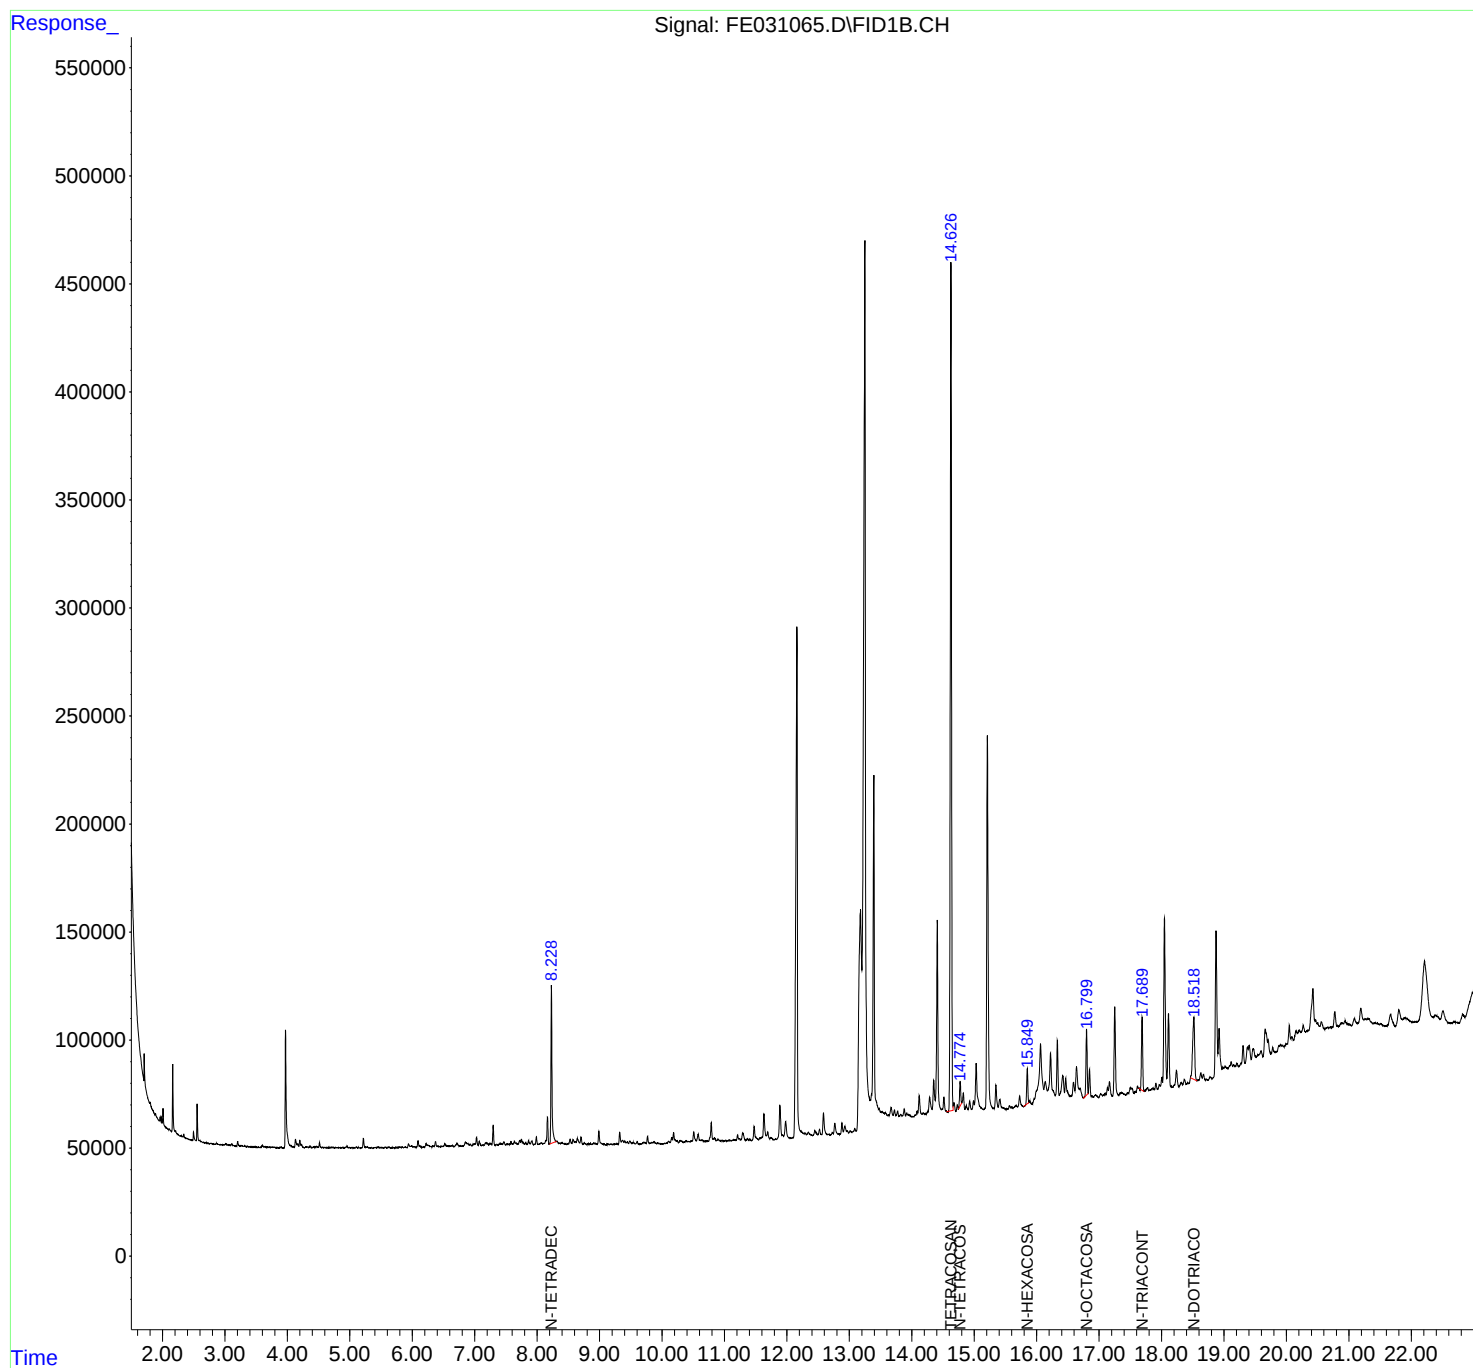


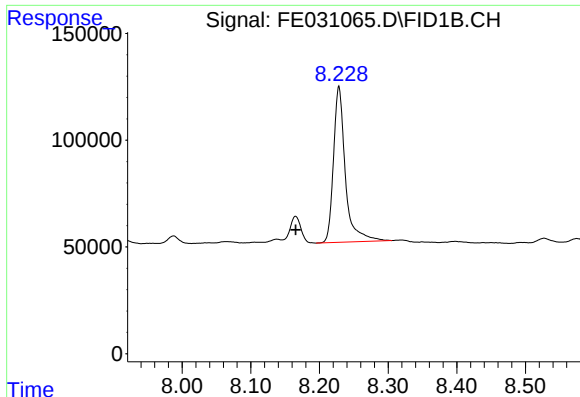

#4 N-TETRADECANE


R.T.: 8.228 min
Delta R.T.: 0.063 min
Response: 875063
Conc: 2.29 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3F-(8.5-10.5)

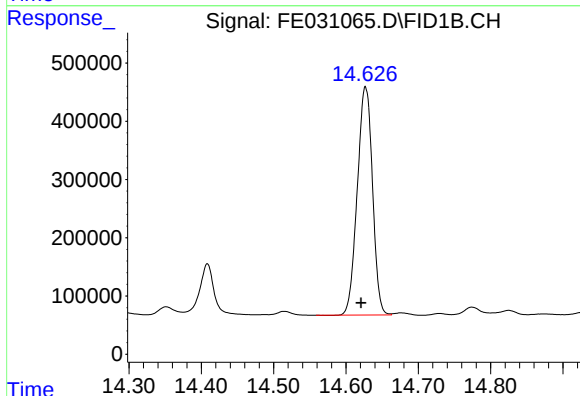


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: 0.006 min
Response: 5723643
Conc: 17.15 ug/ml

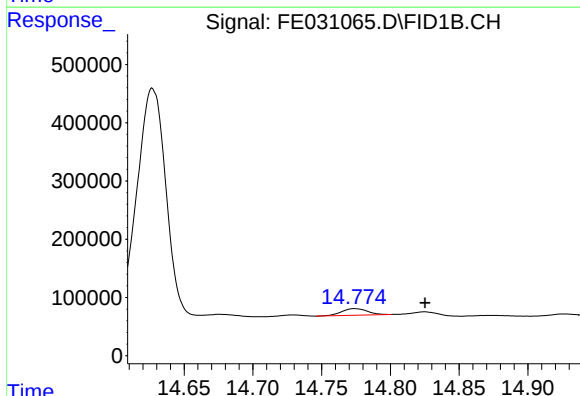


#10 N-TETRACOSANE

R.T.: 14.774 min
Delta R.T.: -0.051 min
Response: 146467
Conc: 0.38 ug/ml

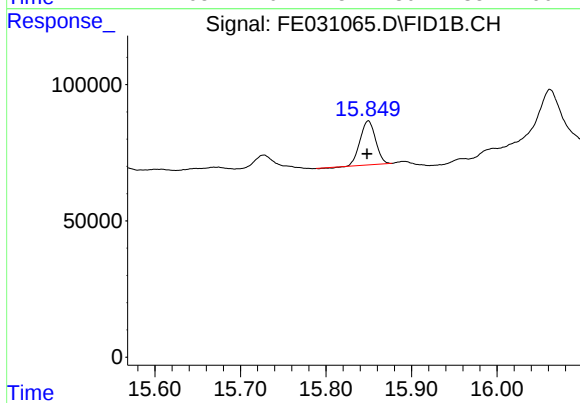

#11 N-HEXACOSANE


R.T.: 15.849 min
Delta R.T.: 0.001 min
Response: 201667
Conc: 0.53 ug/ml

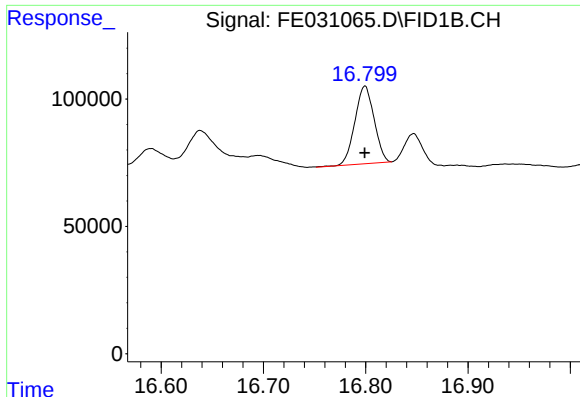

#12 N-OCTACOSANE


R.T.: 16.799 min
Delta R.T.: 0.000 min
Response: 398975
Conc: 1.04 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3F-(8.5-10.5)

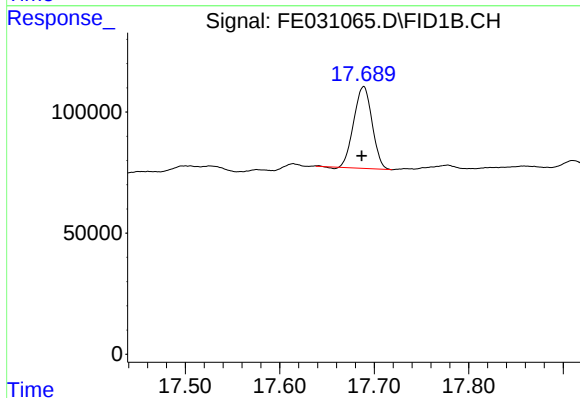

#13 N-TRIACONTANE

R.T.: 17.689 min
Delta R.T.: 0.002 min
Response: 455196
Conc: 1.19 ug/ml

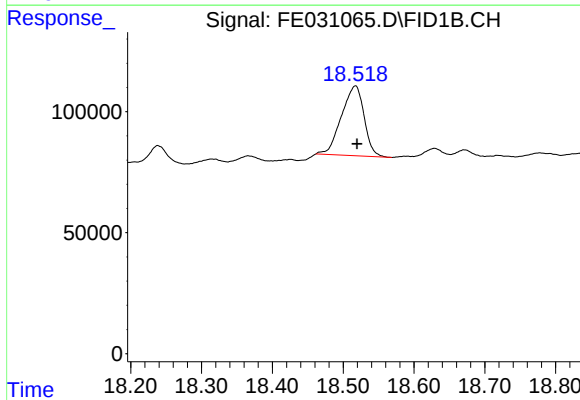

#14 N-DOTRIACONTANE

R.T.: 18.517 min
Delta R.T.: -0.002 min
Response: 639430
Conc: 1.77 ug/ml