

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010820\
 Data File : FE031068.D
 Signal(s) : FID1B.CH
 Acq On : 08 Jan 2020 17:45
 Operator : DD\AJ
 Sample : L1051-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SB-3H-(8.5-10.5)

Integration File: autoint1.e
 Quant Time: Jan 09 00:52:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	7297650	21.870 ug/ml
Target Compounds			
4) N-TETRADECANE	8.232f	3140714	8.214 ug/ml
11) N-HEXACOSANE	15.849	152293	0.398 ug/ml
12) N-OCTACOSANE	16.800	285701	0.743 ug/ml
13) N-TRIACONTANE	17.688	350270	0.914 ug/ml
14) N-DOTRIACONTANE	18.520	266976	0.738 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010820\
Data File : FE031068.D
Signal(s) : FID1B.CH
Acq On : 08 Jan 2020 17:45
Operator : DD\AJ
Sample : L1051-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)

Integration File: autoint1.e
Quant Time: Jan 09 00:52:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

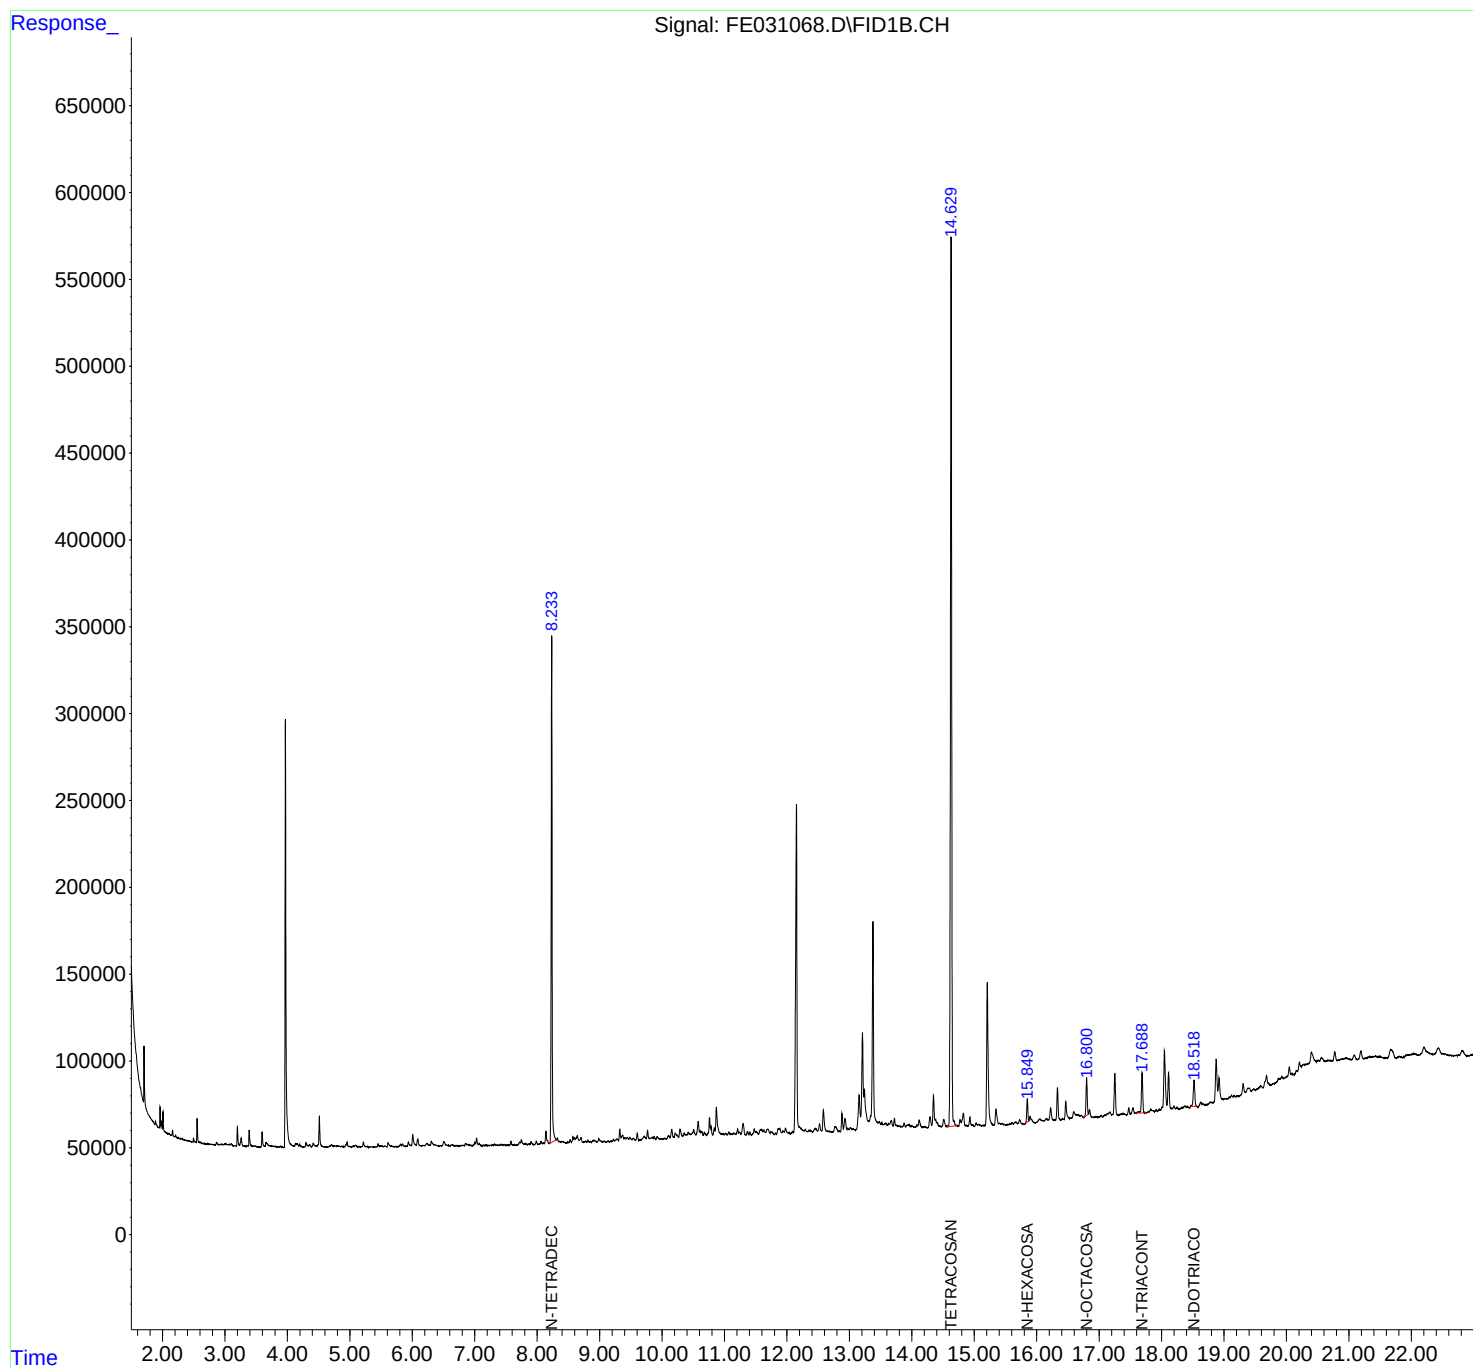


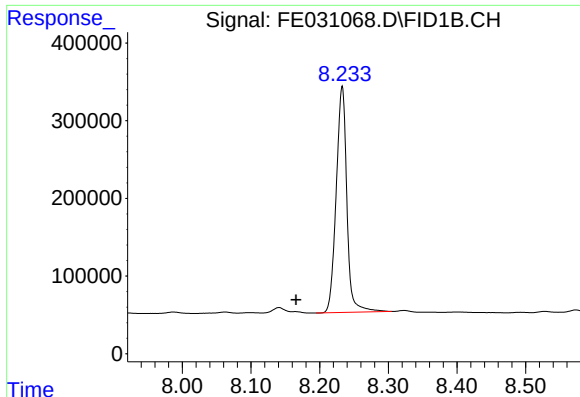

#4 N-TETRADECANE


R.T.: 8.232 min
Delta R.T.: 0.067 min
Response: 3140714
Conc: 8.21 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)

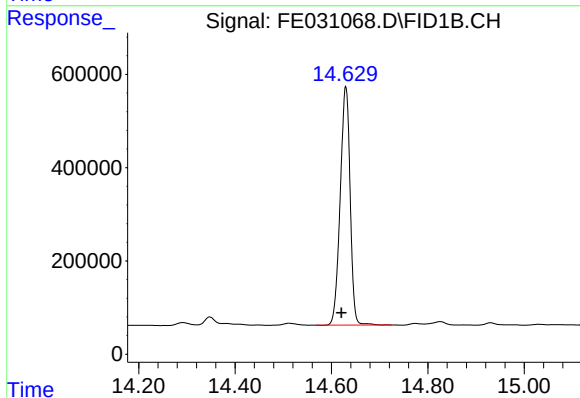


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: 0.009 min
Response: 7297650
Conc: 21.87 ug/ml

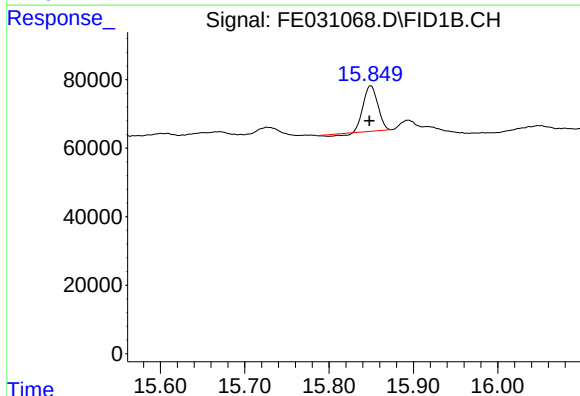


#11 N-HEXACOSANE

R.T.: 15.849 min
Delta R.T.: 0.001 min
Response: 152293
Conc: 0.40 ug/ml

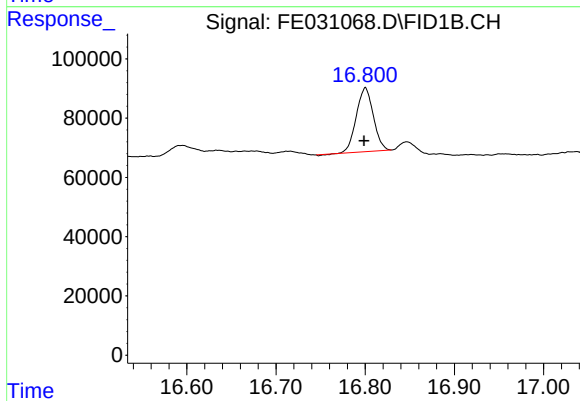

#12 N-OCTACOSANE


R.T.: 16.800 min
Delta R.T.: 0.001 min
Response: 285701
Conc: 0.74 ug/ml

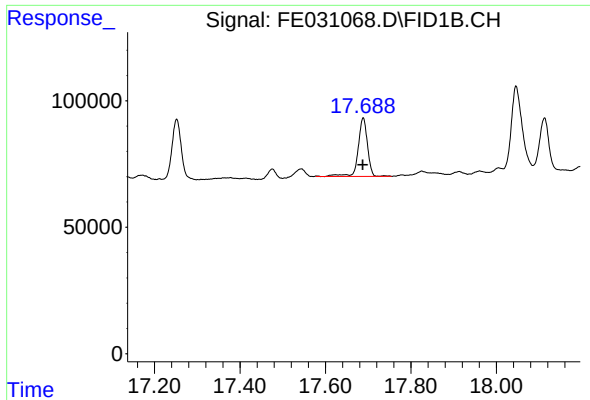

#13 N-TRIACONTANE

R.T.: 17.688 min
Delta R.T.: 0.001 min
Response: 350270
Conc: 0.91 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)

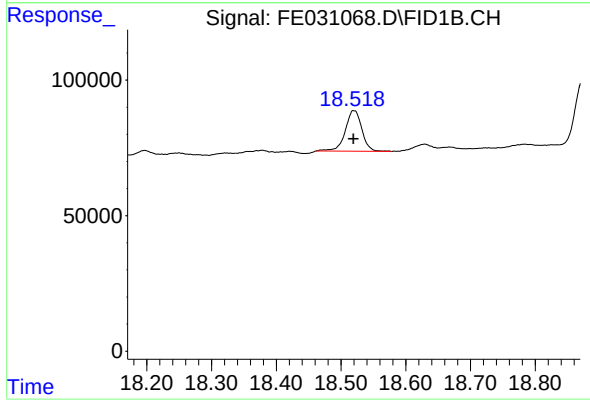

#14 N-DOTRIACONTANE

R.T.: 18.520 min
Delta R.T.: 0.000 min
Response: 266976
Conc: 0.74 ug/ml