

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010820\
 Data File : FE031069.D
 Signal(s) : FID1B.CH
 Acq On : 08 Jan 2020 18:18
 Operator : DD\AJ
 Sample : L1051-10MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SB-3H-(8.5-10.5)MS

Manual Integrations
 APPROVED

Ankita
 1/16/2020 11:54:21 AM

Integration File: autoint1.e
 Quant Time: Jan 09 00:52:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	5919298	17.739 ug/ml
Target Compounds			
1) N-OCTANE	2.341	5431179	14.135 ug/ml
2) N-DECANE	4.366	6423653	17.096 ug/ml
3) N-DODECANE	6.374	6509727	18.445 ug/ml
4) N-TETRADECANE	8.171	6716816	17.566 ug/mlm
5) N-HEXADECANE	9.771	6779523	17.512 ug/ml
6) N-OCTADECANE	11.215	6772727	17.604 ug/ml
7) N-EICOSANE	12.527	6707539	17.240 ug/ml
8) N-DOCOSANE	13.726	6650148	17.220 ug/ml
10) N-TETRACOSANE	14.832	6826523	17.798 ug/ml
11) N-HEXACOSANE	15.854	6715524	17.557 ug/ml
12) N-OCTACOSANE	16.805	6715658	17.469 ug/ml
13) N-TRIACONTANE	17.692	6549683	17.085 ug/mlm
14) N-DOTRIACONTANE	18.526	6207661	17.164 ug/ml
15) N-TETRATRIACONTANE	19.310	5624378	16.867 ug/ml
16) N-HEXATRIACONTANE	20.050	5160229	17.442 ug/ml
17) N-OCTATRIACONTANE	20.780	4548926	17.543 ug/ml
18) N-TETRACONTANE	21.670	4523938	18.229 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010820\
Data File : FE031069.D
Signal(s) : FID1B.CH
Acq On : 08 Jan 2020 18:18
Operator : DD\AJ
Sample : L1051-10MS
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
FID_E
ClientSampled :
SB-3H-(8.5-10.5)MS


Manual Integrations
APPROVED

Ankita
1/16/2020 11:54:21 AM

Integration File: autoint1.e
Quant Time: Jan 09 00:52:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

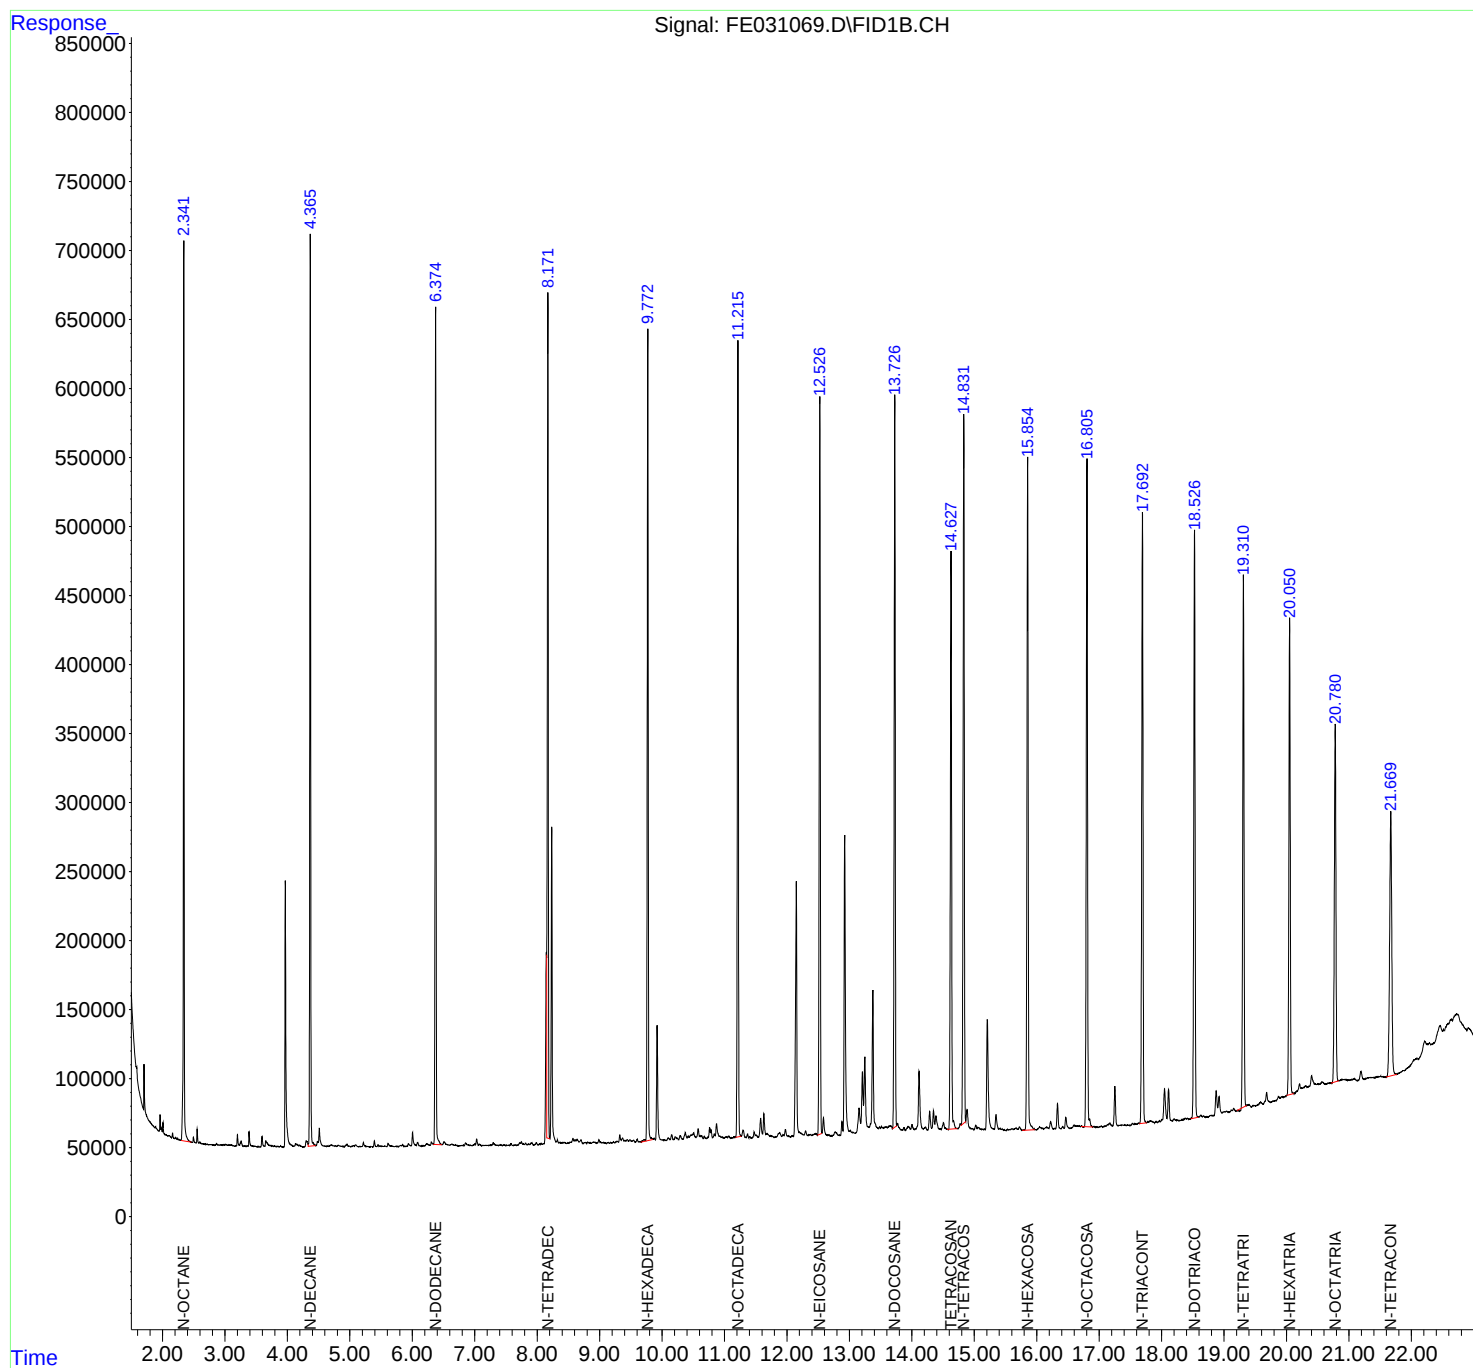

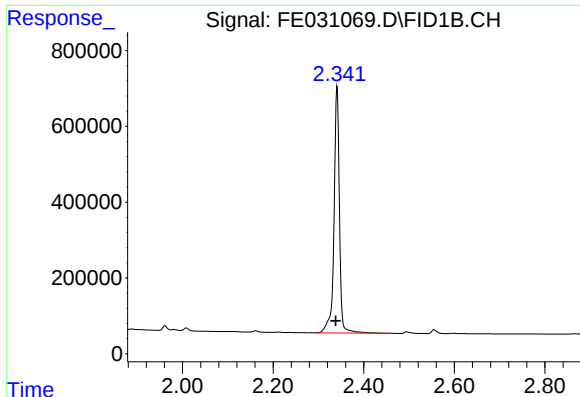


#1 N-OCTANE

R.T.: 2.341 min
Delta R.T.: 0.003 min
Response: 5431179
Conc: 14.13 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)MS


Manual Integrations
APPROVED

Ankita
1/16/2020 11:54:21 AM

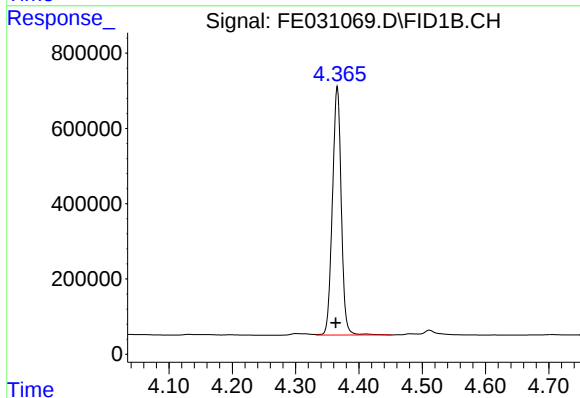


#2 N-DECANE

R.T.: 4.366 min
Delta R.T.: 0.002 min
Response: 6423653
Conc: 17.10 ug/ml

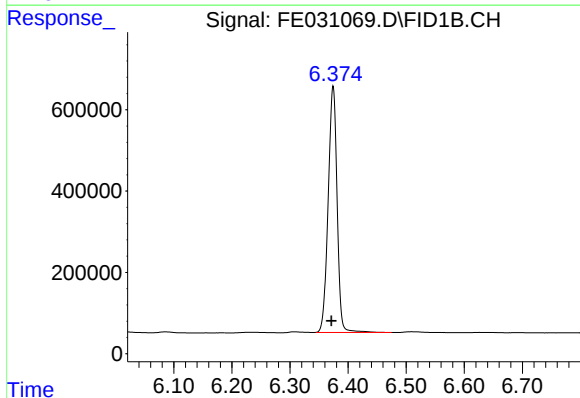


#3 N-DODECANE

R.T.: 6.374 min
Delta R.T.: 0.003 min
Response: 6509727
Conc: 18.44 ug/ml

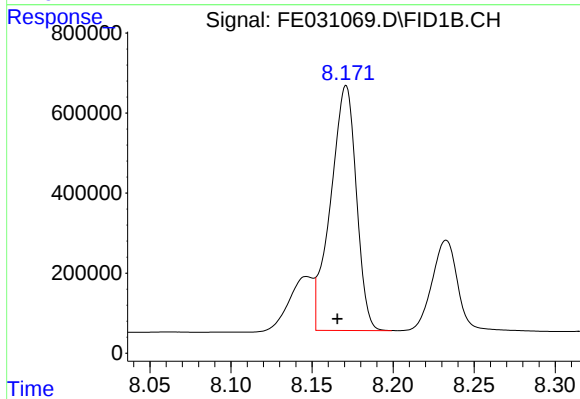

#4 N-TETRADECANE

R.T.: 8.171 min
Delta R.T.: 0.005 min
Response: 6716816
Conc: 17.57 ug/ml m

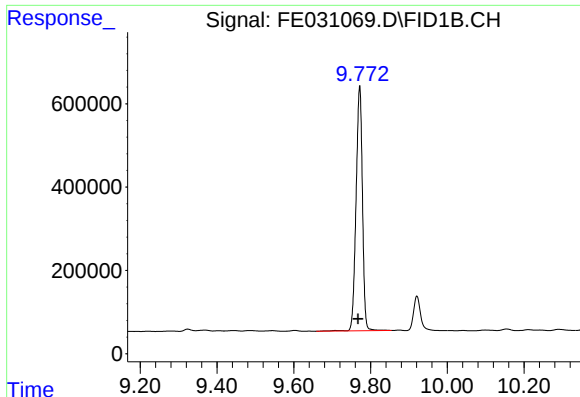


#5 N-HEXADECANE

R.T.: 9.771 min
Delta R.T.: 0.004 min
Response: 6779523
Conc: 17.51 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)MS


Manual Integrations
APPROVED

Ankita
1/16/2020 11:54:21 AM

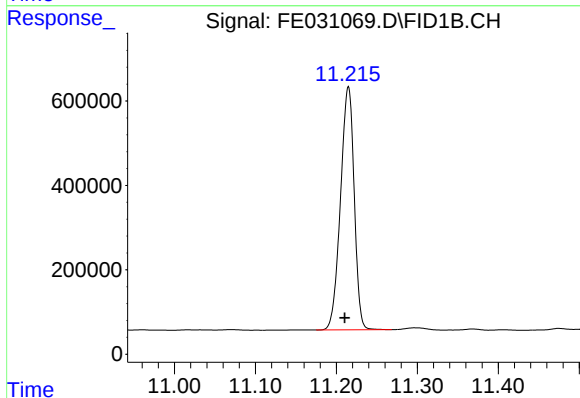


#6 N-OCTADECANE

R.T.: 11.215 min
Delta R.T.: 0.004 min
Response: 6772727
Conc: 17.60 ug/ml

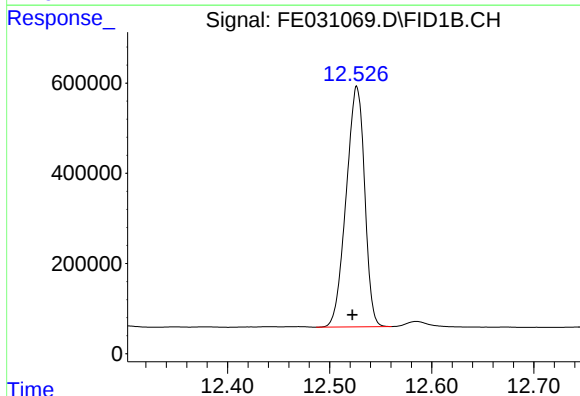


#7 N-EICOSANE

R.T.: 12.527 min
Delta R.T.: 0.004 min
Response: 6707539
Conc: 17.24 ug/ml

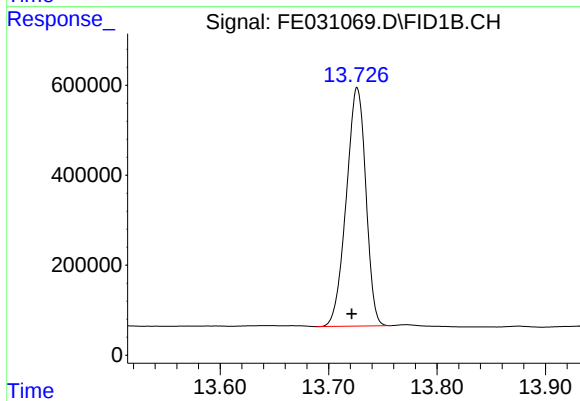

#8 N-DOCOSANE

R.T.: 13.726 min
Delta R.T.: 0.005 min
Response: 6650148
Conc: 17.22 ug/ml

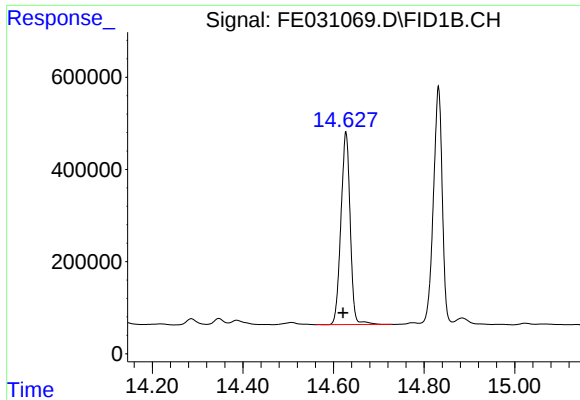


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: 0.007 min
Response: 5919298
Conc: 17.74 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)MS


Manual Integrations
APPROVED

Ankita
1/16/2020 11:54:21 AM

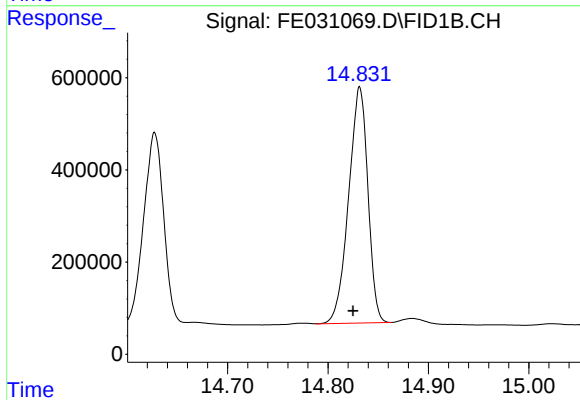


#10 N-TETRACOSANE

R.T.: 14.832 min
Delta R.T.: 0.007 min
Response: 6826523
Conc: 17.80 ug/ml

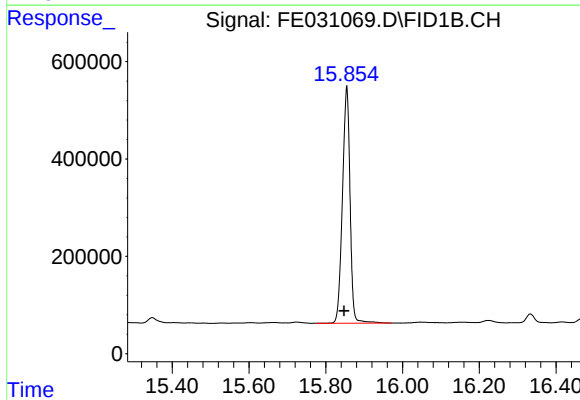


#11 N-HEXACOSANE

R.T.: 15.854 min
Delta R.T.: 0.006 min
Response: 6715524
Conc: 17.56 ug/ml

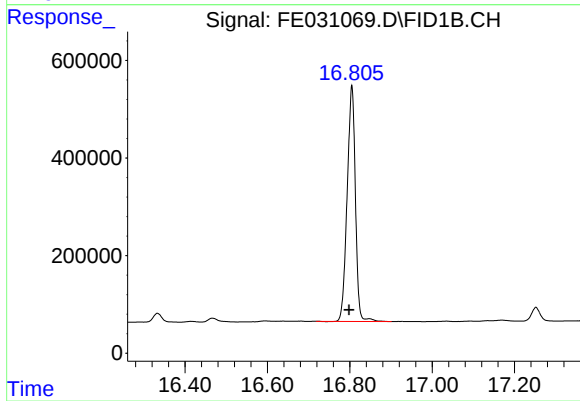

#12 N-OCTACOSANE

R.T.: 16.805 min
Delta R.T.: 0.006 min
Response: 6715658
Conc: 17.47 ug/ml

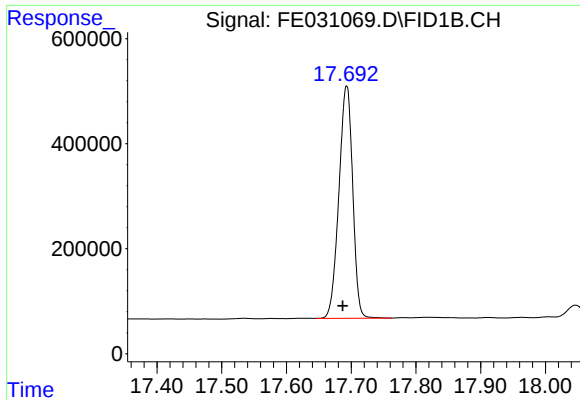


#13 N-TRIACONTANE

R.T.: 17.692 min
Delta R.T.: 0.005 min
Response: 6549683
Conc: 17.08 ug/ml m

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)MS


Manual Integrations
APPROVED

Ankita
1/16/2020 11:54:21 AM

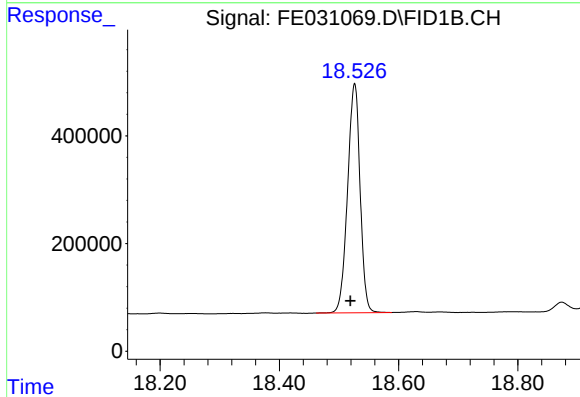


#14 N-DOTRIACONTANE

R.T.: 18.526 min
Delta R.T.: 0.007 min
Response: 6207661
Conc: 17.16 ug/ml

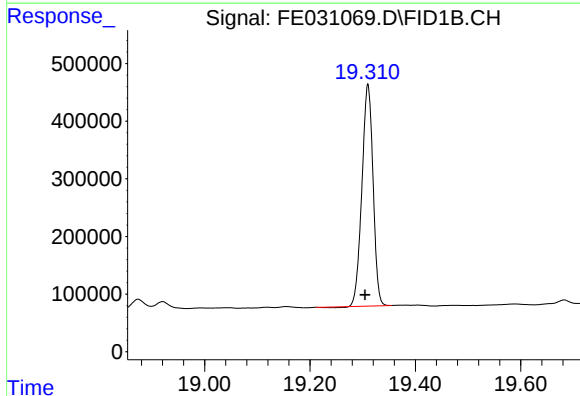


#15 N-TETRATRIACONTANE

R.T.: 19.310 min
Delta R.T.: 0.006 min
Response: 5624378
Conc: 16.87 ug/ml

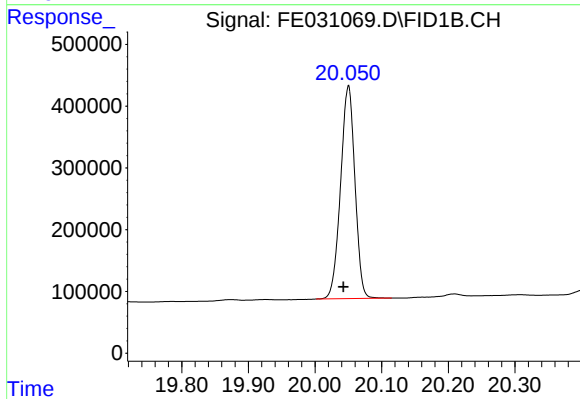

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.008 min
Response: 5160229
Conc: 17.44 ug/ml

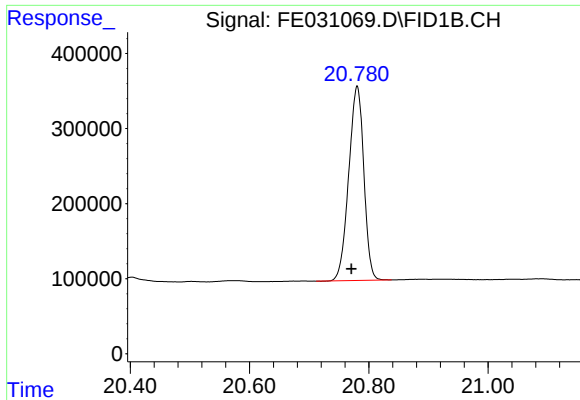


#17 N-OCTATRIACONTANE

R.T.: 20.780 min
Delta R.T.: 0.010 min
Response: 4548926
Conc: 17.54 ug/ml

Instrument :
FID_E
ClientSampleId :
SB-3H-(8.5-10.5)MS

Manual Integrations
APPROVED

Ankita
1/16/2020 11:54:21 AM

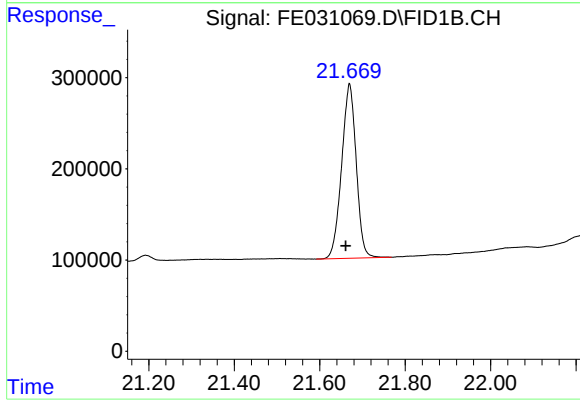

#18 N-TETRACONTANE

R.T.: 21.670 min
Delta R.T.: 0.008 min
Response: 4523938
Conc: 18.23 ug/ml