

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010825AL\
Data File : FE051878.D
Signal(s) : FID1B.ch
Acq On : 08 Jan 2025 21:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 08 23:02:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 010225.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 04:14:12 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.277	297006	2.259 ug/ml
18) T	n-Dotriacontane (C32)	19.108	251916	1.985 ug/ml
19) T	n-Tetratriacontane (C34)	19.913	329900	2.969 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010825AL\
Data File : FE051878.D
Signal(s) : FID1B.ch
Acq On : 08 Jan 2025 21:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 08 23:02:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 010225.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 04:14:12 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

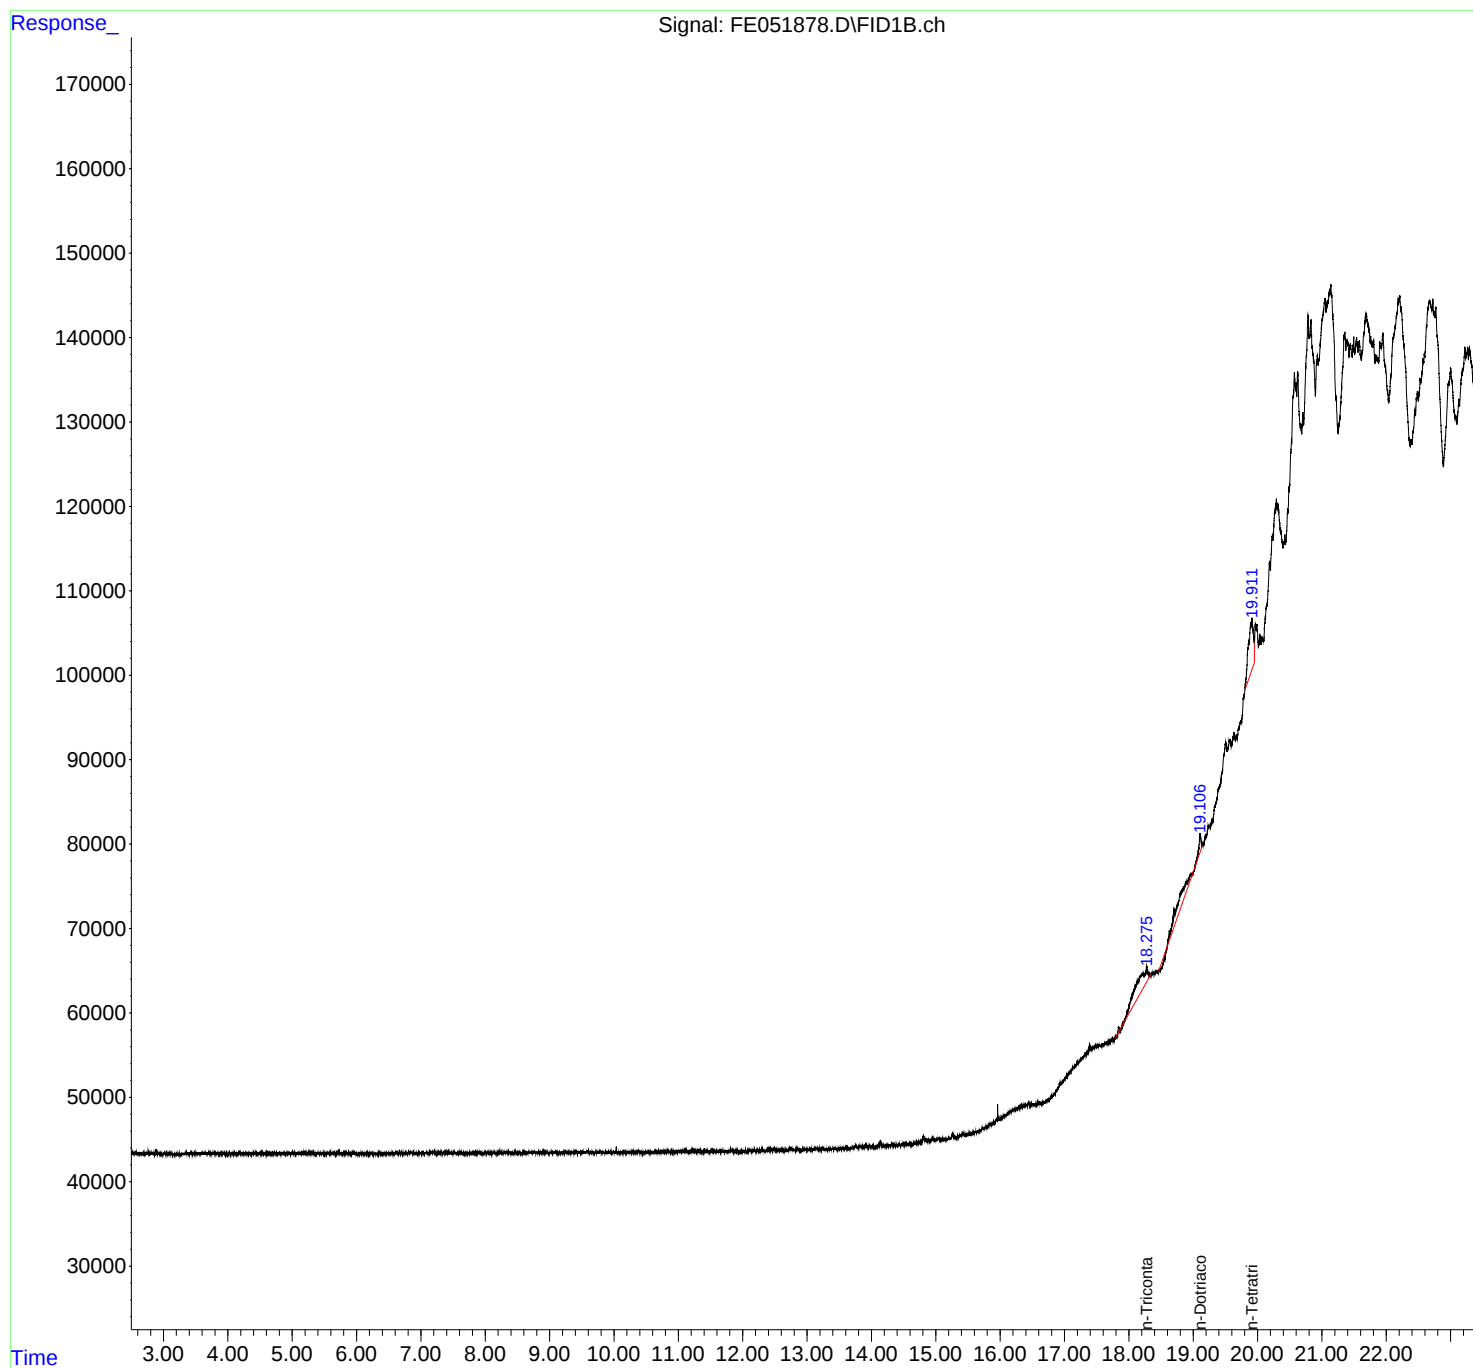


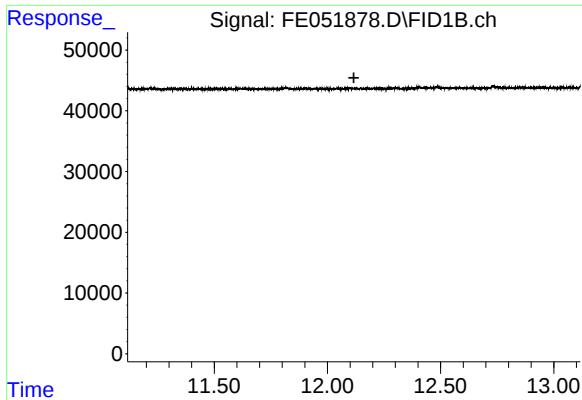

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.117 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

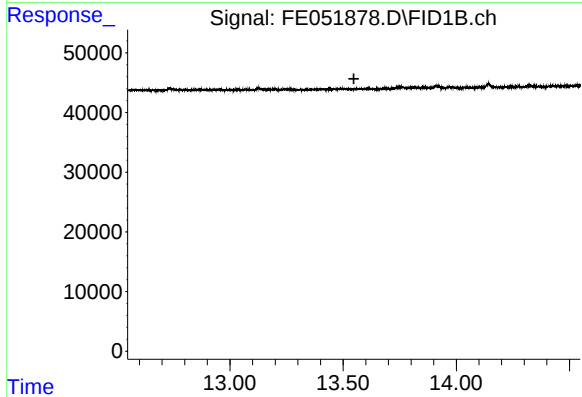


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.548 min
Response: 0
Conc: N.D.

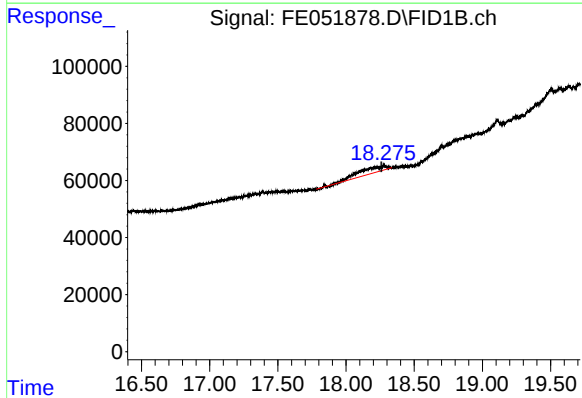


#17 n-Tricontane (C30)

R.T.: 18.277 min
Delta R.T.: 0.017 min
Response: 297006
Conc: 2.26 ug/ml

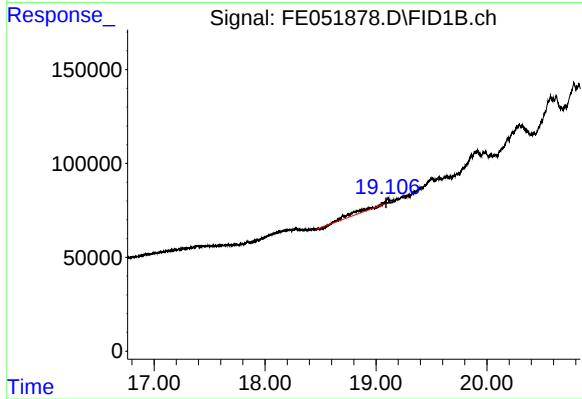

#18 n-Dotriacontane (C32)

R.T.: 19.108 min
Delta R.T.: 0.015 min
Response: 251916
Conc: 1.99 ug/ml

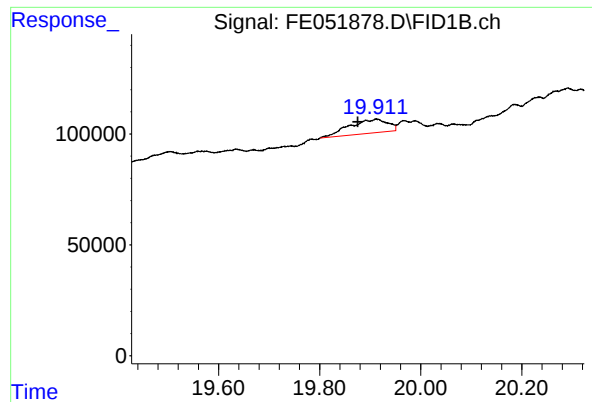

#19 n-Tetratriacontane (C34)

R.T.: 19.913 min
Delta R.T.: 0.037 min
Response: 329900
Conc: 2.97 ug/ml

Instrument :

FID_E

ClientSampleId :