

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010920\
 Data File : FE031082.D
 Signal(s) : FID1B.CH
 Acq On : 09 Jan 2020 10:10
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jan 09 14:14:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.370	7427192	20.761 ug/ml
12)	N-OCTACOSANE	16.795	7714251	20.067 ug/ml
13)	N-TRIACONTANE	17.680	342933	0.895 ug/ml
14)	N-DOTRIACONTANE	18.512	353648	0.978 ug/ml
15)	N-TETRATRIACONTANE	19.295	251093	0.753 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE010920\
Data File : FE031082.D
Signal(s) : FID1B.CH
Acq On : 09 Jan 2020 10:10
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jan 09 14:14:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

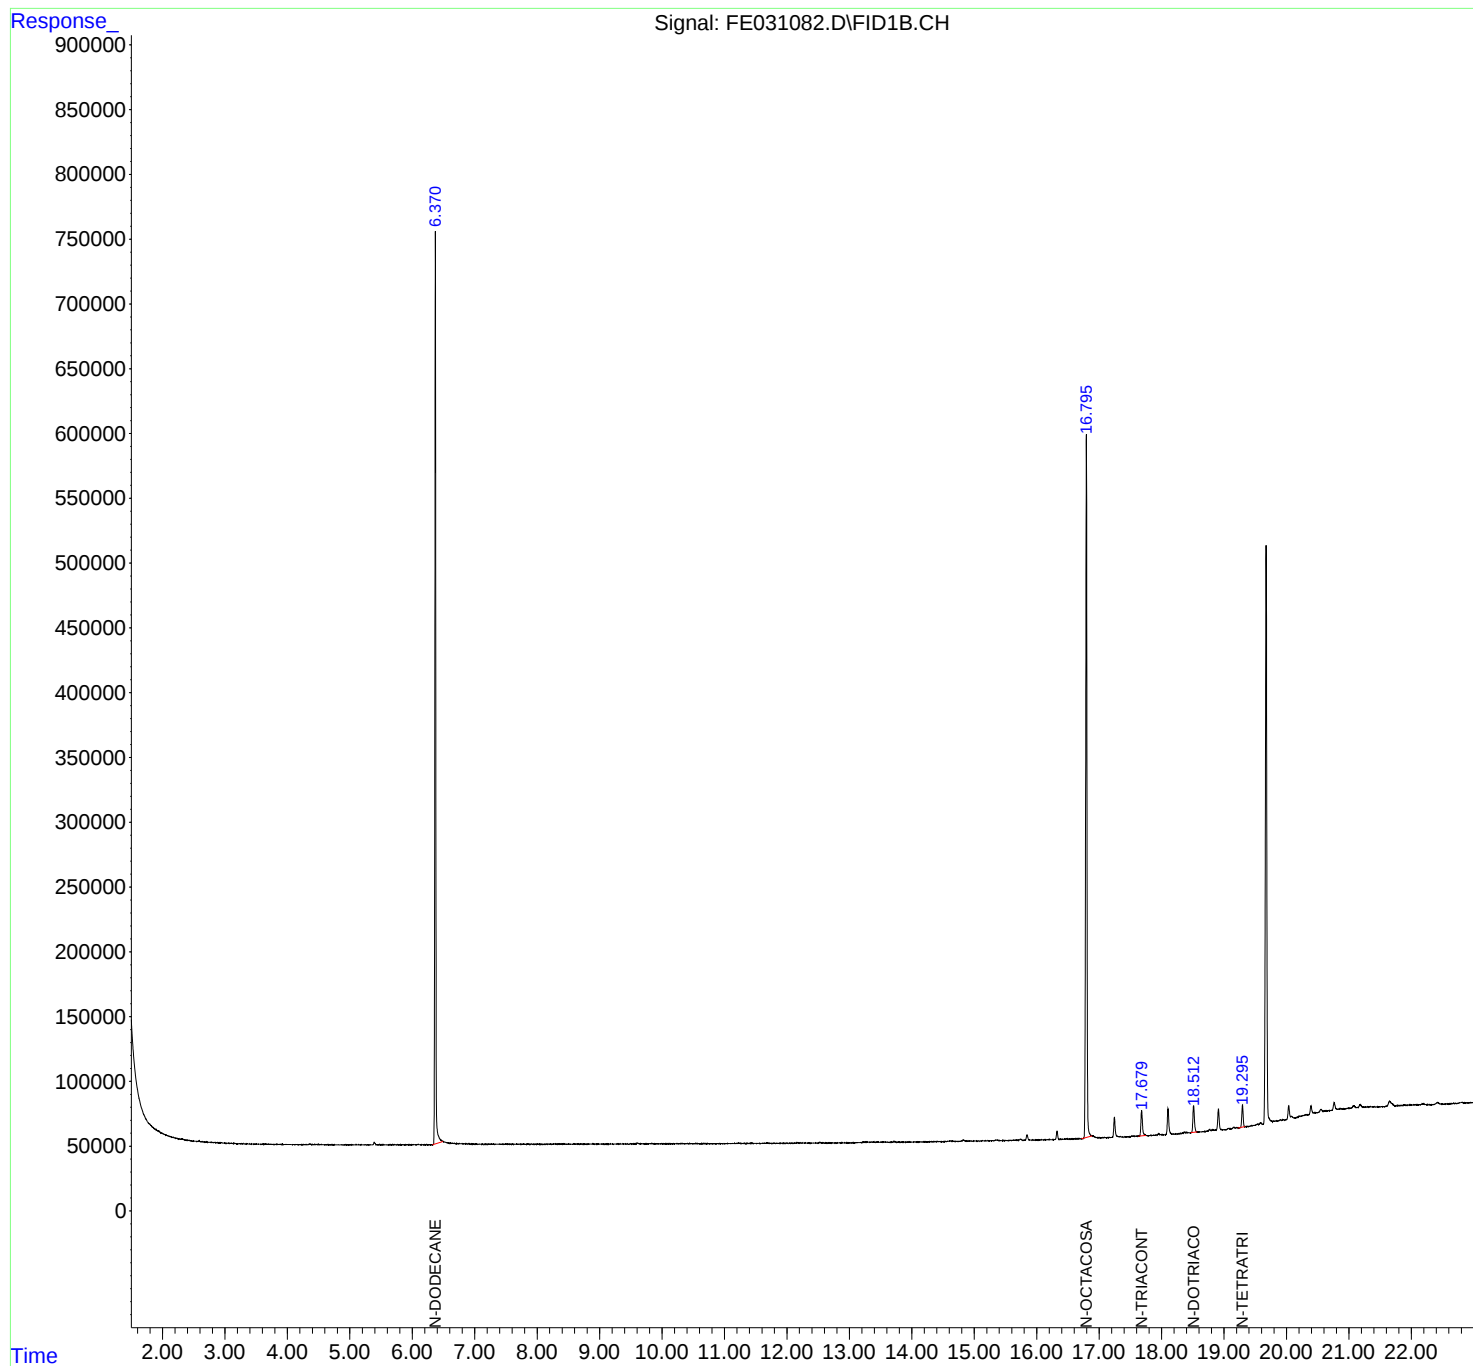


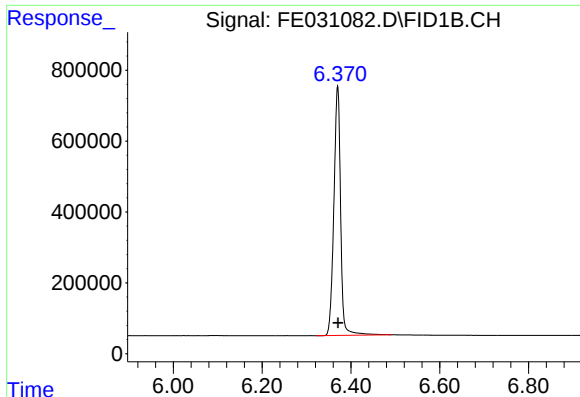

#3 N-DODECANE


R.T.: 6.370 min
Delta R.T.: -0.002 min
Response: 7427192
Conc: 20.76 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

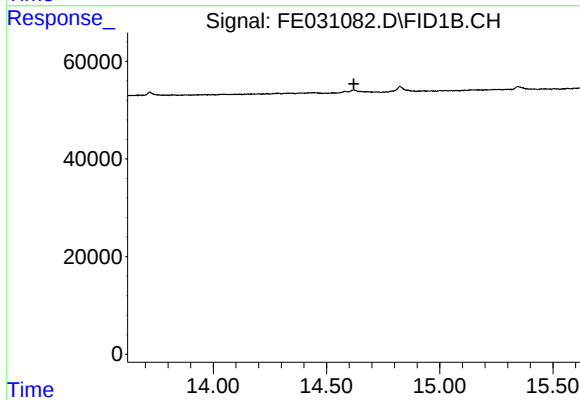


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.621 min
Response: 0
Conc: N.D.

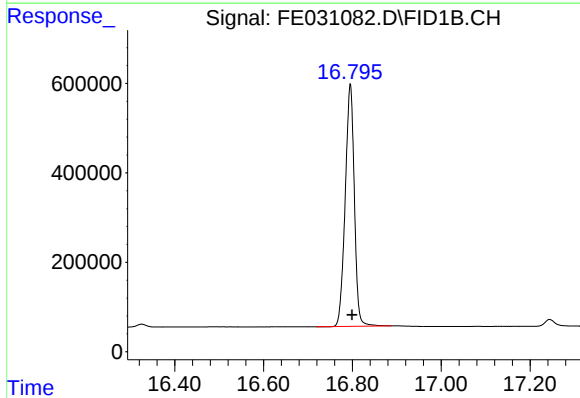


#12 N-OCTACOSANE

R.T.: 16.795 min
Delta R.T.: -0.004 min
Response: 7714251
Conc: 20.07 ug/ml

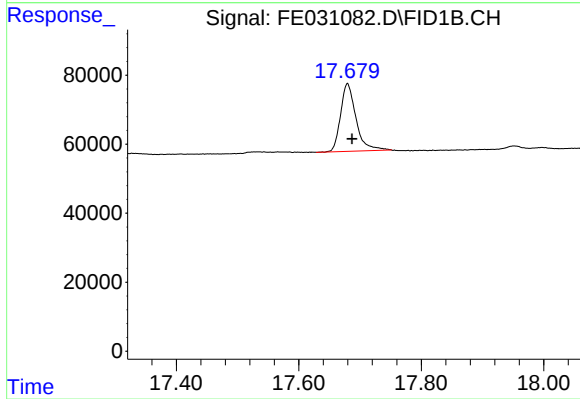

#13 N-TRIACONTANE


R.T.: 17.680 min
Delta R.T.: -0.007 min
Response: 342933
Conc: 0.89 ug/ml

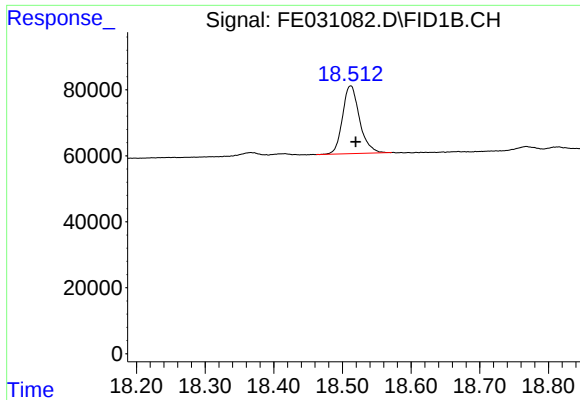

#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: -0.007 min
Response: 353648
Conc: 0.98 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

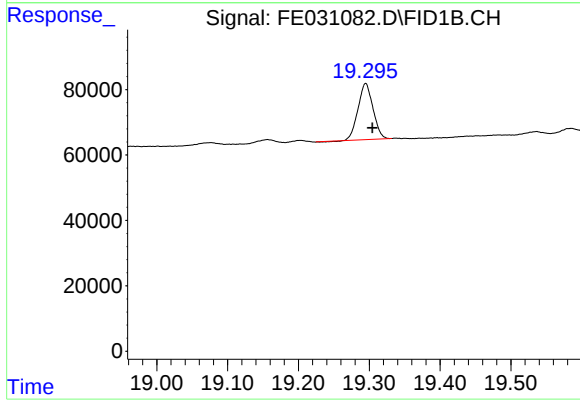

#15 N-TETRATRIACONTANE

R.T.: 19.295 min
Delta R.T.: -0.009 min
Response: 251093
Conc: 0.75 ug/ml