

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010924AL\  
 Data File : FE046107.D  
 Signal(s) : FID1B.ch  
 Acq On : 09 Jan 2024 08:09  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jan 10 02:34:37 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 122923.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Dec 29 03:49:54 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units  |
|--------------------------------|--------|----------|-------------|
| -----                          |        |          |             |
| System Monitoring Compounds    |        |          |             |
| Target Compounds               |        |          |             |
| 18) T n-Dotriacontane (C32)    | 18.851 | 24070    | 0.161 ug/ml |
| 19) T n-Tetratriacontane (C34) | 19.677 | 14397    | 0.100 ug/ml |
| 22) T n-Tetracontane (C40)     | 22.033 | 5271     | 0.034 ug/ml |
| -----                          |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE010924AL\  
Data File : FE046107.D  
Signal(s) : FID1B.ch  
Acq On : 09 Jan 2024 08:09  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jan 10 02:34:37 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 122923.M  
Quant Title : GC Extractables  
QLast Update : Fri Dec 29 03:49:54 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

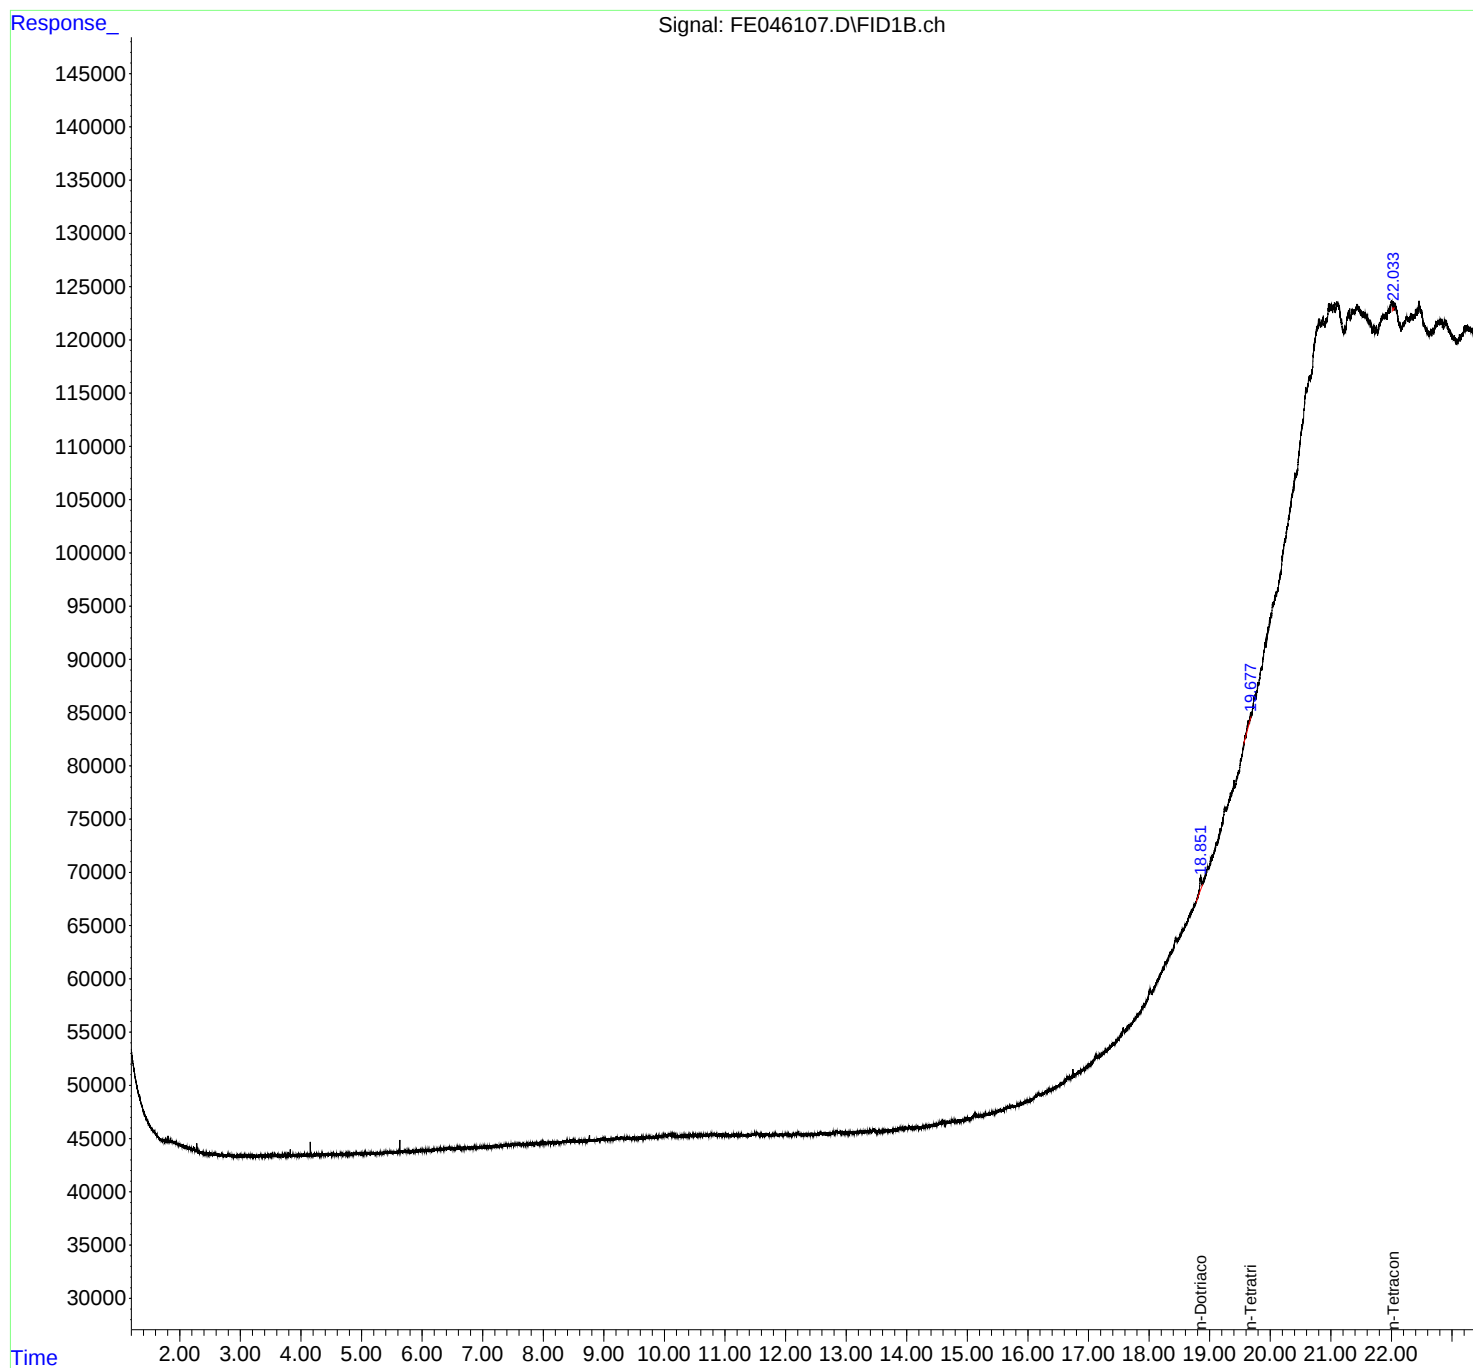


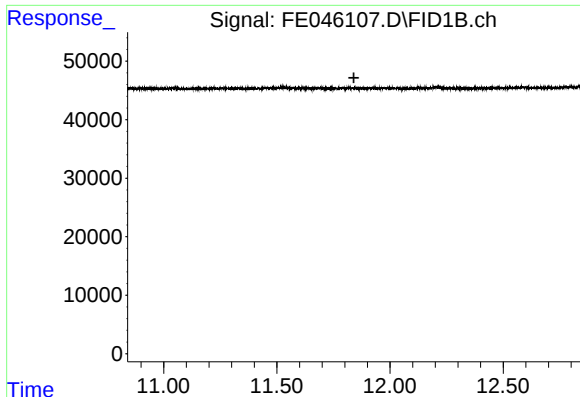

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 11.840 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

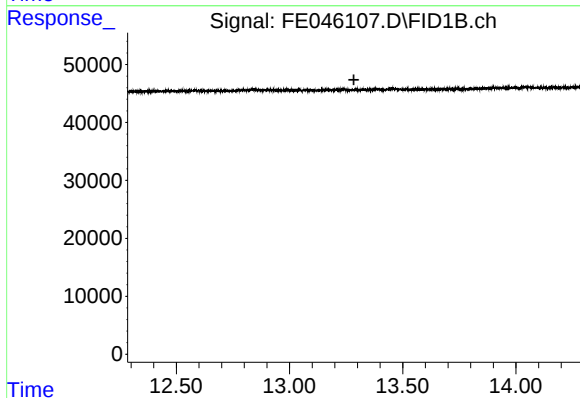


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T.: 13.284 min  
Response: 0  
Conc: N.D.

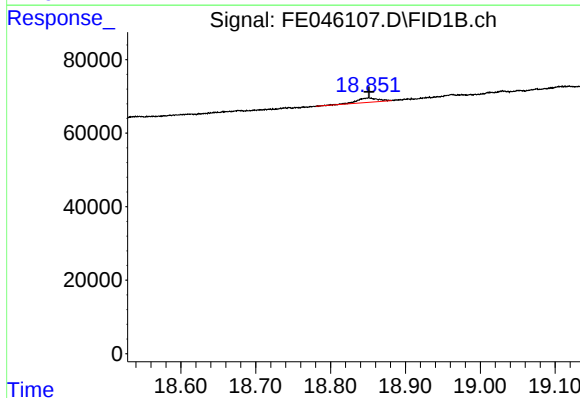


#18 n-Dotriacontane (C32)

R.T.: 18.851 min  
Delta R.T.: 0.000 min  
Response: 24070  
Conc: 0.16 ug/ml

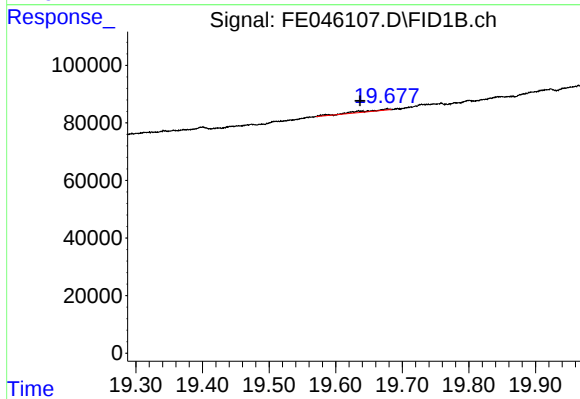

#19 n-Tetratriacontane (C34)

R.T.: 19.677 min  
Delta R.T.: 0.041 min  
Response: 14397  
Conc: 0.10 ug/ml

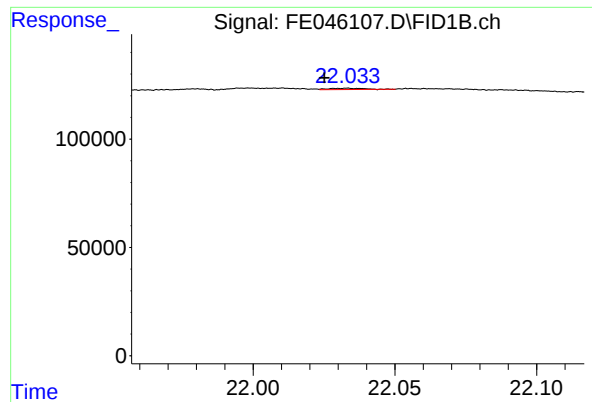

#22 n-Tetracontane (C40)

R.T.: 22.033 min  
Delta R.T.: 0.008 min  
Response: 5271  
Conc: 0.03 ug/ml

Instrument :

FID\_E

ClientSampleId :