

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
 Data File : FE031098.D
 Signal(s) : FID1B.CH
 Acq On : 13 Jan 2020 17:45
 Operator : DD\AJ
 Sample : L1106-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 14 07:31:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.621	5308701	15.909 ug/ml
Target Compounds			
4) N-TETRADECANE	8.224f	485237	1.269 ug/ml
6) N-OCTADECANE	11.211	516445	1.342 ug/ml
7) N-EICOSANE	12.573f	2522844	6.484 ug/ml
8) N-DOCOSANE	13.737	418557	1.084 ug/ml
10) N-TETRACOSANE	14.795	1963488	5.119 ug/ml
12) N-OCTACOSANE	16.797	440831	1.147 ug/ml
13) N-TRIACONTANE	17.681	554448	1.446 ug/ml
14) N-DOTRIACONTANE	18.508	347739	0.961 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
Data File : FE031098.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2020 17:45
Operator : DD\AJ
Sample : L1106-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 14 07:31:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

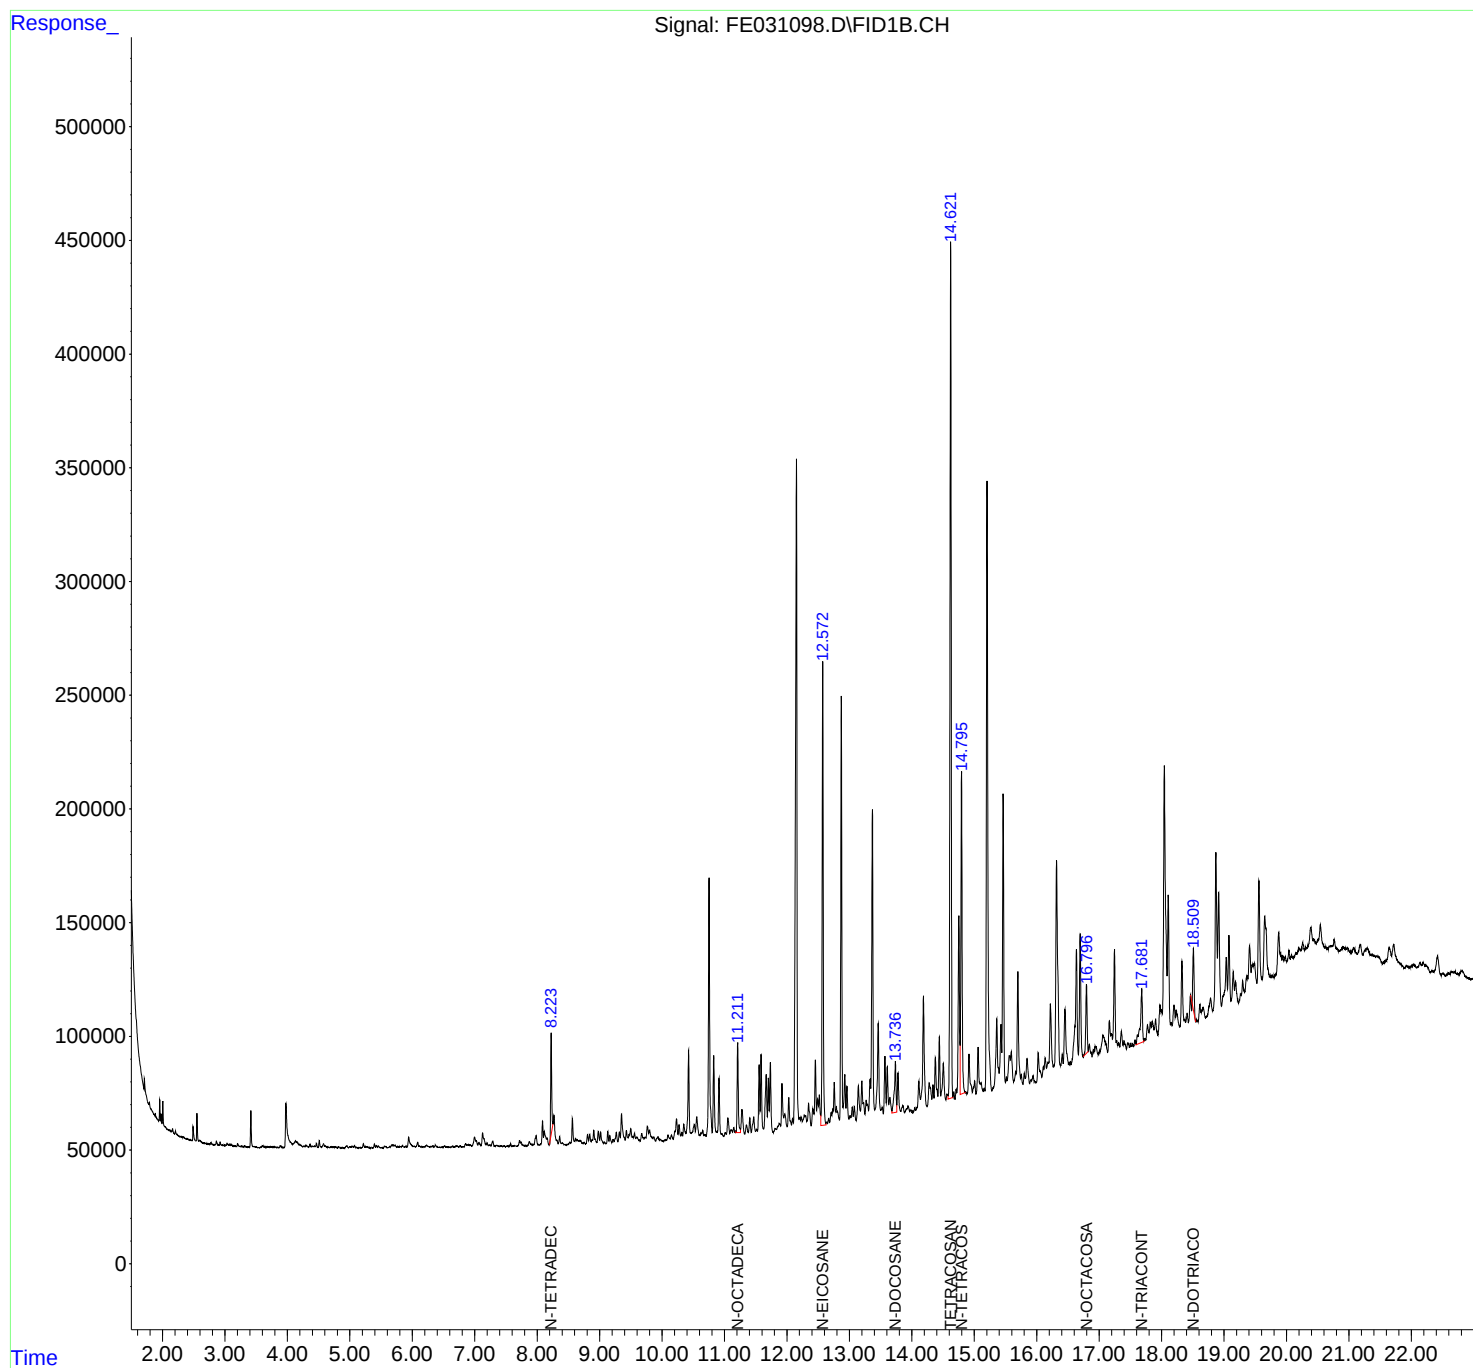


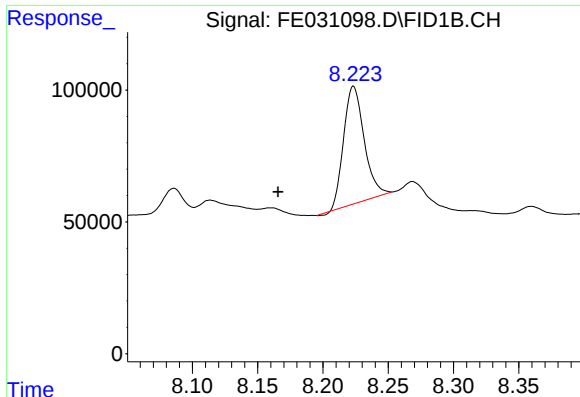

#4 N-TETRADECANE


R.T.: 8.224 min
Delta R.T.: 0.058 min
Response: 485237
Conc: 1.27 ug/ml

Instrument :
FID_E
ClientSampleId :

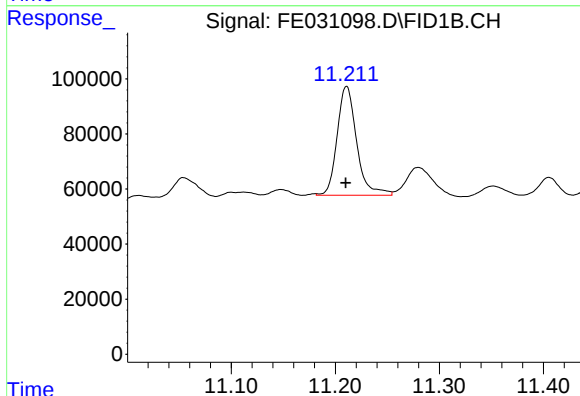


#6 N-OCTADECANE

R.T.: 11.211 min
Delta R.T.: 0.000 min
Response: 516445
Conc: 1.34 ug/ml

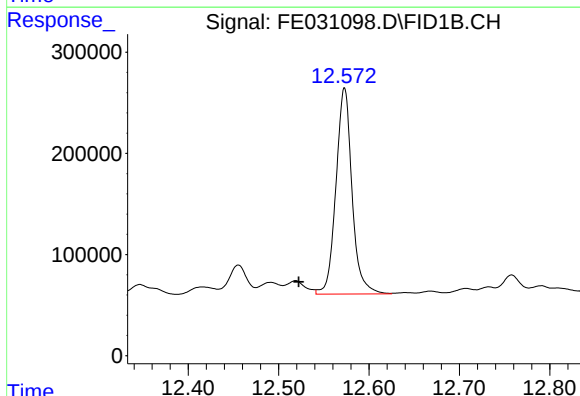


#7 N-EICOSANE

R.T.: 12.573 min
Delta R.T.: 0.051 min
Response: 2522844
Conc: 6.48 ug/ml

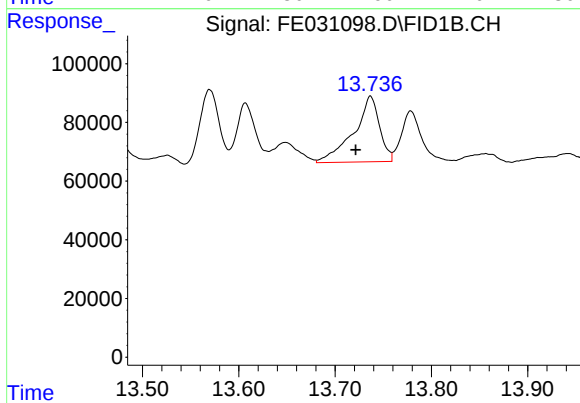

#8 N-DOCOSANE


R.T.: 13.737 min
Delta R.T.: 0.015 min
Response: 418557
Conc: 1.08 ug/ml

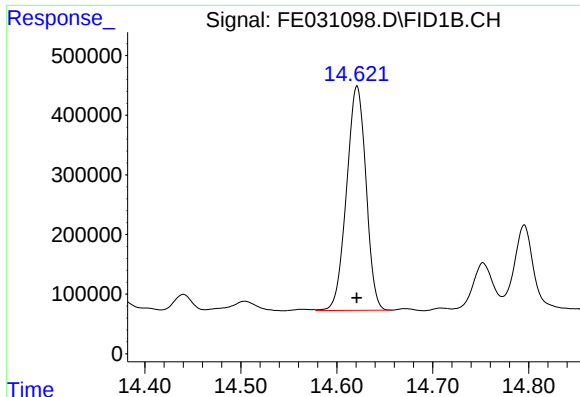

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.621 min
Delta R.T.: 0.000 min
Response: 5308701
Conc: 15.91 ug/ml

Instrument :
FID_E
ClientSampleId :

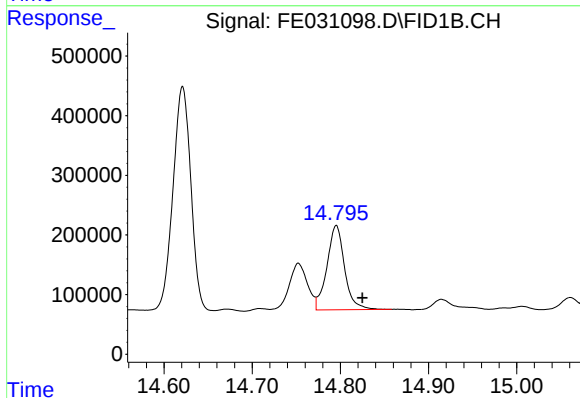


#10 N-TETRACOSANE

R.T.: 14.795 min
Delta R.T.: -0.030 min
Response: 1963488
Conc: 5.12 ug/ml

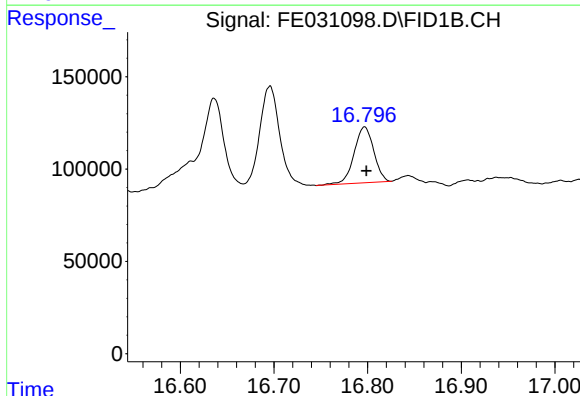


#12 N-OCTACOSANE

R.T.: 16.797 min
Delta R.T.: -0.002 min
Response: 440831
Conc: 1.15 ug/ml

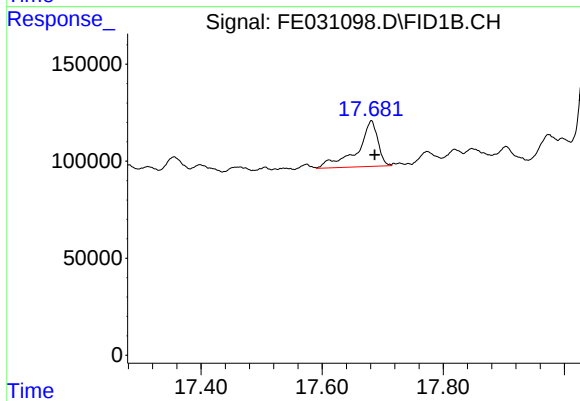

#13 N-TRIACONTANE

R.T.: 17.681 min
Delta R.T.: -0.006 min
Response: 554448
Conc: 1.45 ug/ml

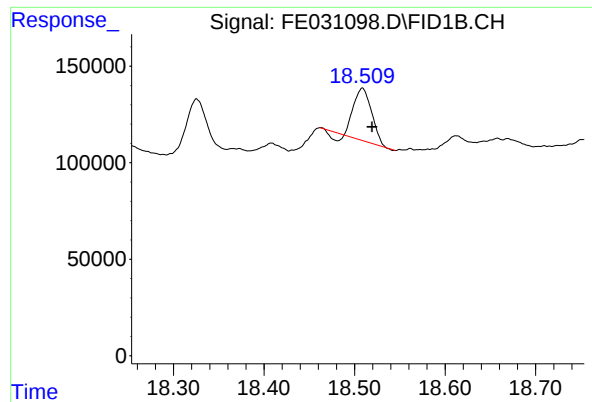

#14 N-DOTRIACONTANE

R.T.: 18.508 min
Delta R.T.: -0.011 min
Response: 347739
Conc: 0.96 ug/ml

Instrument :
FID_E
ClientSampleId :