

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
 Data File : FE031102.D
 Signal(s) : FID1B.CH
 Acq On : 13 Jan 2020 19:57
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 14 07:32:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.622	6271957	18.796 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.680	329113	0.858 ug/ml
14) N-DOTRIACONTANE	18.513	354586	0.980 ug/ml
15) N-TETRATRIACONTANE	19.298	215529	0.646 ug/ml
16) N-HEXATRIACONTANE	19.982f	57957	0.196 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
Data File : FE031102.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2020 19:57
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 14 07:32:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

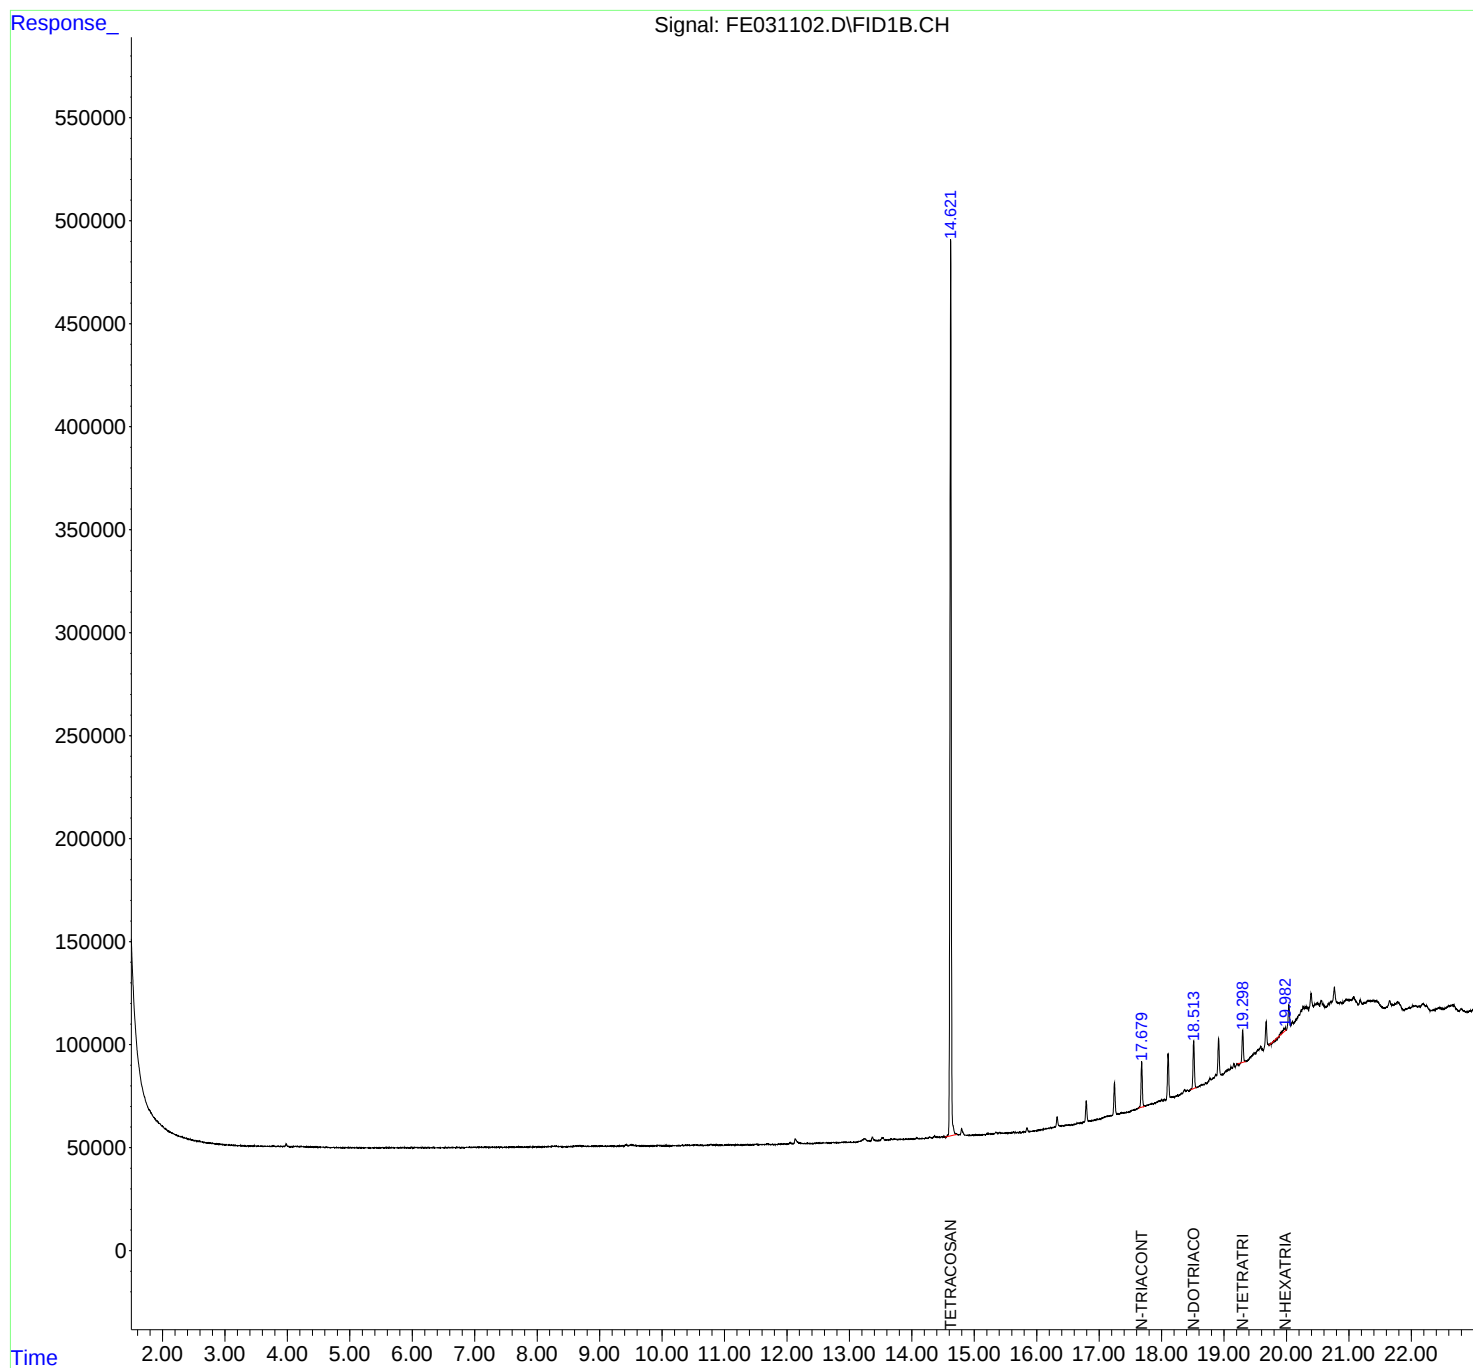


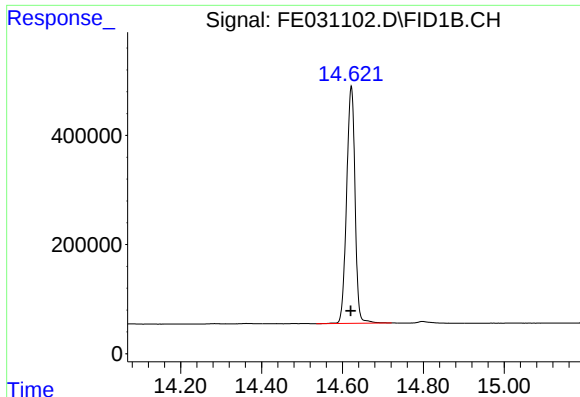

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.622 min
Delta R.T.: 0.000 min
Response: 6271957
Conc: 18.80 ug/ml

Instrument :
FID_E
ClientSampleId :

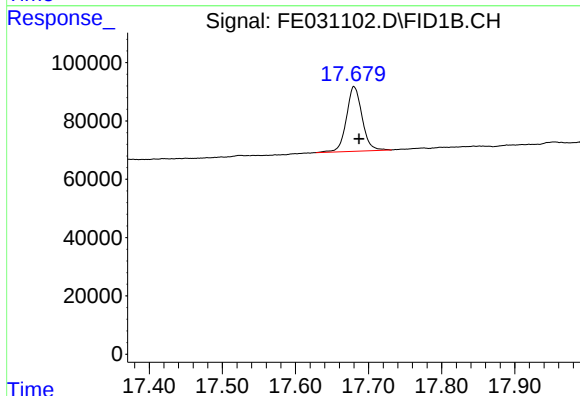


#13 N-TRIACONTANE

R.T.: 17.680 min
Delta R.T.: -0.007 min
Response: 329113
Conc: 0.86 ug/ml

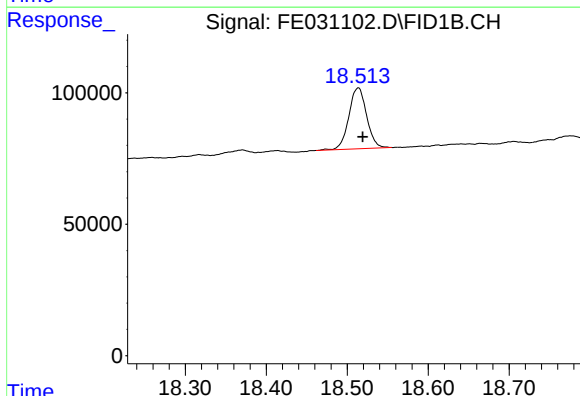


#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: -0.006 min
Response: 354586
Conc: 0.98 ug/ml

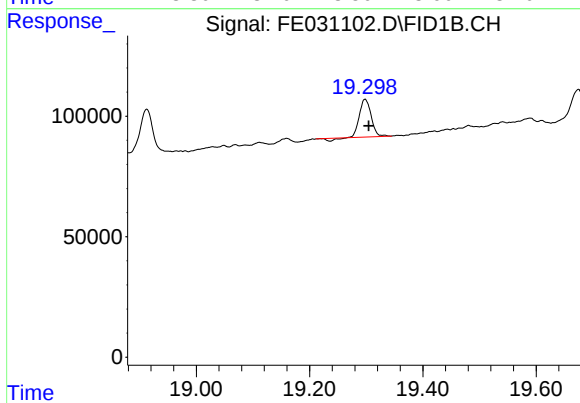

#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.006 min
Response: 215529
Conc: 0.65 ug/ml

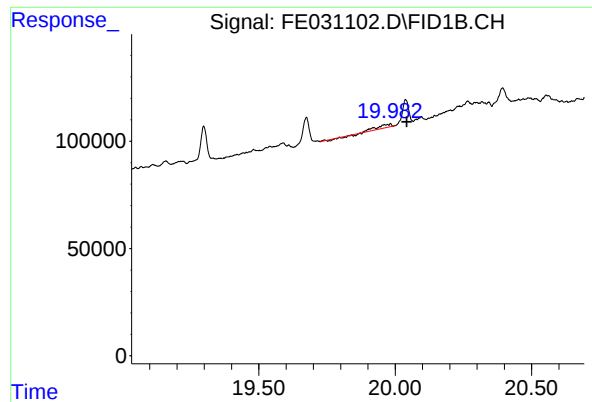

#16 N-HEXATRIACONTANE

R.T.: 19.982 min
Delta R.T.: -0.060 min
Response: 57957
Conc: 0.20 ug/ml

Instrument :
FID_E
ClientSampleId :