

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
 Data File : FE031109.D
 Signal(s) : FID1B.CH
 Acq On : 13 Jan 2020 23:47
 Operator : DD\AJ
 Sample : L1106-02 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 14 07:32:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.619	1075277	3.222 ug/ml
Target Compounds			
4) N-TETRADECANE	8.112f	297448	0.778 ug/ml
5) N-HEXADECANE	9.772	489938	1.266 ug/ml
7) N-EICOSANE	12.497	323849	0.832 ug/ml
8) N-DOCOSANE	13.736	1429046	3.700 ug/ml
10) N-TETRACOSANE	14.800	5543500	14.453 ug/ml
11) N-HEXACOSANE	15.839	471723	1.233 ug/ml
12) N-OCTACOSANE	16.796	1525383	3.968 ug/ml
13) N-TRIACONTANE	17.686	638144	1.665 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
Data File : FE031109.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2020 23:47
Operator : DD\AJ
Sample : L1106-02 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 14 07:32:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

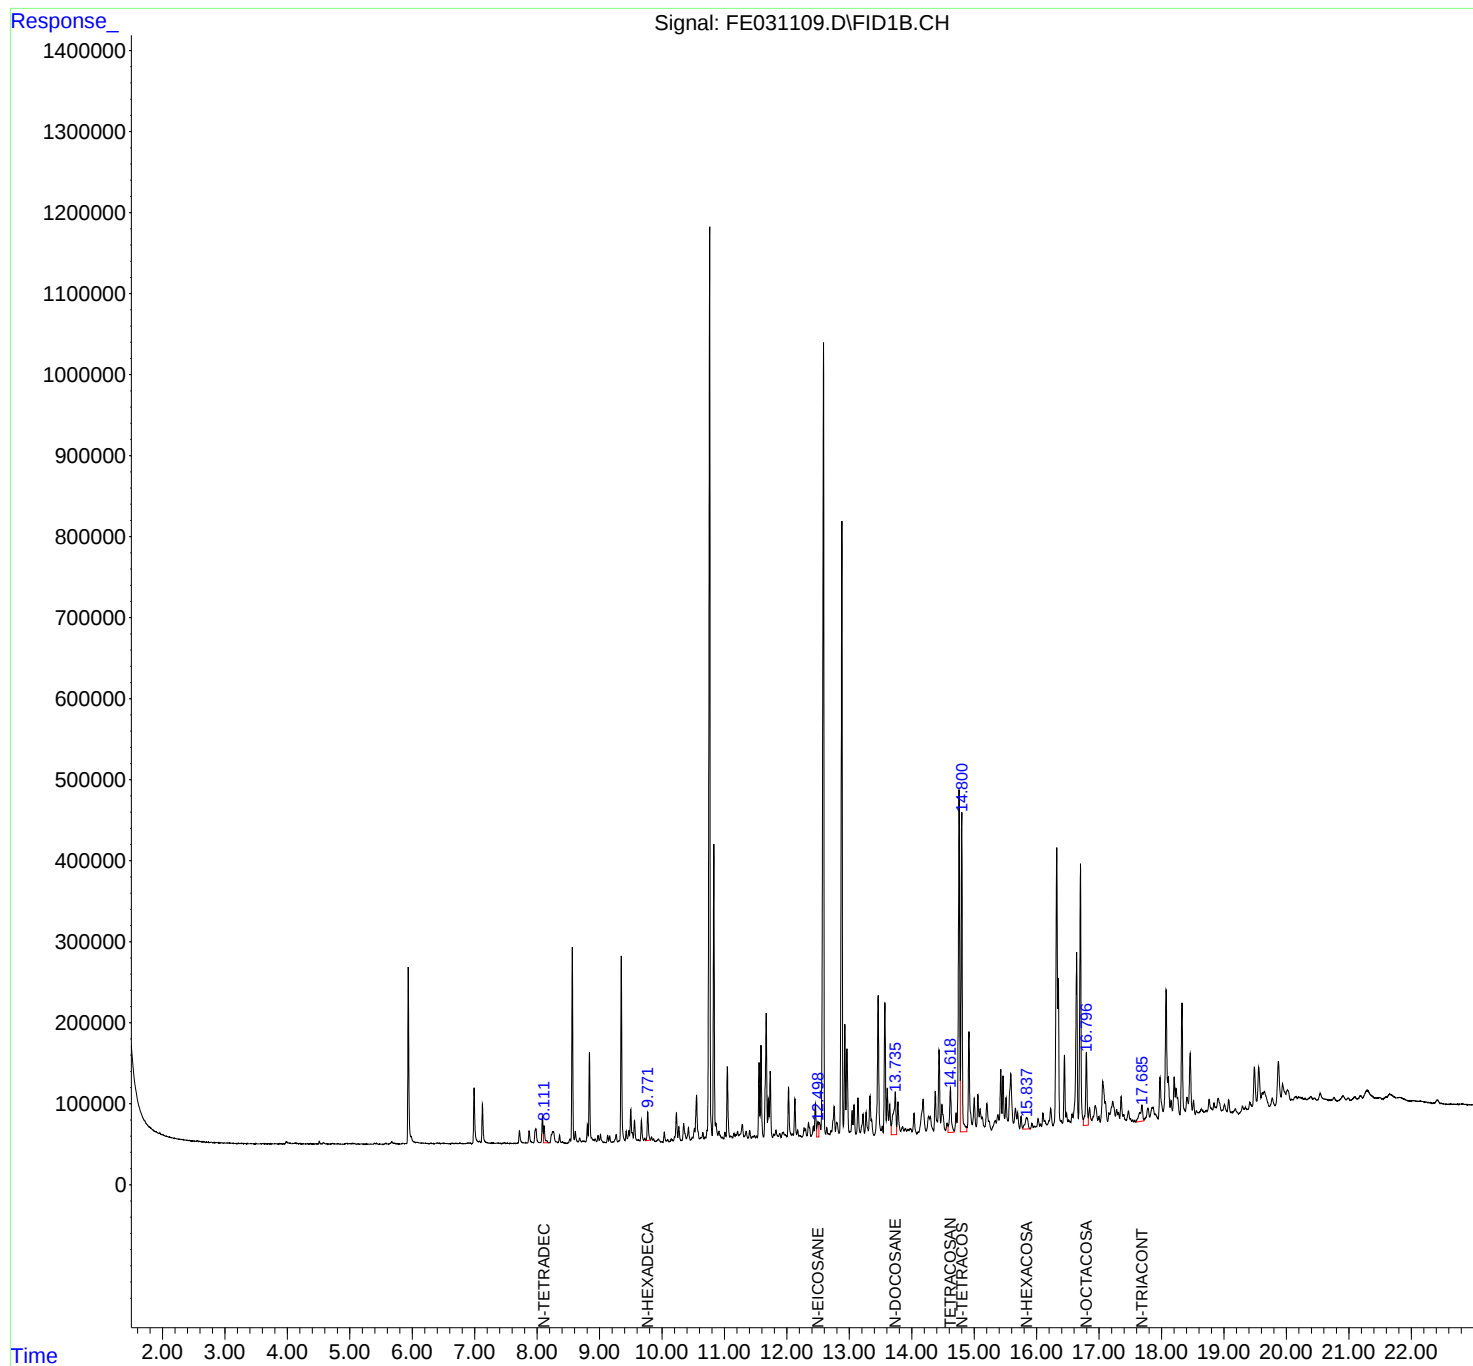


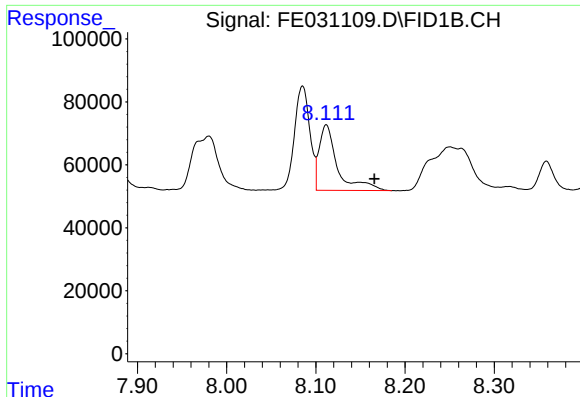

#4 N-TETRADECANE


R.T.: 8.112 min
Delta R.T.: -0.054 min
Response: 297448
Conc: 0.78 ug/ml

Instrument :
FID_E
ClientSampleId :

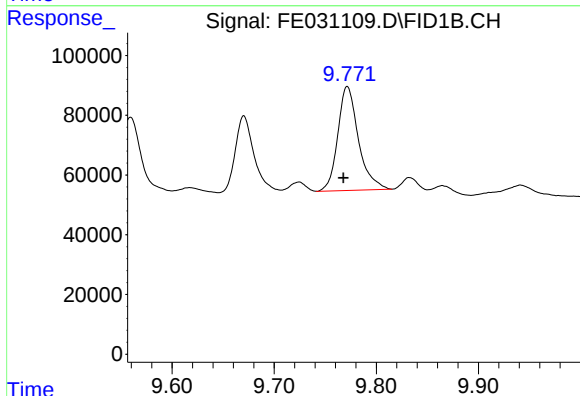


#5 N-HEXADECANE

R.T.: 9.772 min
Delta R.T.: 0.004 min
Response: 489938
Conc: 1.27 ug/ml

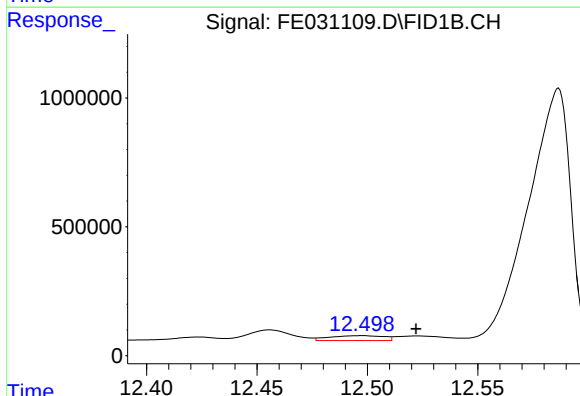


#7 N-EICOSANE

R.T.: 12.497 min
Delta R.T.: -0.025 min
Response: 323849
Conc: 0.83 ug/ml

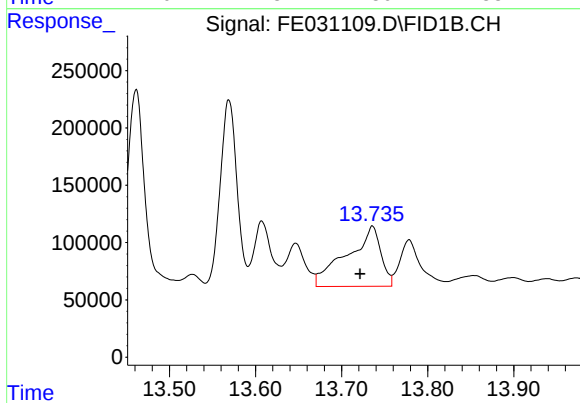

#8 N-DOCOSANE


R.T.: 13.736 min
Delta R.T.: 0.014 min
Response: 1429046
Conc: 3.70 ug/ml

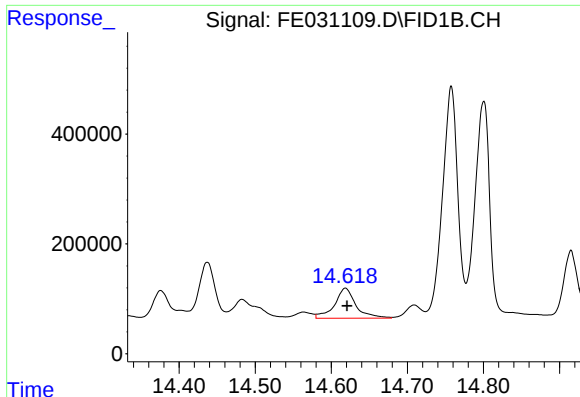

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.619 min
Delta R.T.: -0.002 min
Response: 1075277
Conc: 3.22 ug/ml

Instrument :
FID_E
ClientSampleId :

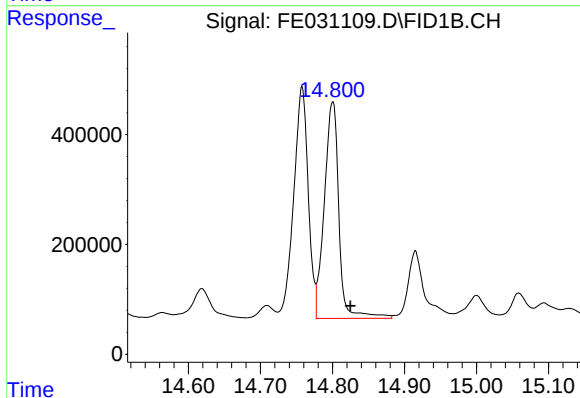


#10 N-TETRACOSANE

R.T.: 14.800 min
Delta R.T.: -0.025 min
Response: 5543500
Conc: 14.45 ug/ml

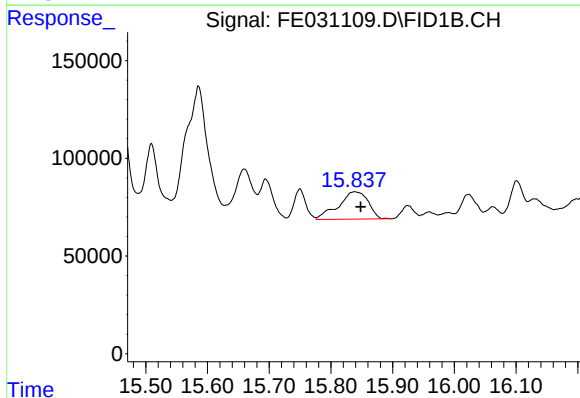


#11 N-HEXACOSANE

R.T.: 15.839 min
Delta R.T.: -0.009 min
Response: 471723
Conc: 1.23 ug/ml

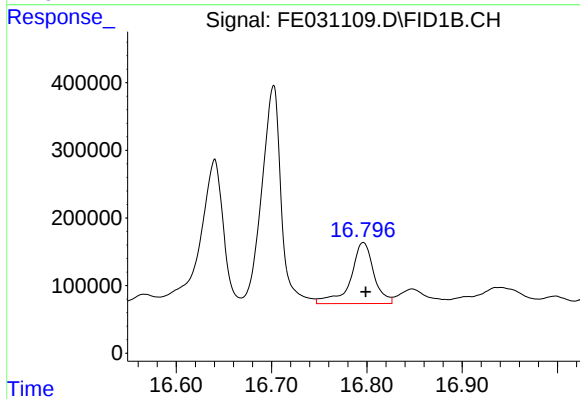

#12 N-OCTACOSANE

R.T.: 16.796 min
Delta R.T.: -0.003 min
Response: 1525383
Conc: 3.97 ug/ml

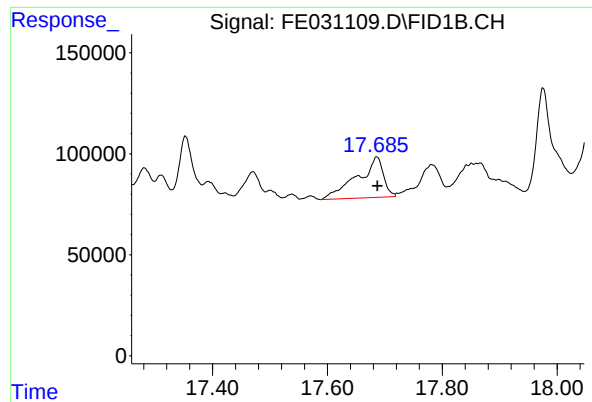

#13 N-TRIACONTANE

R.T.: 17.686 min
Delta R.T.: 0.000 min
Response: 638144
Conc: 1.66 ug/ml

Instrument :
FID_E
ClientSampleId :