

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
 Data File : FE031111.D
 Signal(s) : FID1B.CH
 Acq On : 14 Jan 2020 00:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 14 07:33:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.620	6381055	19.123 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.680	379323	0.989 ug/ml
14) N-DOTRIACONTANE	18.513	420771	1.163 ug/ml
15) N-TETRATRIACONTANE	19.296	273849	0.821 ug/ml
16) N-HEXATRIACONTANE	20.037	183198	0.619 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
Data File : FE031111.D
Signal(s) : FID1B.CH
Acq On : 14 Jan 2020 00:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 14 07:33:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

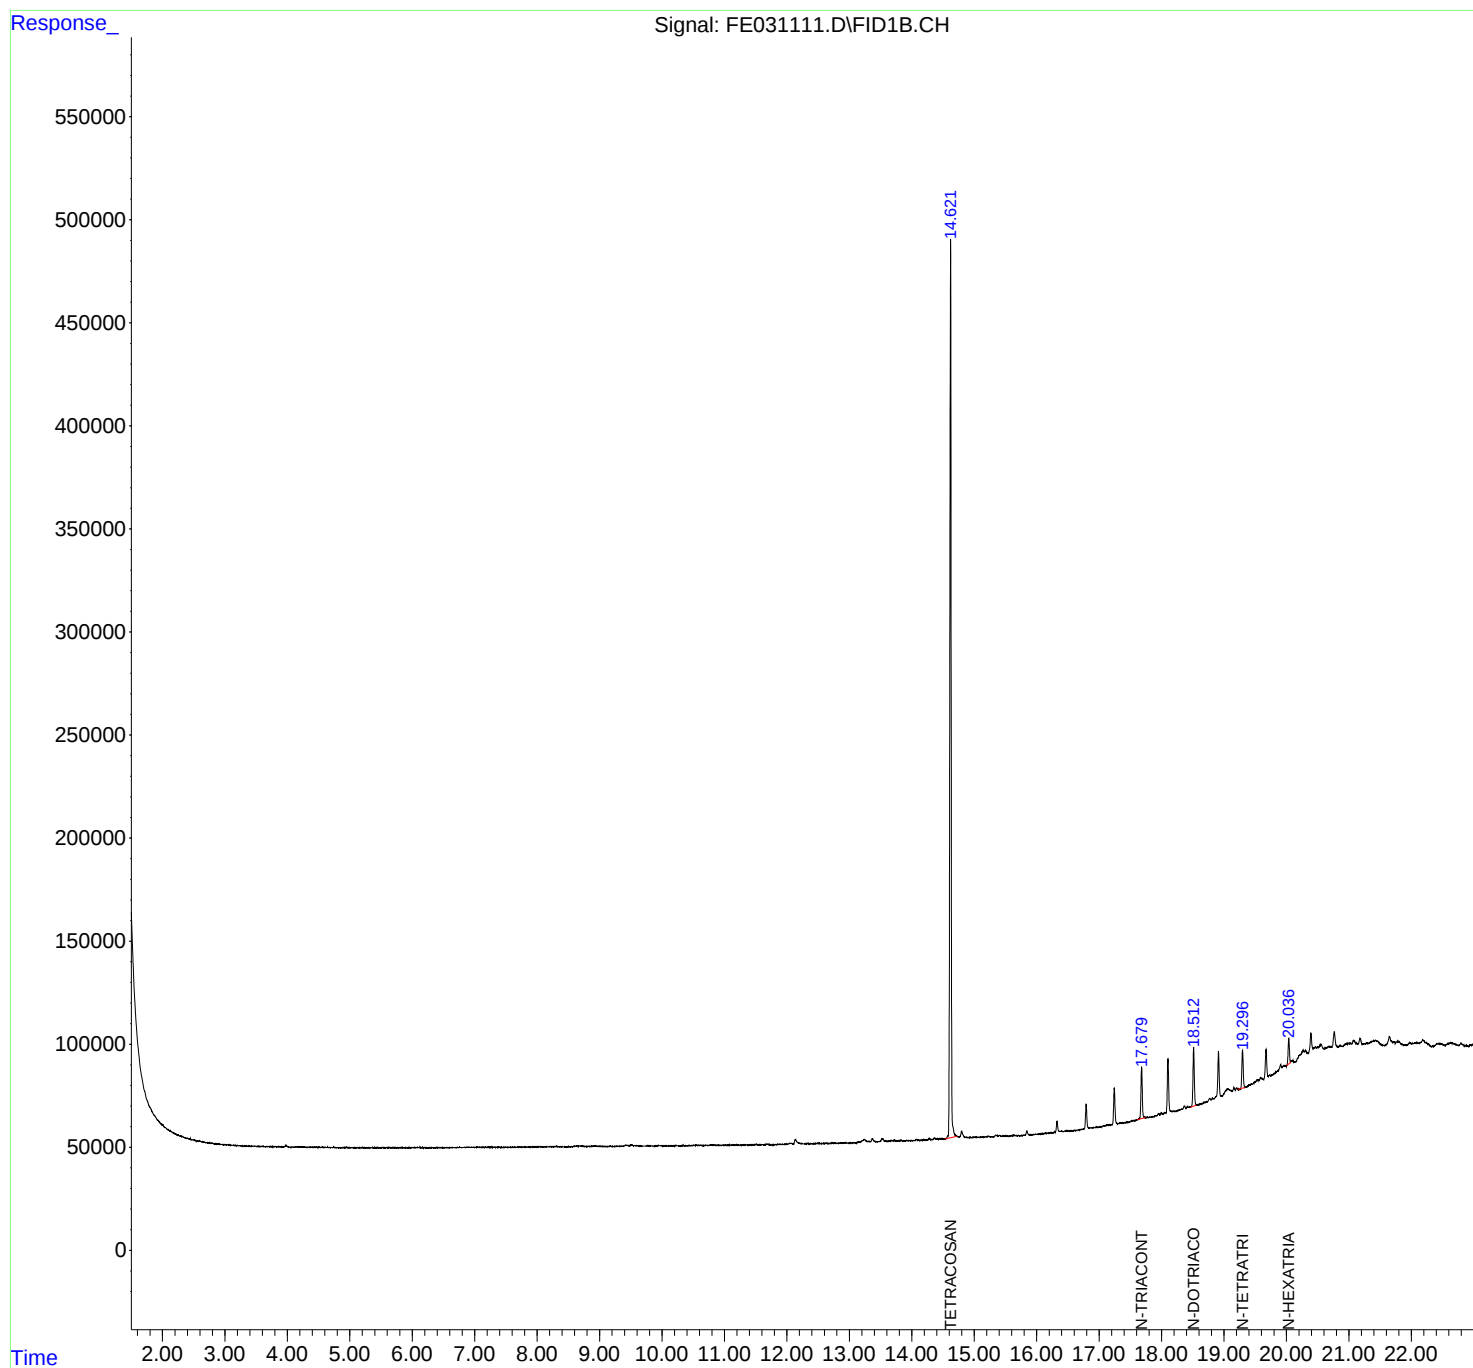


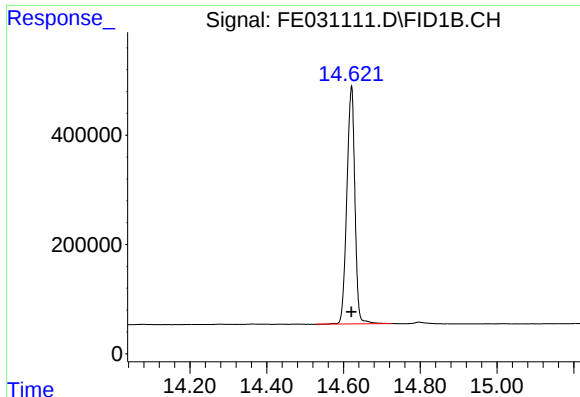

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.620 min
Delta R.T.: 0.000 min
Response: 6381055
Conc: 19.12 ug/ml

Instrument :
FID_E
ClientSampleId :

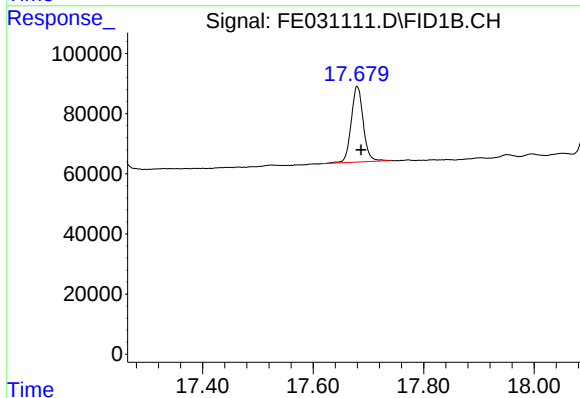


#13 N-TRIACONTANE

R.T.: 17.680 min
Delta R.T.: -0.007 min
Response: 379323
Conc: 0.99 ug/ml

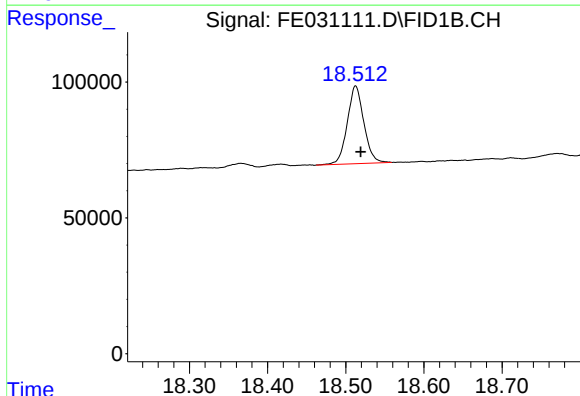


#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: -0.007 min
Response: 420771
Conc: 1.16 ug/ml

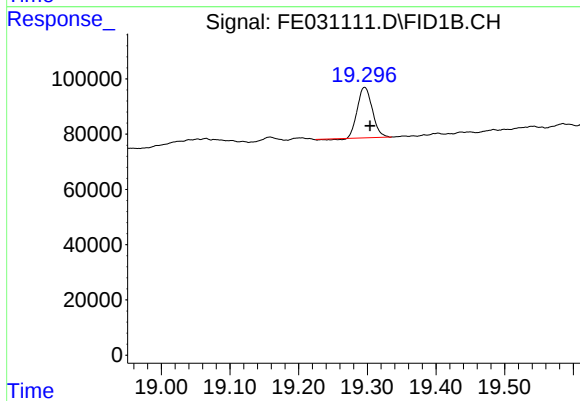

#15 N-TETRATRIACONTANE

R.T.: 19.296 min
Delta R.T.: -0.008 min
Response: 273849
Conc: 0.82 ug/ml

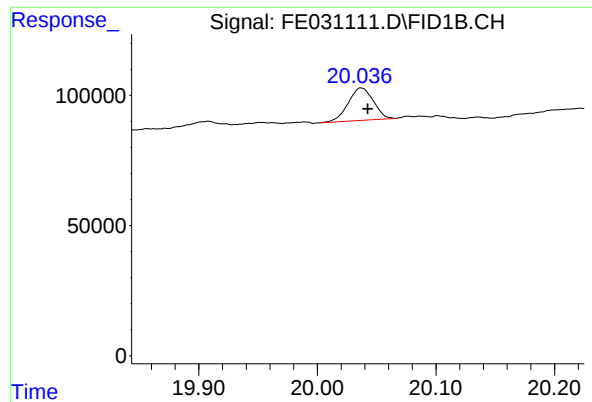

#16 N-HEXATRIACONTANE

R.T.: 20.037 min
Delta R.T.: -0.005 min
Response: 183198
Conc: 0.62 ug/ml

Instrument :
FID_E
ClientSampleId :