

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
Data File : FE031109.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2020 23:47
Operator : DD\AJ
Sample : L1106-02 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
CIY1-BC-SB-04-0-5

Manual Integrations
APPROVED

Ankita
1/14/2020 10:31:15 AM

Integration File: autoint1.e
Quant Time: Jan 14 07:32:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.618	963893	2.889 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011320\
Data File : FE031109.D
Signal(s) : FID1B.CH
Acq On : 13 Jan 2020 23:47
Operator : DD\AJ
Sample : L1106-02 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
CIY1-BC-SB-04-0-5


Manual Integrations
APPROVED

Ankita
1/14/2020 10:31:15 AM

Integration File: autoint1.e
Quant Time: Jan 14 07:32:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

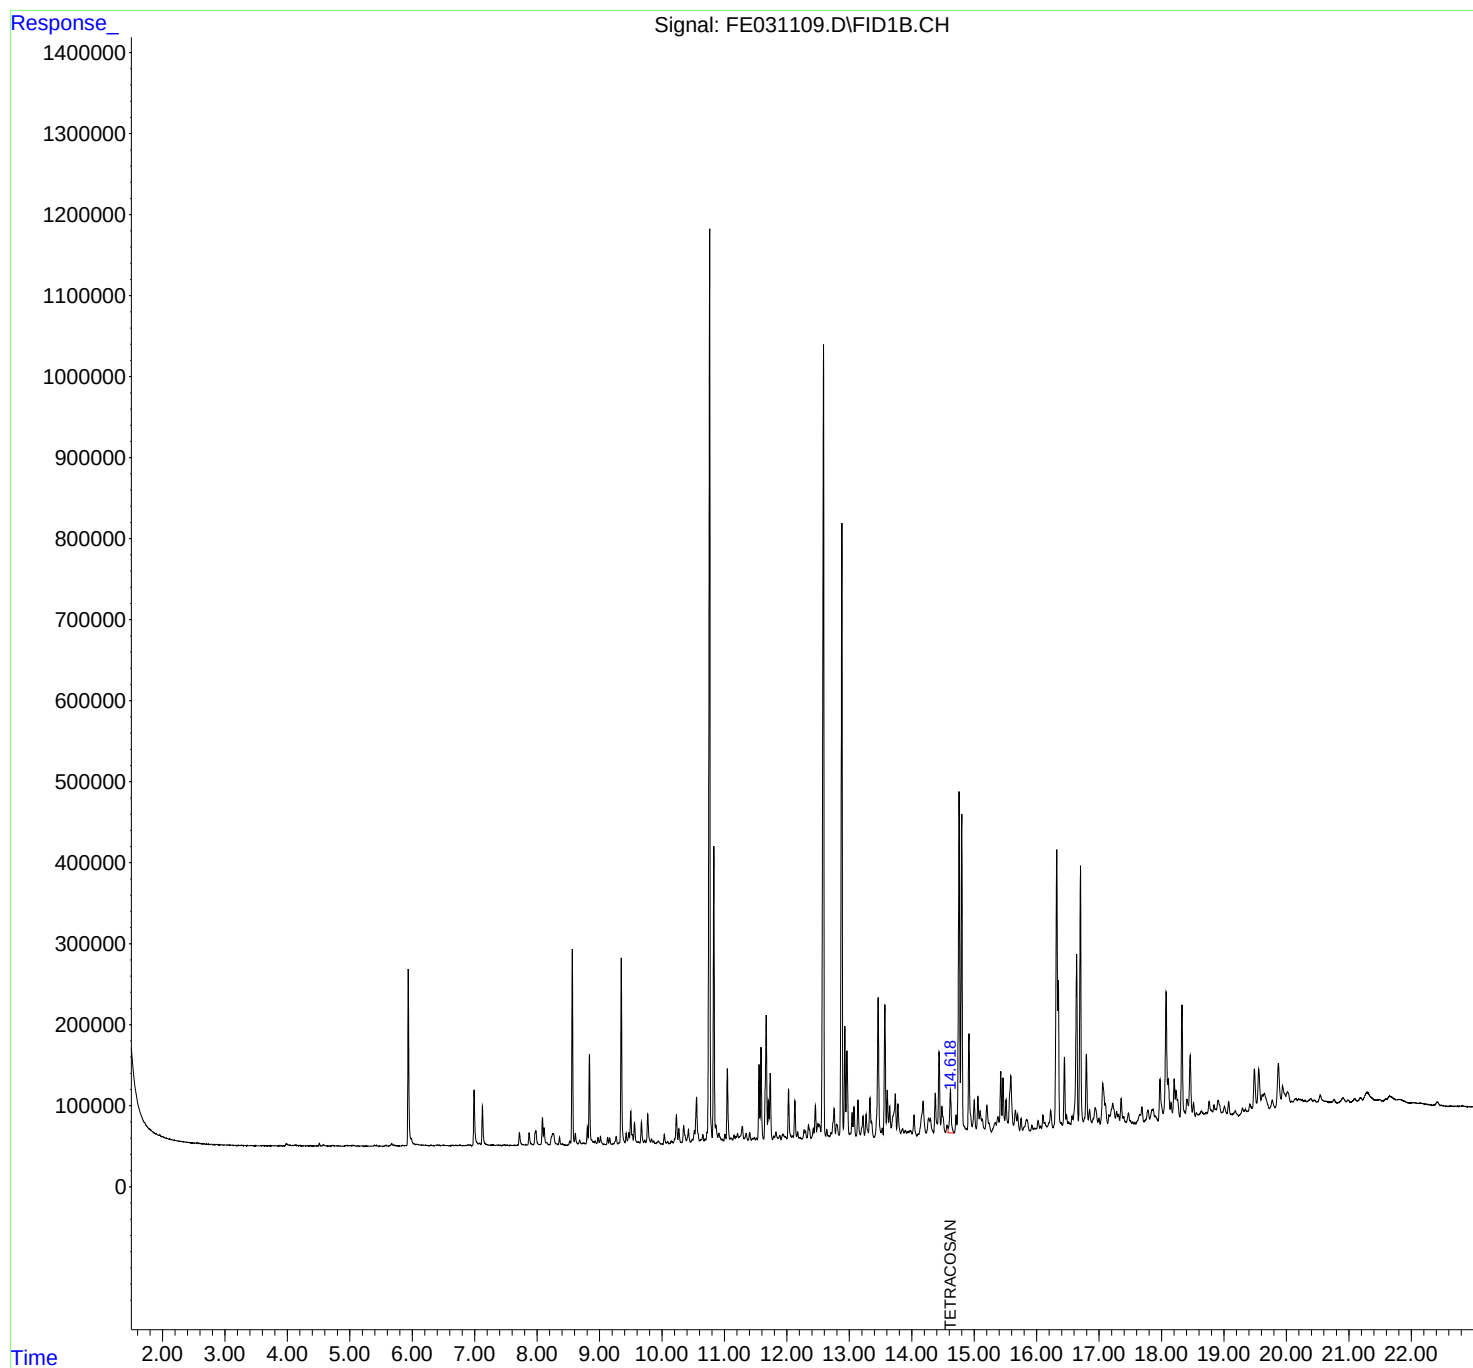

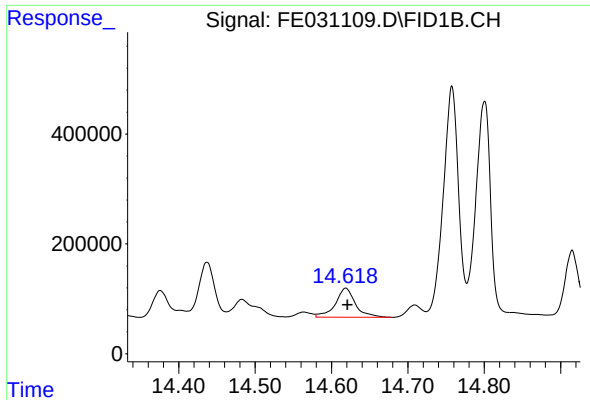

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.618 min
Delta R.T.: -0.003 min
Response: 963893
Conc: 2.89 ug/ml m

Instrument :
FID_E
ClientSampleId :
CIY1-BC-SB-04-0-5

Manual Integrations
APPROVED

Ankita
1/14/2020 10:31:15 AM