

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011420\
 Data File : FE031117.D
 Signal(s) : FID1B.CH
 Acq On : 14 Jan 2020 11:40
 Operator : DD\AJ
 Sample : L1106-08 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 14 22:01:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.617	2613122	7.831 ug/ml
Target Compounds			
4) N-TETRADECANE	8.222f	110630	0.289 ug/ml
5) N-HEXADECANE	9.771	296459	0.766 ug/ml
7) N-EICOSANE	12.492	269982	0.694 ug/ml
8) N-DOCOSANE	13.735	1044608	2.705 ug/ml
10) N-TETRACOSANE	14.797	4028370	10.503 ug/ml
11) N-HEXACOSANE	15.841	448683	1.173 ug/ml
12) N-OCTACOSANE	16.796	1229462	3.198 ug/ml
13) N-TRIACONTANE	17.682	761613	1.987 ug/ml
15) N-TETRATRIACONTANE	19.297	92968	0.279 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011420\
Data File : FE031117.D
Signal(s) : FID1B.CH
Acq On : 14 Jan 2020 11:40
Operator : DD\AJ
Sample : L1106-08 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 14 22:01:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

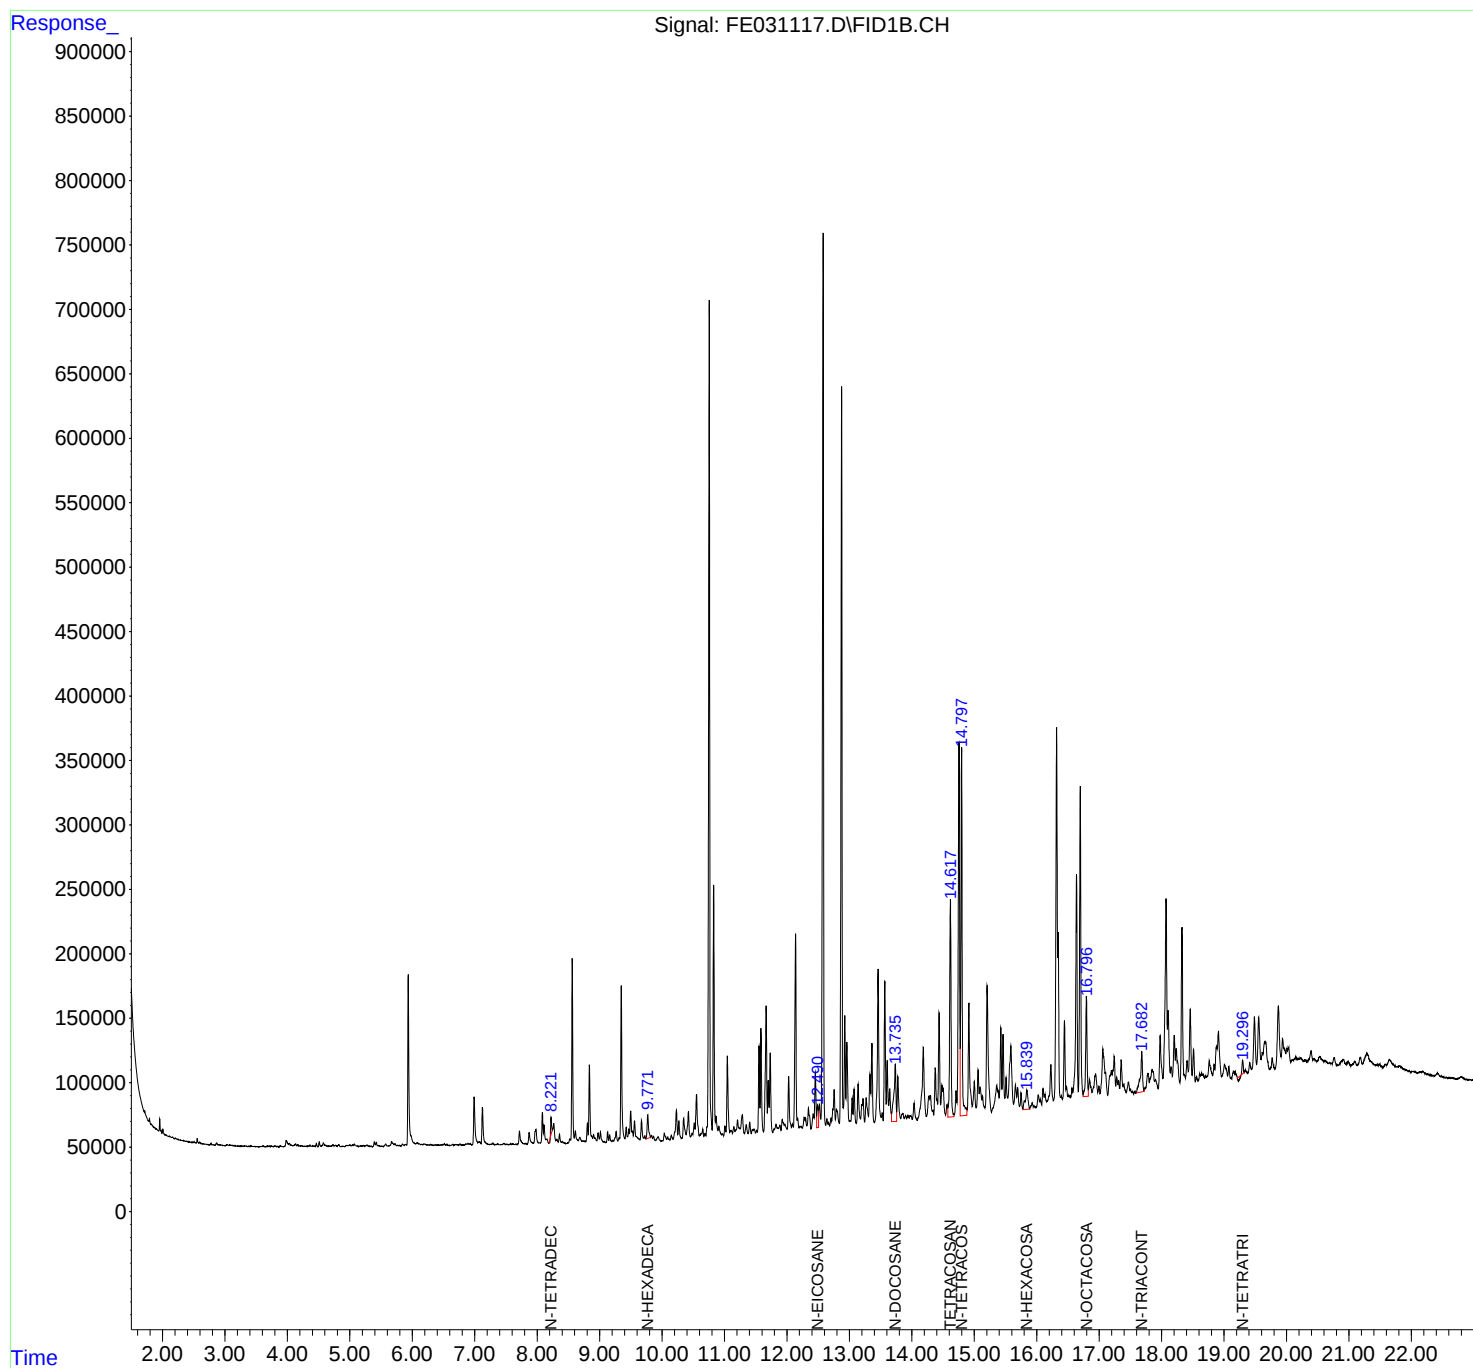

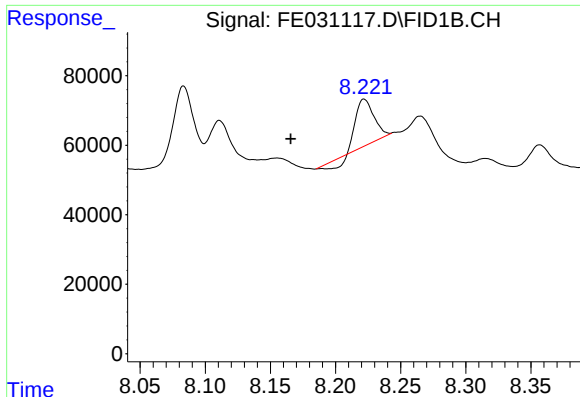


#4 N-TETRADECANE

R.T.: 8.222 min
Delta R.T.: 0.057 min
Response: 110630
Conc: 0.29 ug/ml

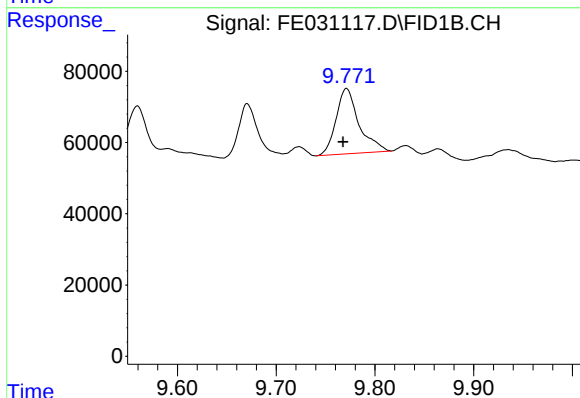


#5 N-HEXADECANE

R.T.: 9.771 min
Delta R.T.: 0.004 min
Response: 296459
Conc: 0.77 ug/ml

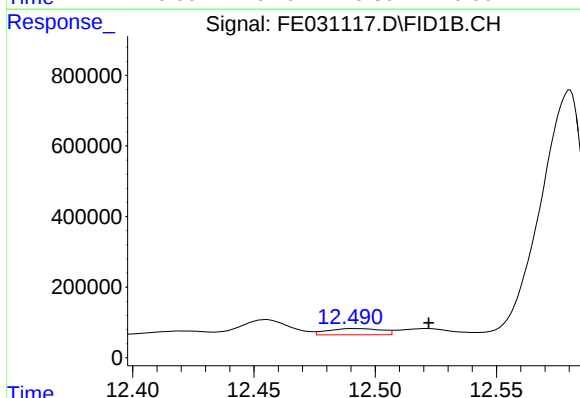


#7 N-EICOSANE

R.T.: 12.492 min
Delta R.T.: -0.030 min
Response: 269982
Conc: 0.69 ug/ml

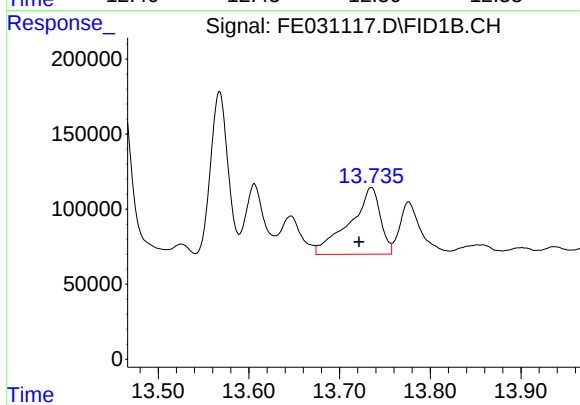


#8 N-DOCOSANE

R.T.: 13.735 min
Delta R.T.: 0.013 min
Response: 1044608
Conc: 2.70 ug/ml

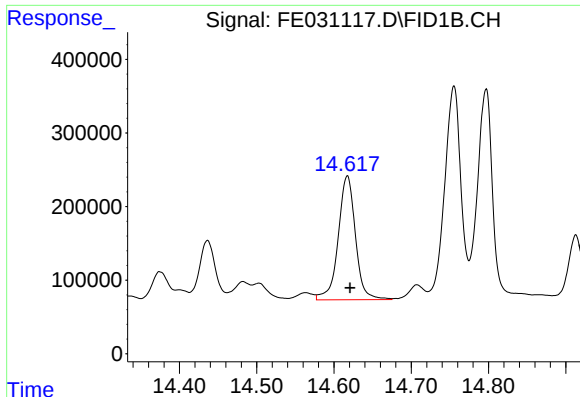


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.617 min
Delta R.T.: -0.004 min
Response: 2613122
Conc: 7.83 ug/ml

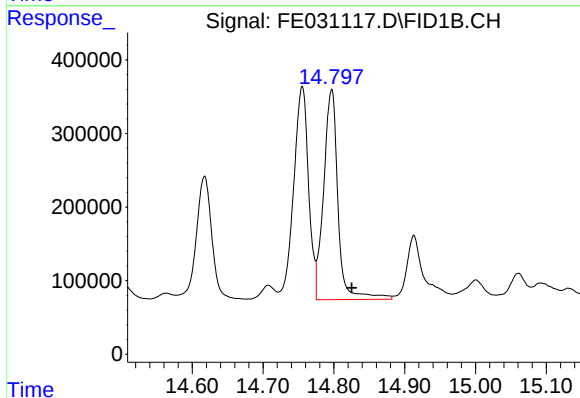


#10 N-TETRACOSANE

R.T.: 14.797 min
Delta R.T.: -0.029 min
Response: 4028370
Conc: 10.50 ug/ml

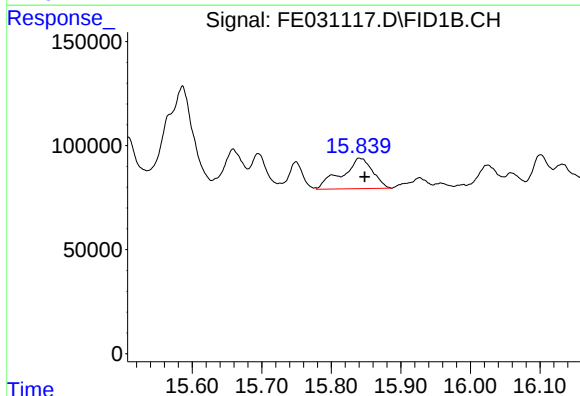


#11 N-HEXACOSANE

R.T.: 15.841 min
Delta R.T.: -0.007 min
Response: 448683
Conc: 1.17 ug/ml

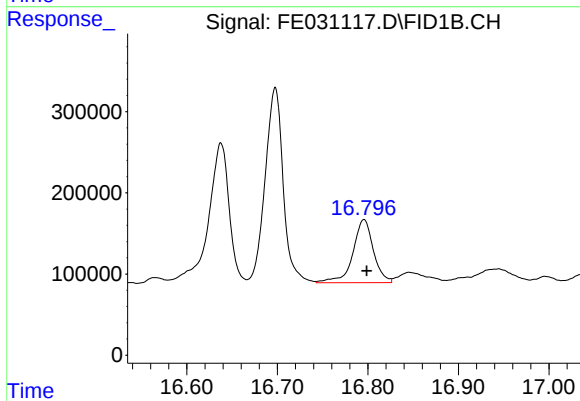


#12 N-OCTACOSANE

R.T.: 16.796 min
Delta R.T.: -0.003 min
Response: 1229462
Conc: 3.20 ug/ml

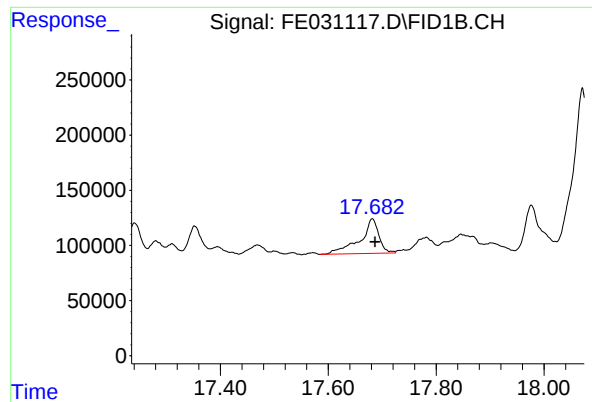

#13 N-TRIACONTANE

R.T.: 17.682 min
Delta R.T.: -0.005 min
Response: 761613
Conc: 1.99 ug/ml

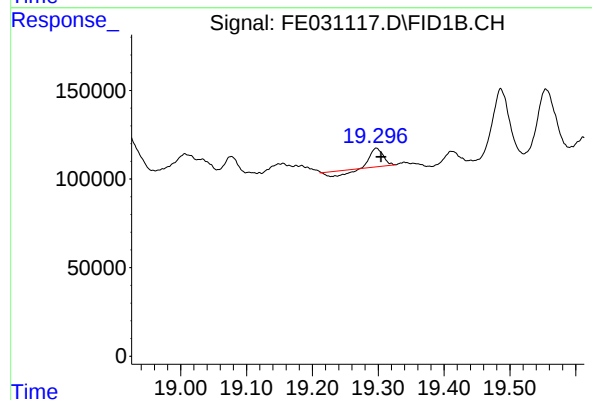

#15 N-TETRATRIACONTANE

R.T.: 19.297 min
Delta R.T.: -0.007 min
Response: 92968
Conc: 0.28 ug/ml