

Data Path : P:\HPCHEM1\FID E\Data\FE011518\
 Data File : FE025596.D
 Signal(s) : FID1B.CH
 Acq On : 15 Jan 2018 12:56
 Operator : UA/AJ
 Sample : J1015-05 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 00:19:05 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.882	349509	1.922 ug/ml
Target Compounds			
7) N-EICOSANE	12.726	243264	1.097 ug/ml
8) N-DOCOSANE	13.895f	352814	1.608 ug/ml
10) N-TETRACOSANE	15.084	1741979	8.168 ug/ml
12) N-OCTACOSANE	17.015	1939658	11.537 ug/ml
13) N-TRIACONTANE	17.900	567630	3.595 ug/ml
14) N-DOTRIACONTANE	18.734	524902	3.236 ug/ml
15) N-TETRATRIACONTANE	19.517	188171	1.211 ug/ml
16) N-HEXATRIACONTANE	20.258	301567	2.269 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011518\
Data File : FE025596.D
Signal(s) : FID1B.CH
Acq On : 15 Jan 2018 12:56
Operator : UA/AJ
Sample : J1015-05 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 00:19:05 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

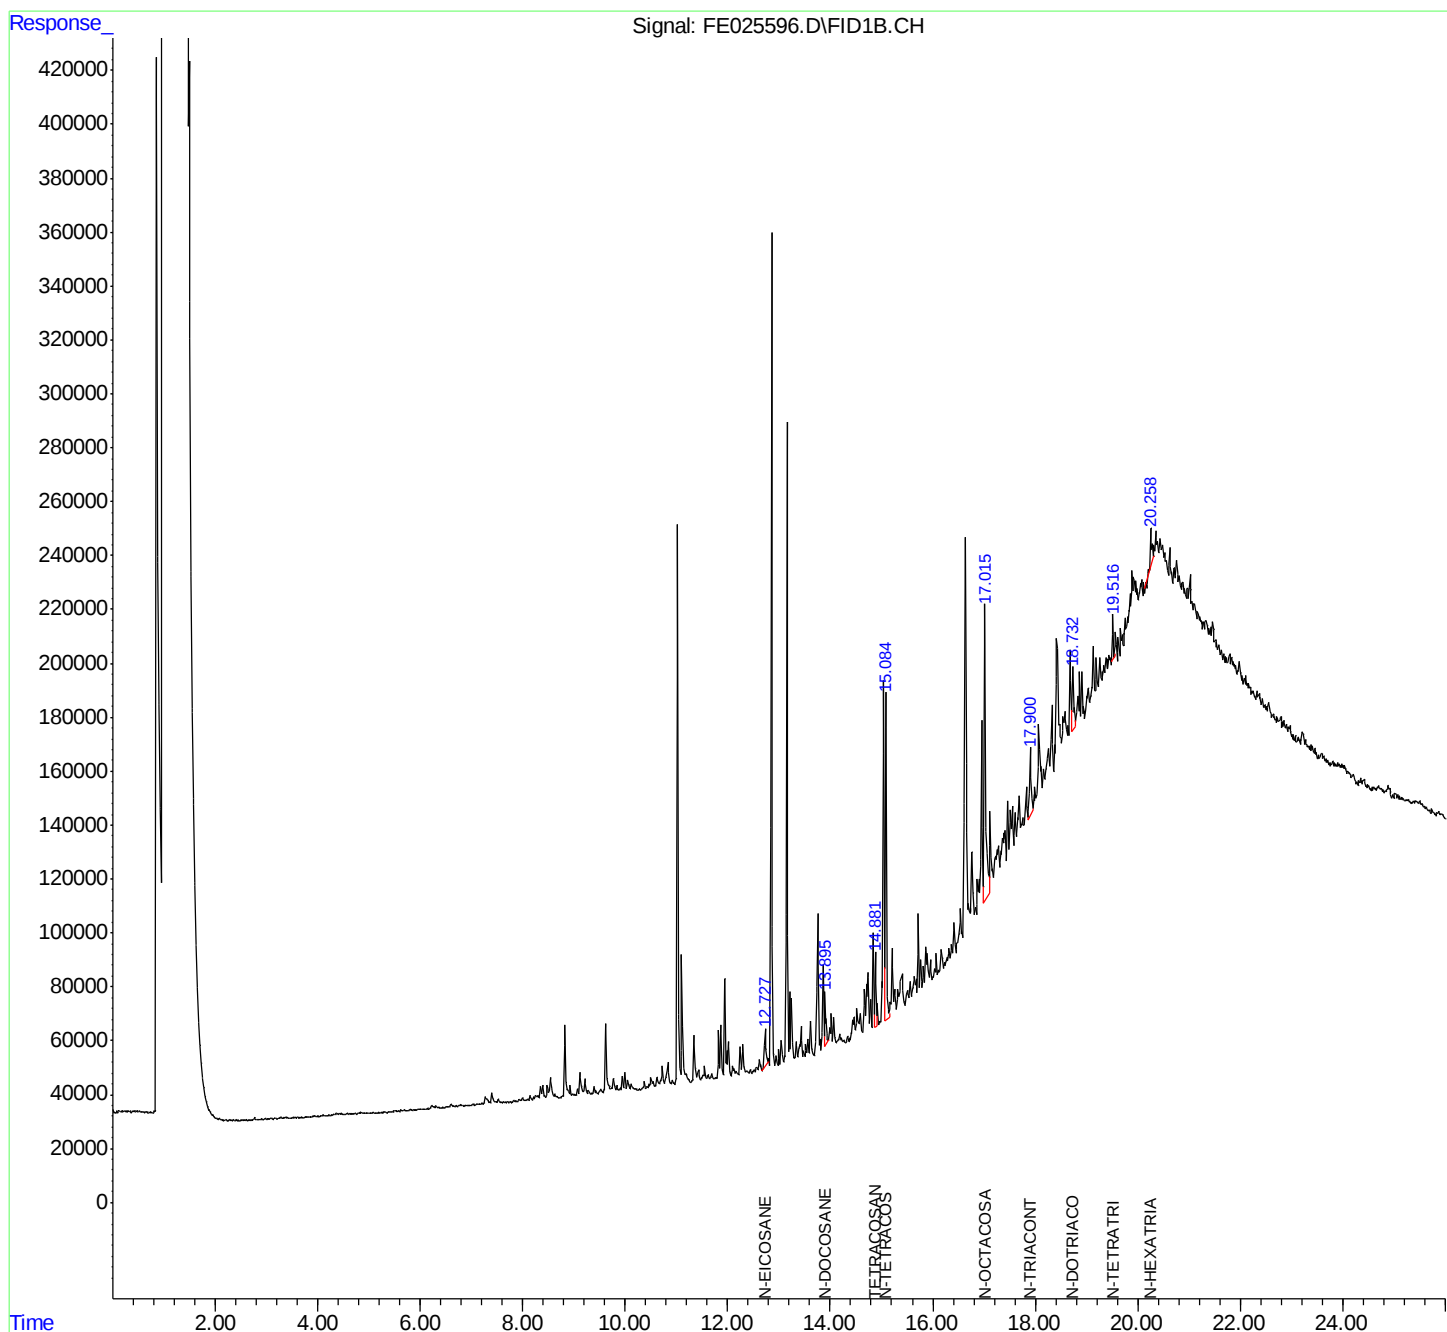


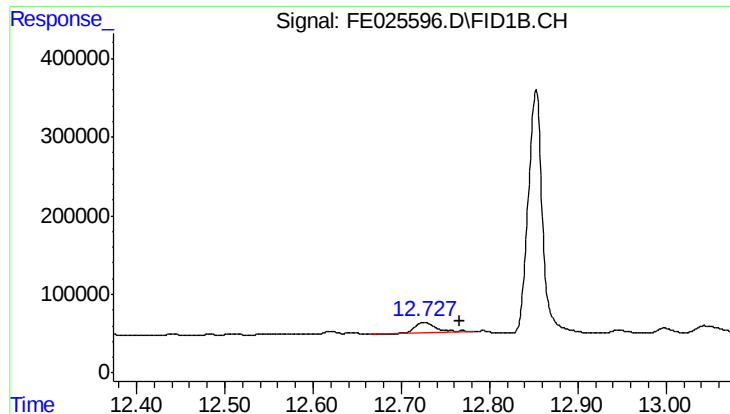

#7 N-EICOSANE


R.T.: 12.726 min
Delta R.T.: -0.040 min
Response: 243264
Conc: 1.10 ug/ml

Instrument :
FID_E
ClientSampleId :

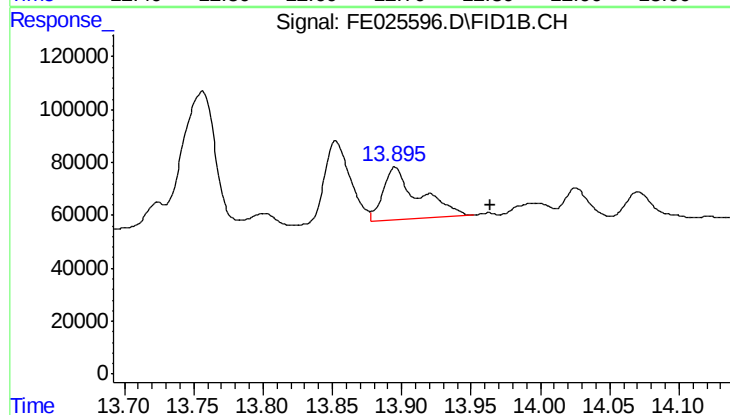


#8 N-DOCOSANE

R.T.: 13.895 min
Delta R.T.: -0.069 min
Response: 352814
Conc: 1.61 ug/ml

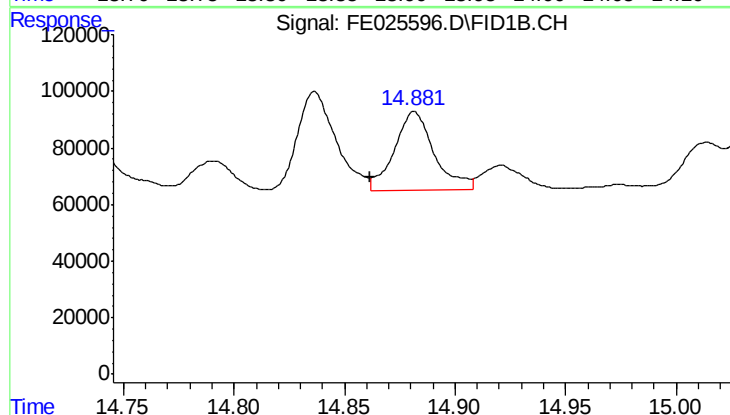


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.882 min
Delta R.T.: 0.020 min
Response: 349509
Conc: 1.92 ug/ml

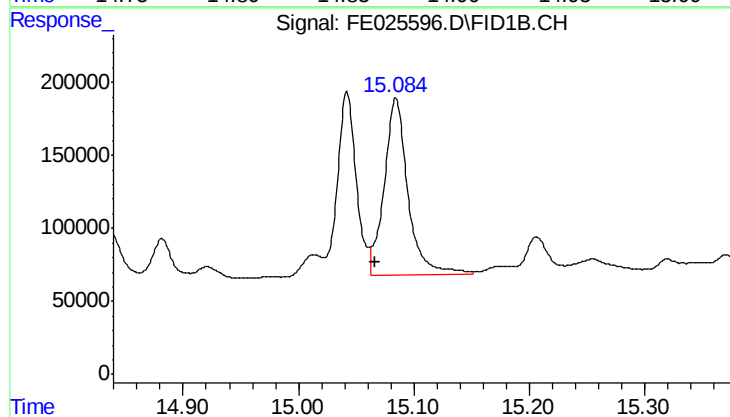

#10 N-TETRACOSANE


R.T.: 15.084 min
Delta R.T.: 0.018 min
Response: 1741979
Conc: 8.17 ug/ml

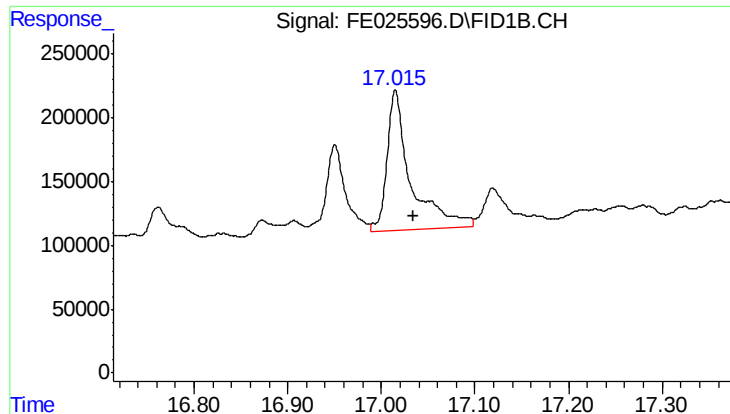

#12 N-OCTACOSANE


R.T.: 17.015 min
Delta R.T.: -0.019 min
Response: 1939658
Conc: 11.54 ug/ml

Instrument :
FID_E
ClientSampleId :

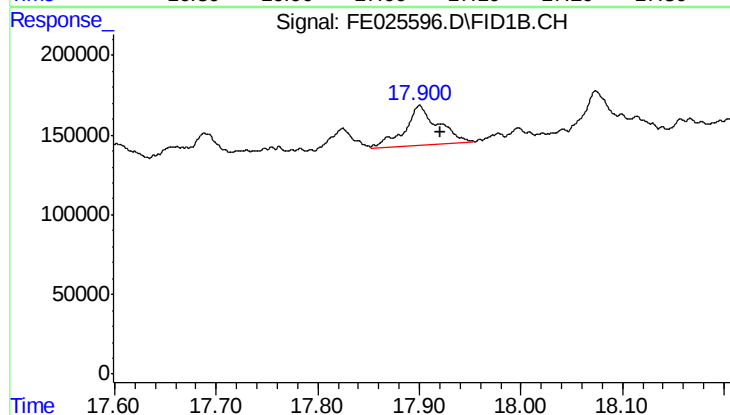


#13 N-TRIACONTANE

R.T.: 17.900 min
Delta R.T.: -0.021 min
Response: 567630
Conc: 3.59 ug/ml

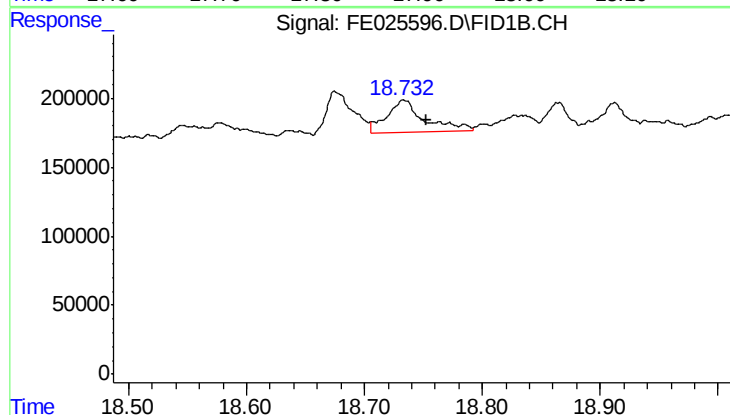


#14 N-DOTRIACONTANE

R.T.: 18.734 min
Delta R.T.: -0.019 min
Response: 524902
Conc: 3.24 ug/ml

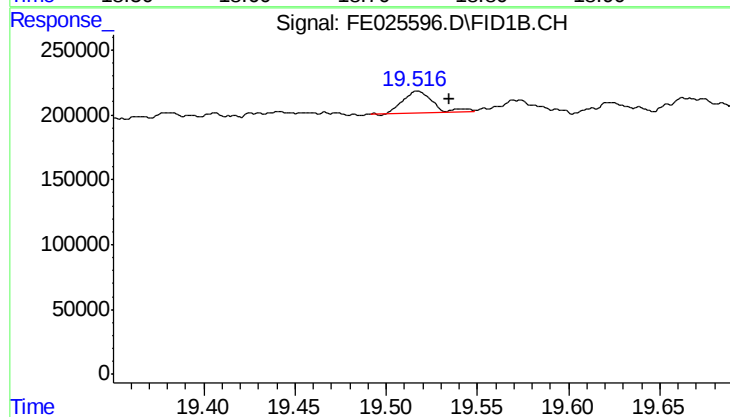

#15 N-TETRATRIACONTANE

R.T.: 19.517 min
Delta R.T.: -0.017 min
Response: 188171
Conc: 1.21 ug/ml

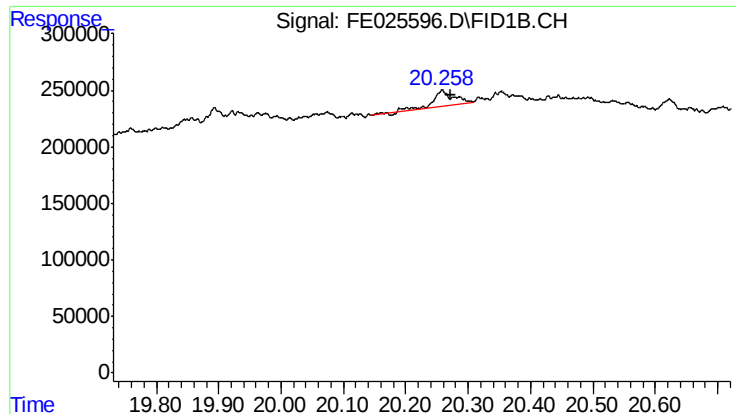

#16 N-HEXATRIACONTANE

R.T.: 20.258 min
Delta R.T.: -0.014 min
Response: 301567
Conc: 2.27 ug/ml

Instrument :
FID_E
ClientSampleId :