

Data Path : P:\HPCHEM1\FID E\Data\FE011518\
 Data File : FE025597.D
 Signal(s) : FID1B.CH
 Acq On : 15 Jan 2018 13:31
 Operator : UA/AJ
 Sample : J1011-14 50X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 00:19:17 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.880	628810	3.457 ug/ml
Target Compounds				
2)	N-DECANE	4.579	2235771	14.981 ug/ml
3)	N-DODECANE	6.597	3489939	21.876 ug/ml
4)	N-TETRADECANE	8.390	1464936	8.038 ug/ml
5)	N-HEXADECANE	9.990	234569	1.148 ug/ml
10)	N-TETRACOSANE	15.039	145992	0.685 ug/ml
11)	N-HEXACOSANE	16.061	182147	0.945 ug/ml
12)	N-OCTACOSANE	17.011	126660	0.753 ug/ml
13)	N-TRIACONTANE	17.897	313293	1.984 ug/ml
14)	N-DOTRIACONTANE	18.730	362519	2.235 ug/ml
15)	N-TETRATRIACONTANE	19.513	179174	1.153 ug/ml
16)	N-HEXATRIACONTANE	20.252	271851	2.045 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011518\
Data File : FE025597.D
Signal(s) : FID1B.CH
Acq On : 15 Jan 2018 13:31
Operator : UA/AJ
Sample : J1011-14 50X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 16 00:19:17 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

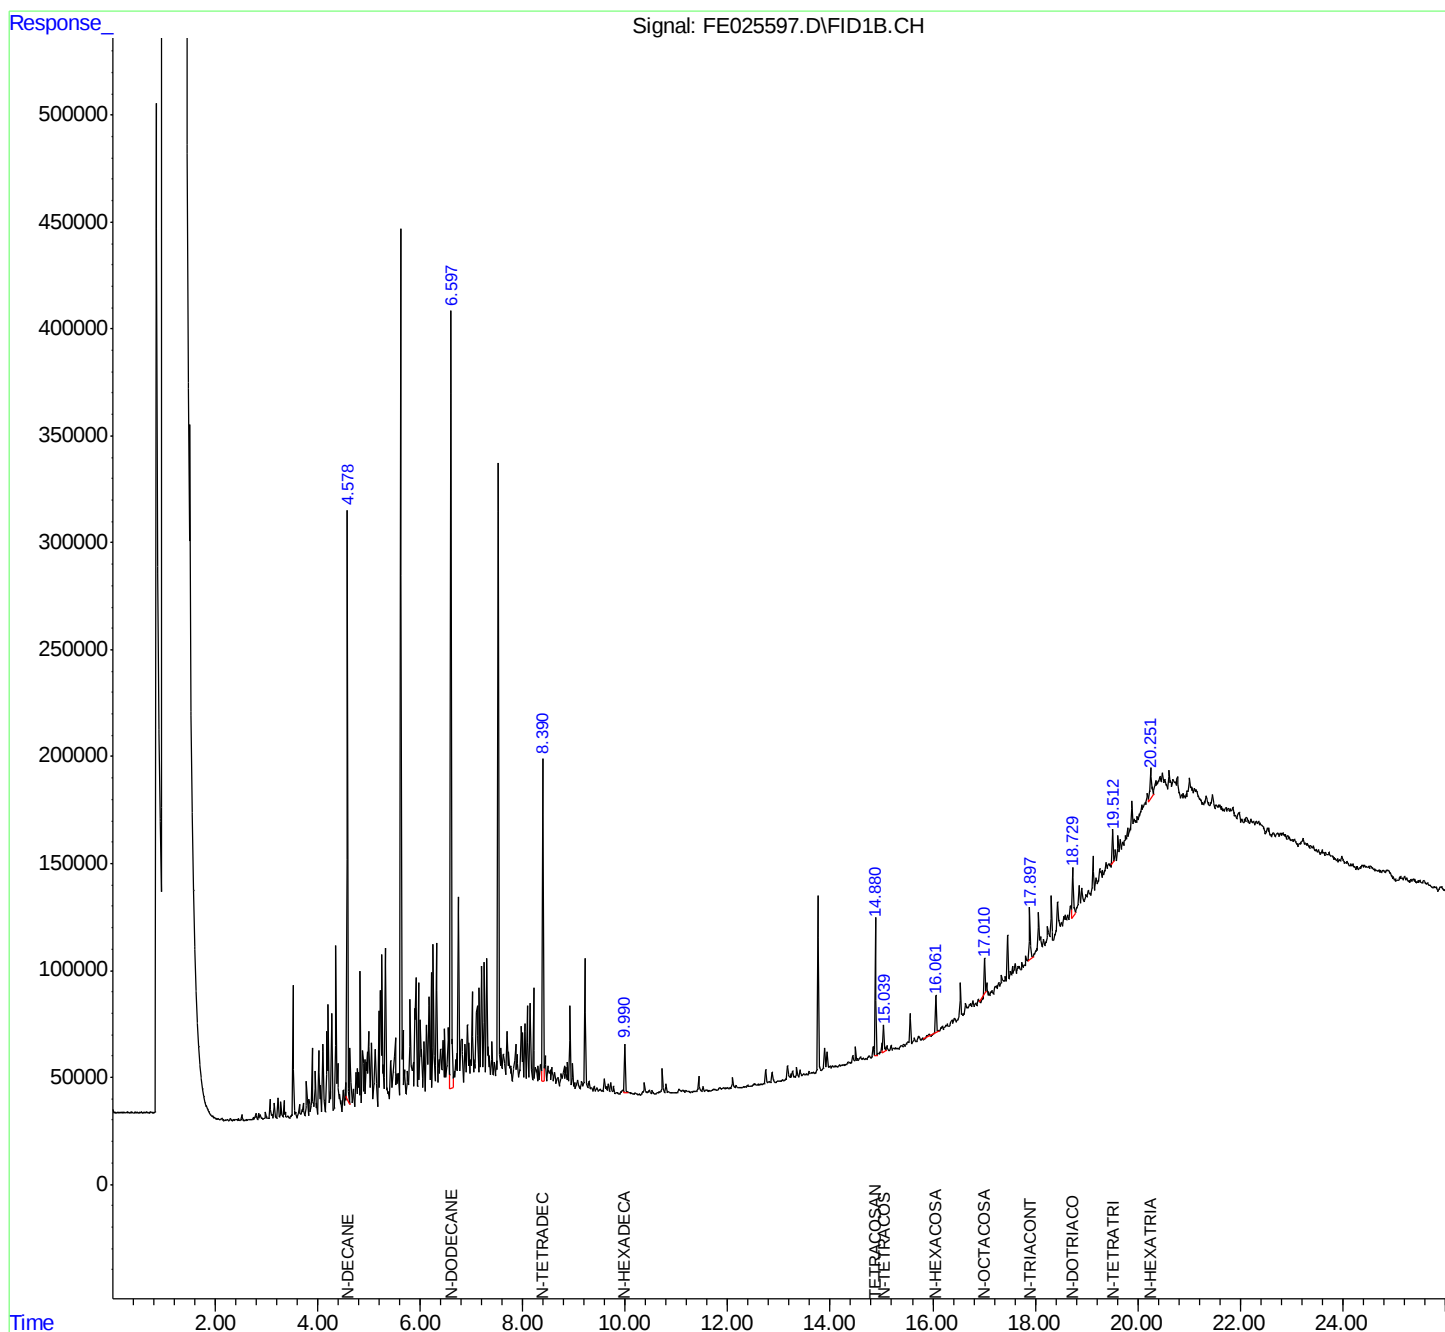


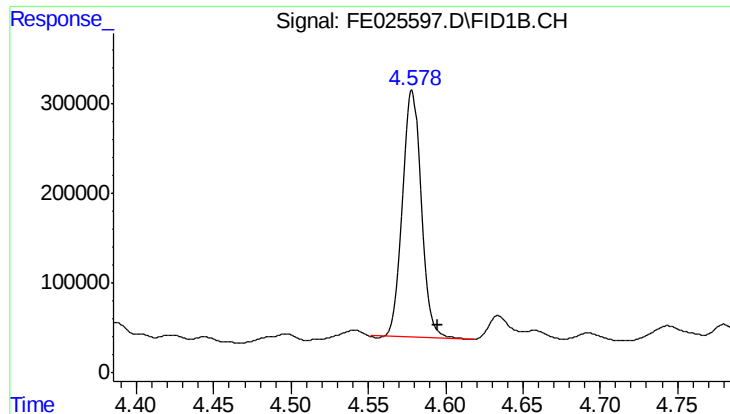

#2 N-DECANE


R.T.: 4.579 min
Delta R.T.: -0.016 min
Response: 2235771
Conc: 14.98 ug/ml

Instrument :
FID_E
ClientSampleId :

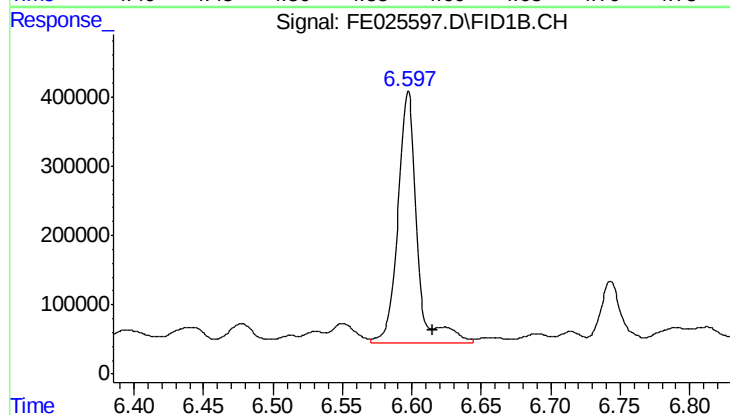


#3 N-DODECANE

R.T.: 6.597 min
Delta R.T.: -0.018 min
Response: 3489939
Conc: 21.88 ug/ml

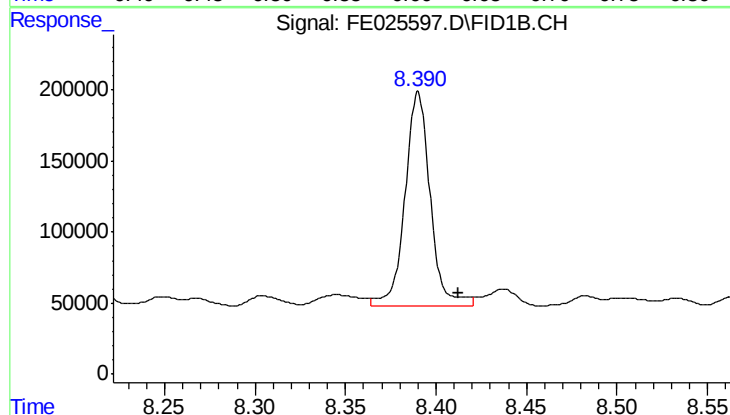


#4 N-TETRADECANE

R.T.: 8.390 min
Delta R.T.: -0.022 min
Response: 1464936
Conc: 8.04 ug/ml

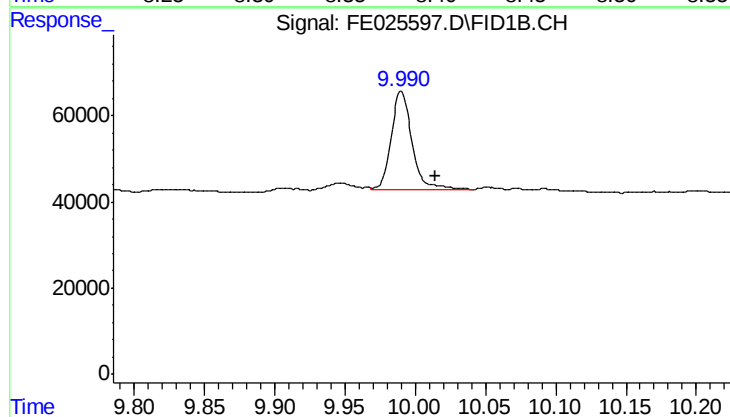

#5 N-HEXADECANE


R.T.: 9.990 min
Delta R.T.: -0.024 min
Response: 234569
Conc: 1.15 ug/ml

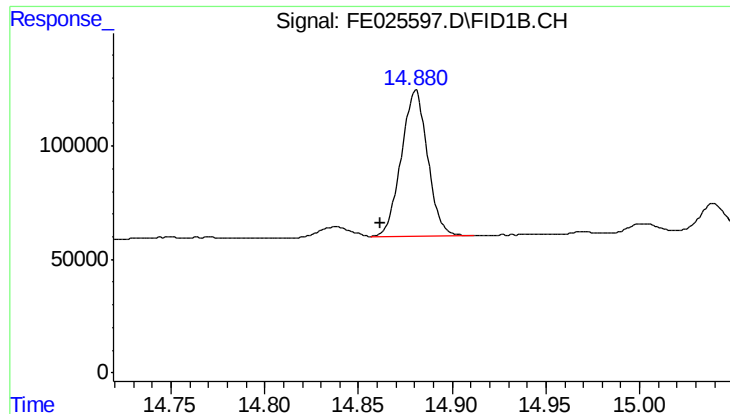

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.880 min
Delta R.T.: 0.019 min
Response: 628810
Conc: 3.46 ug/ml

Instrument :
FID_E
ClientSampleId :

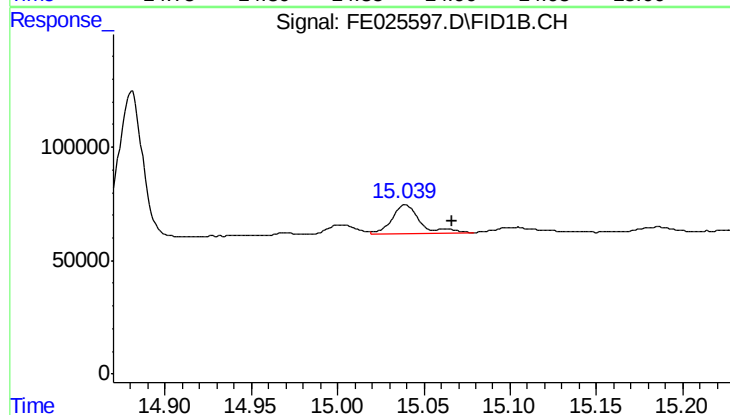


#10 N-TETRACOSANE

R.T.: 15.039 min
Delta R.T.: -0.027 min
Response: 145992
Conc: 0.68 ug/ml

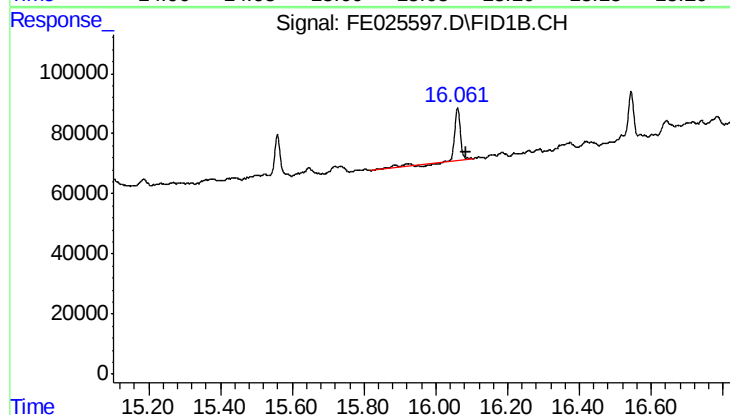


#11 N-HEXACOSANE

R.T.: 16.061 min
Delta R.T.: -0.025 min
Response: 182147
Conc: 0.95 ug/ml

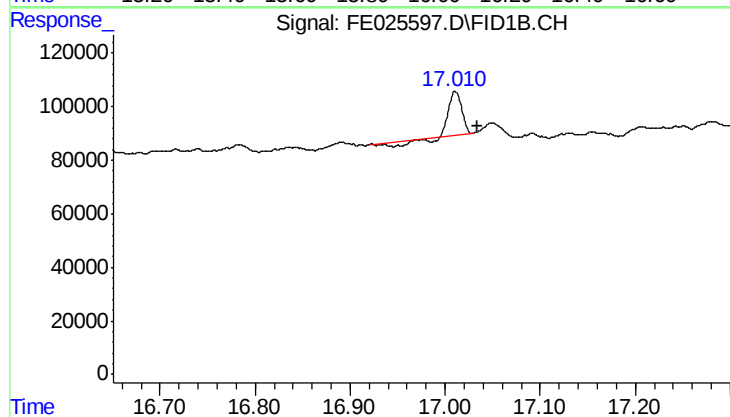

#12 N-OCTACOSANE


R.T.: 17.011 min
Delta R.T.: -0.023 min
Response: 126660
Conc: 0.75 ug/ml

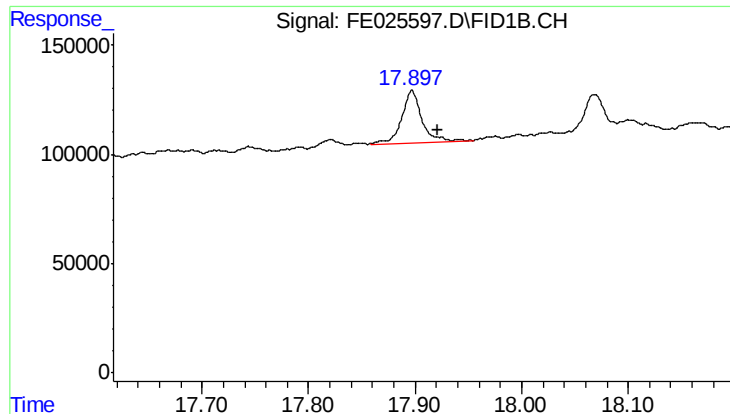

#13 N-TRIACONTANE


R.T.: 17.897 min
Delta R.T.: -0.024 min
Response: 313293
Conc: 1.98 ug/ml

Instrument :
FID_E
ClientSampleId :

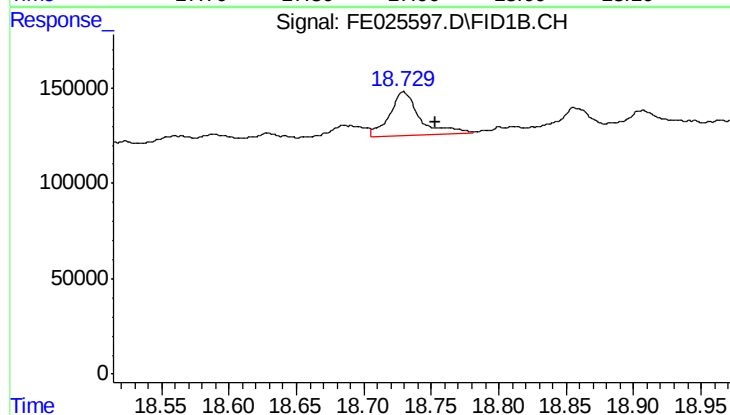


#14 N-DOTRIACONTANE

R.T.: 18.730 min
Delta R.T.: -0.023 min
Response: 362519
Conc: 2.24 ug/ml

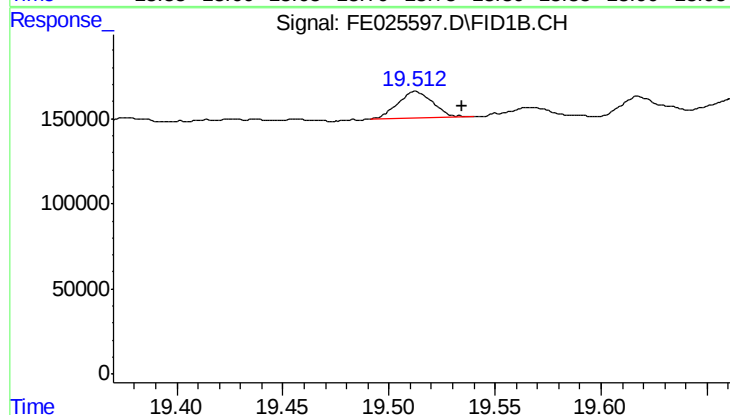

#15 N-TETRATRIACONTANE

R.T.: 19.513 min
Delta R.T.: -0.022 min
Response: 179174
Conc: 1.15 ug/ml

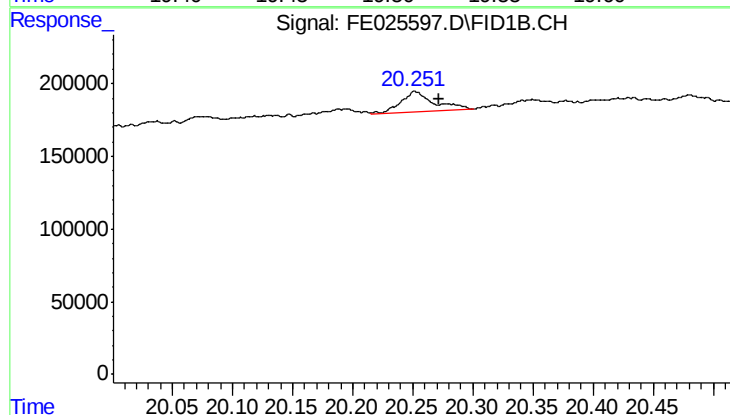

#16 N-HEXATRIACONTANE

R.T.: 20.252 min
Delta R.T.: -0.020 min
Response: 271851
Conc: 2.05 ug/ml