

Data Path : P:\HPCHEM1\FID E\Data\FE011518\
 Data File : FE025619.D
 Signal(s) : FID1B.CH
 Acq On : 16 Jan 2018 2:16
 Operator : UA/AJ
 Sample : J1115-18
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 05:28:14 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.831	2396088	13.174 ug/ml
Target Compounds			
4) N-TETRADECANE	8.464f	889602	4.881 ug/ml
5) N-HEXADECANE	9.984	321791	1.575 ug/ml
6) N-OCTADECANE	11.425	188936	0.855 ug/ml
12) N-OCTACOSANE	17.001	129359	0.769 ug/ml
13) N-TRIACONTANE	17.887	189076	1.197 ug/ml
14) N-DOTRIACONTANE	18.714	226833	1.399 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011518\
Data File : FE025619.D
Signal(s) : FID1B.CH
Acq On : 16 Jan 2018 2:16
Operator : UA/AJ
Sample : J1115-18
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 05:28:14 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

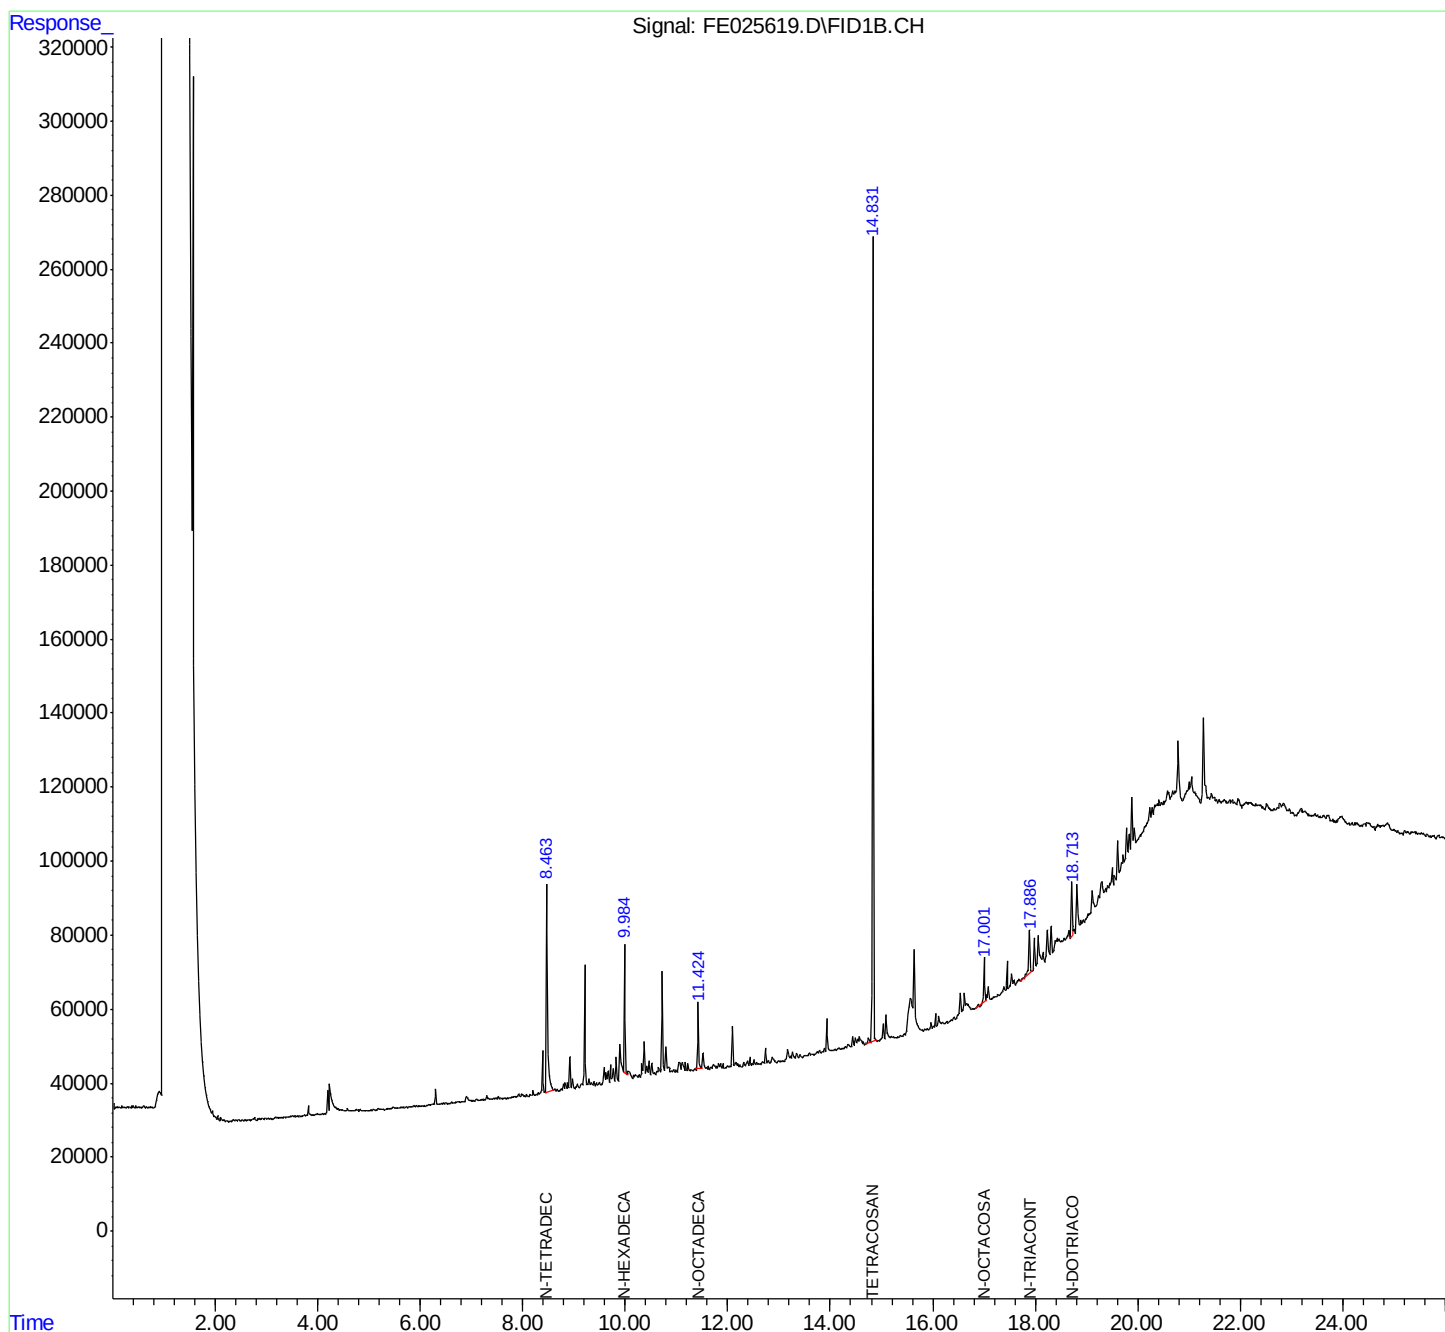


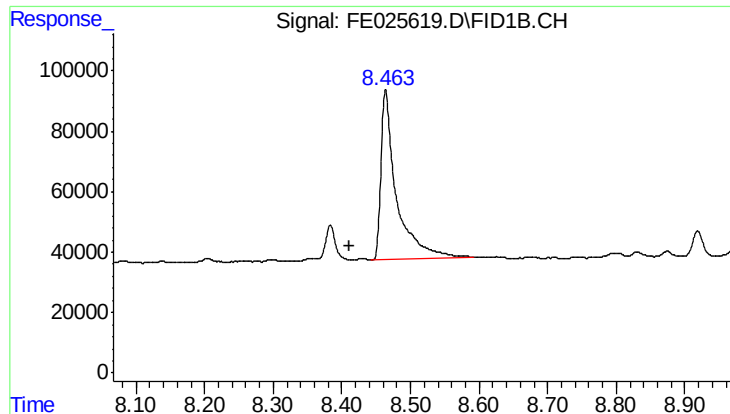

#4 N-TETRADECANE


R.T.: 8.464 min
Delta R.T.: 0.052 min
Response: 889602
Conc: 4.88 ug/ml

Instrument :
FID_E
ClientSampleId :

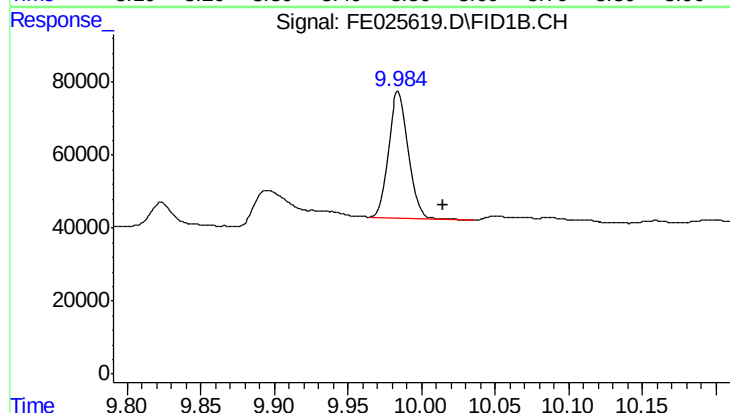


#5 N-HEXADECANE

R.T.: 9.984 min
Delta R.T.: -0.030 min
Response: 321791
Conc: 1.58 ug/ml

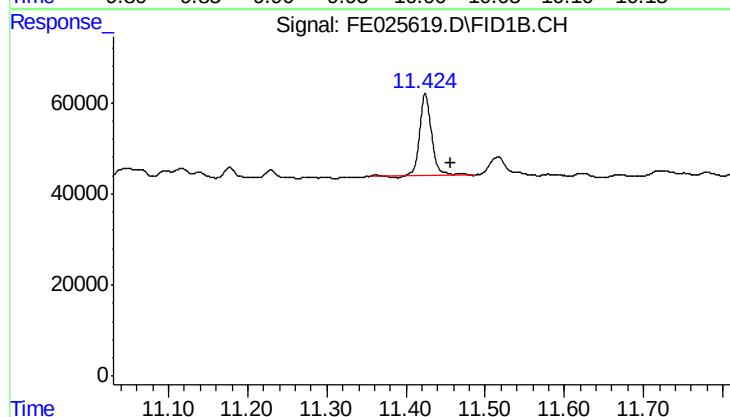


#6 N-OCTADECANE

R.T.: 11.425 min
Delta R.T.: -0.031 min
Response: 188936
Conc: 0.85 ug/ml

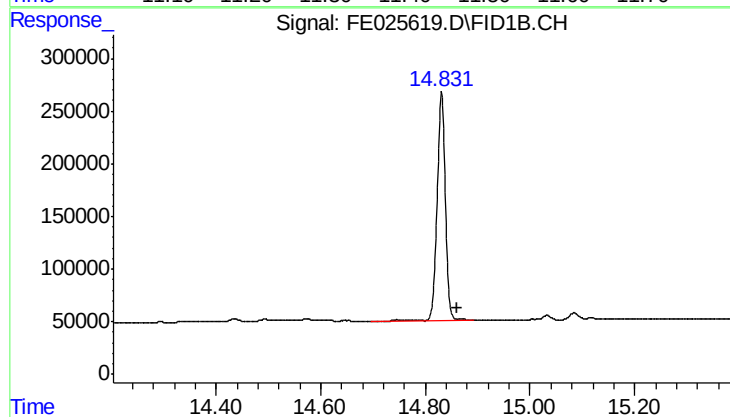

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.831 min
Delta R.T.: -0.030 min
Response: 2396088
Conc: 13.17 ug/ml

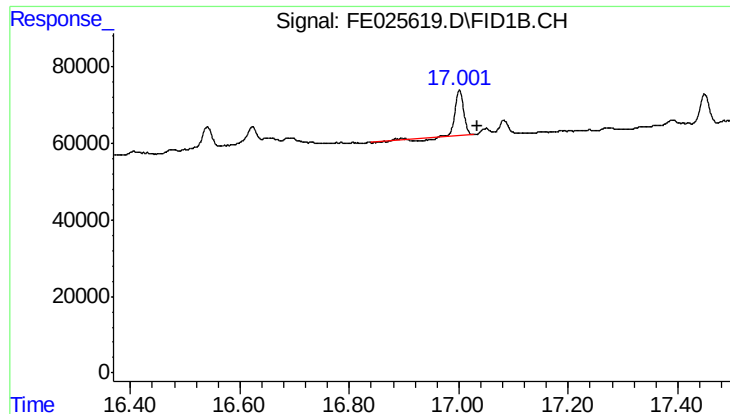

#12 N-OCTACOSANE


R.T.: 17.001 min
Delta R.T.: -0.033 min
Response: 129359
Conc: 0.77 ug/ml

Instrument :
FID_E
ClientSampleId :

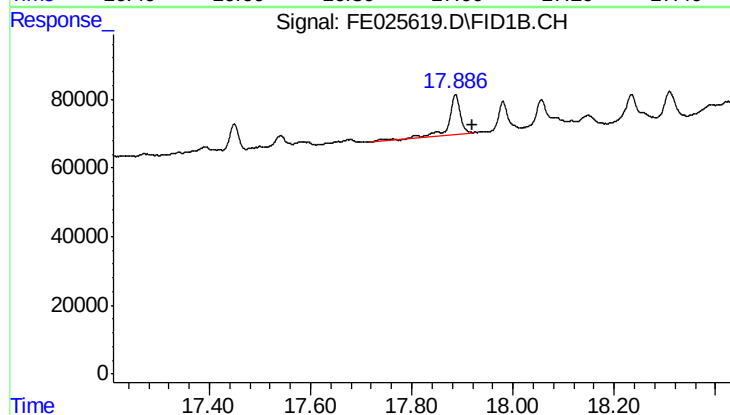

#13 N-TRIACONTANE

R.T.: 17.887 min
Delta R.T.: -0.034 min
Response: 189076
Conc: 1.20 ug/ml

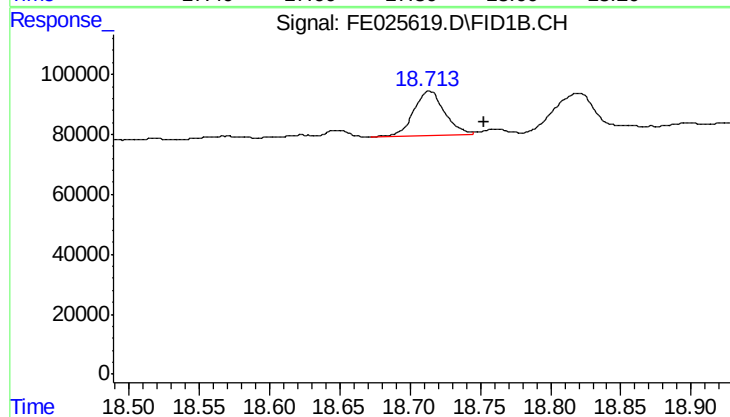

#14 N-DOTRIACONTANE

R.T.: 18.714 min
Delta R.T.: -0.039 min
Response: 226833
Conc: 1.40 ug/ml