

Data Path : P:\HPCHEM1\FID E\Data\FE011518\
 Data File : FE025624.D
 Signal(s) : FID1B.CH
 Acq On : 16 Jan 2018 5:09
 Operator : UA/AJ
 Sample : J1115-12
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 06:13:09 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.833	2855436	15.699 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.463f	824276	4.523 ug/ml
5)	N-HEXADECANE	9.983	510678	2.500 ug/ml
6)	N-OCTADECANE	11.424	191089	0.865 ug/ml
10)	N-TETRACOSANE	15.087	289207	1.356 ug/ml
12)	N-OCTACOSANE	17.002	368074	2.189 ug/ml
13)	N-TRIACONTANE	17.889	357200	2.262 ug/ml
14)	N-DOTRIACONTANE	18.716	503468	3.104 ug/ml
16)	N-HEXATRIACONTANE	20.246	44733	0.337 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE011518\
Data File : FE025624.D
Signal(s) : FID1B.CH
Acq On : 16 Jan 2018 5:09
Operator : UA/AJ
Sample : J1115-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 06:13:09 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

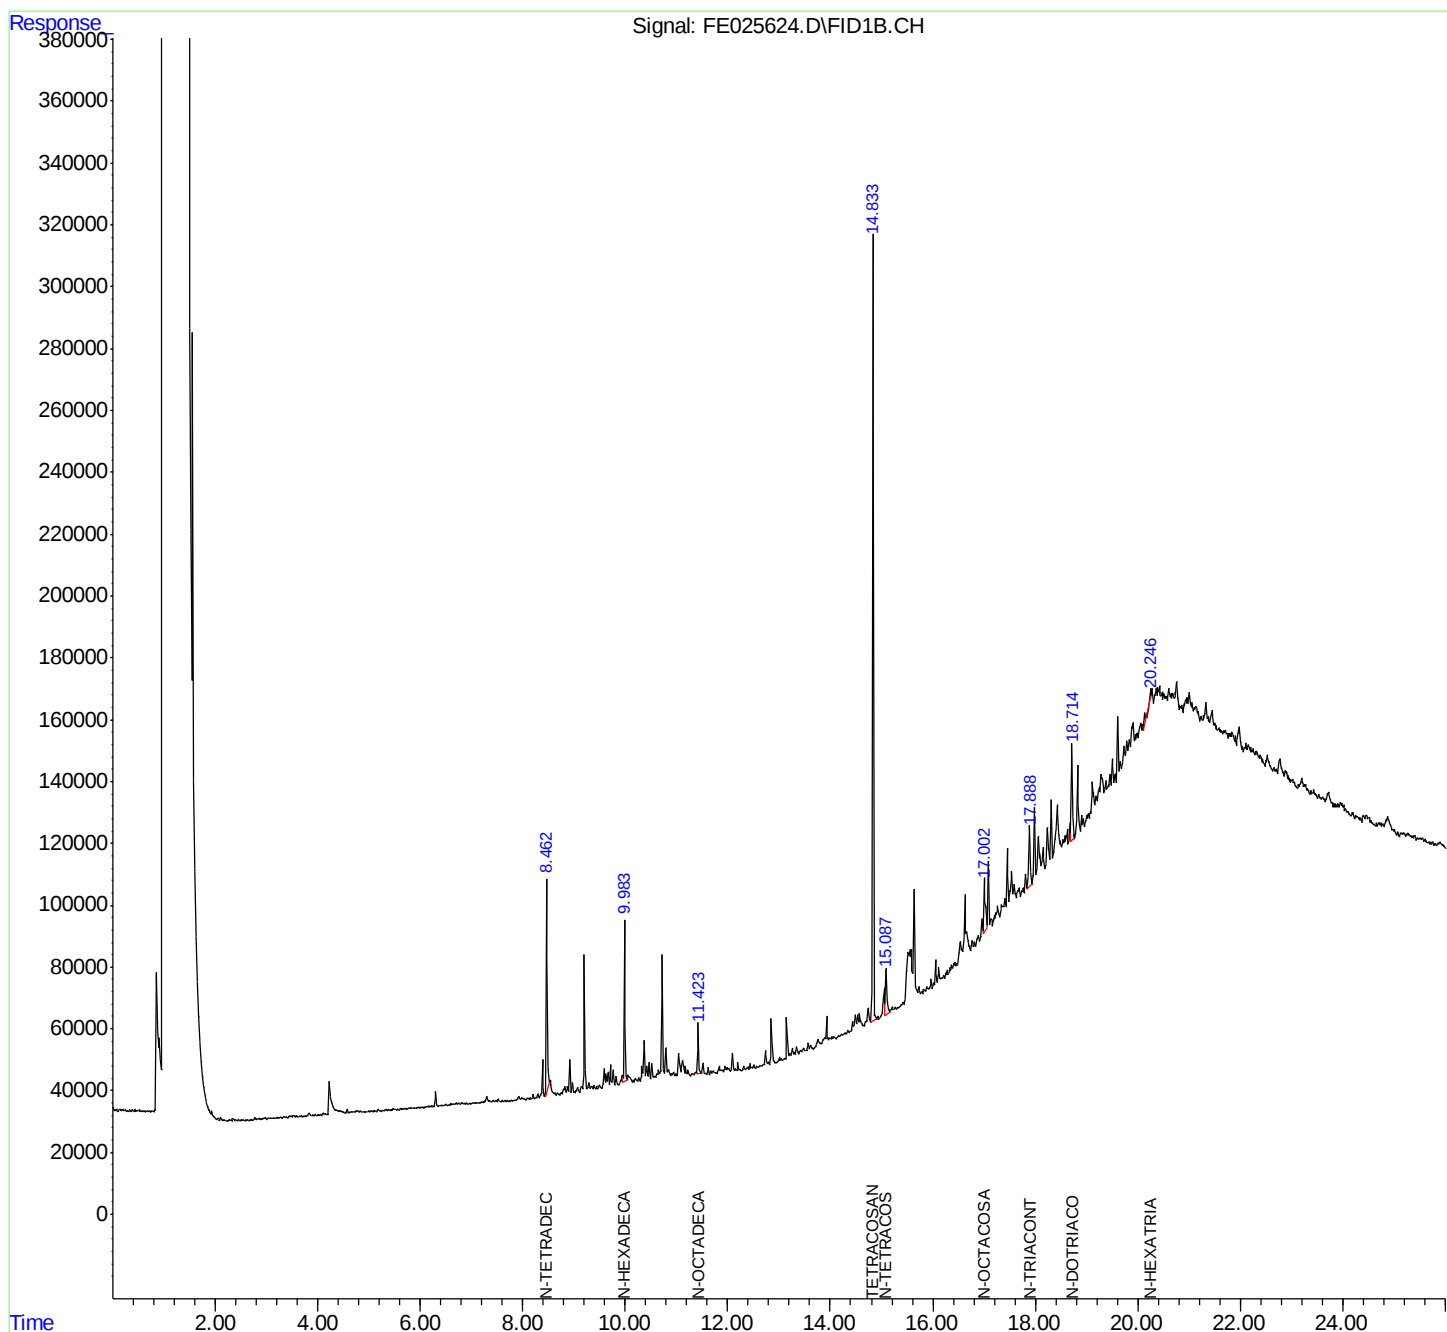


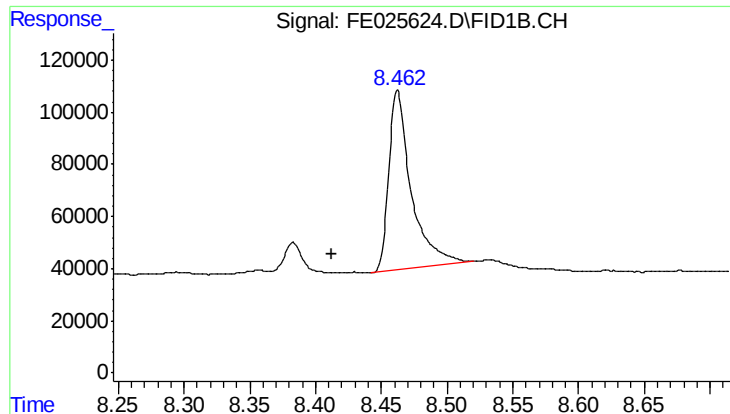

#4 N-TETRADECANE


R.T.: 8.463 min
Delta R.T.: 0.051 min
Response: 824276
Conc: 4.52 ug/ml

Instrument :
FID_E
ClientSampleId :

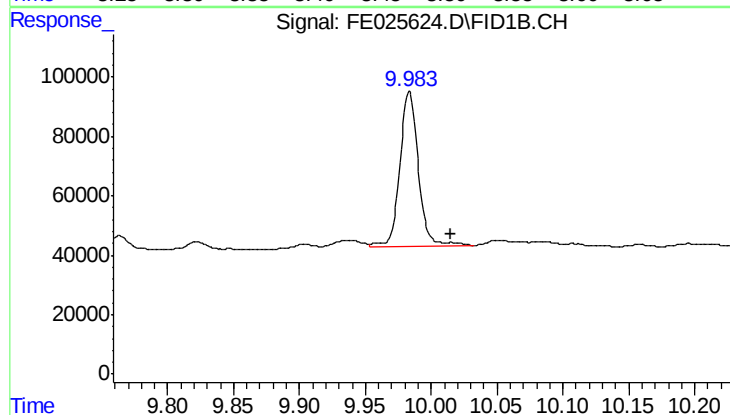


#5 N-HEXADECANE

R.T.: 9.983 min
Delta R.T.: -0.031 min
Response: 510678
Conc: 2.50 ug/ml

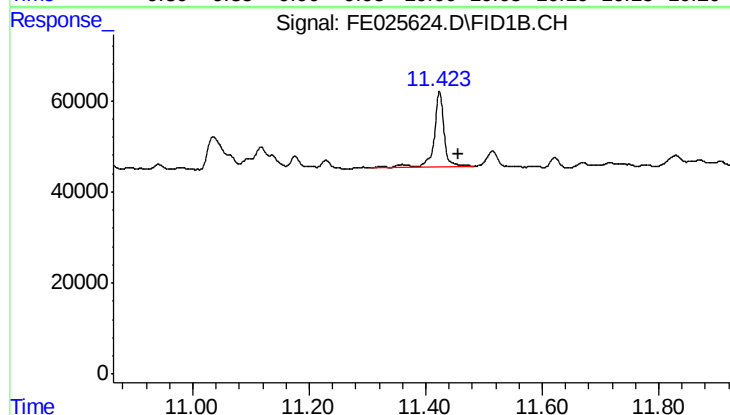


#6 N-OCTADECANE

R.T.: 11.424 min
Delta R.T.: -0.032 min
Response: 191089
Conc: 0.86 ug/ml

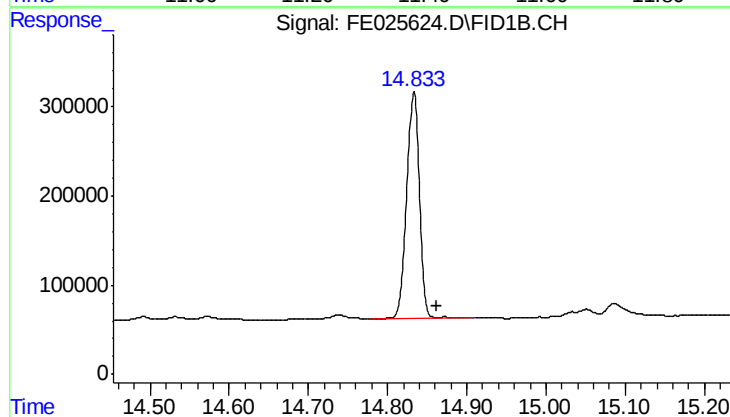

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.833 min
Delta R.T.: -0.028 min
Response: 2855436
Conc: 15.70 ug/ml

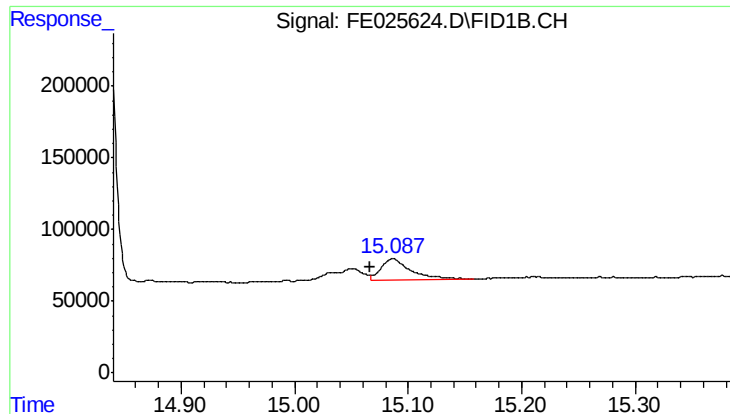

#10 N-TETRACOSANE


R.T.: 15.087 min
Delta R.T.: 0.020 min
Response: 289207
Conc: 1.36 ug/ml

Instrument :
FID_E
ClientSampleId :

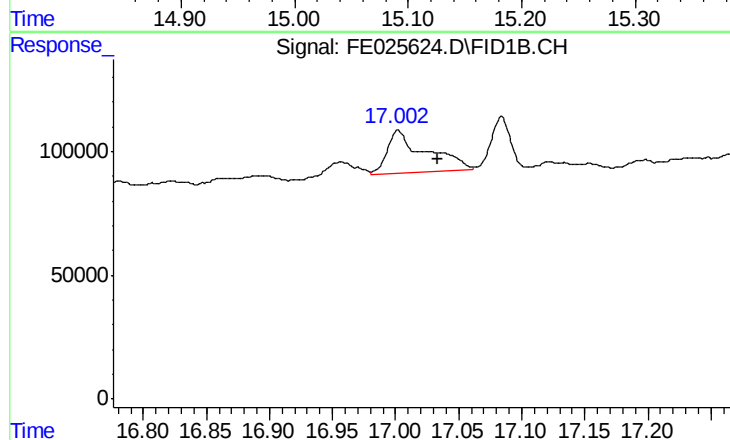


#12 N-OCTACOSANE

R.T.: 17.002 min
Delta R.T.: -0.032 min
Response: 368074
Conc: 2.19 ug/ml

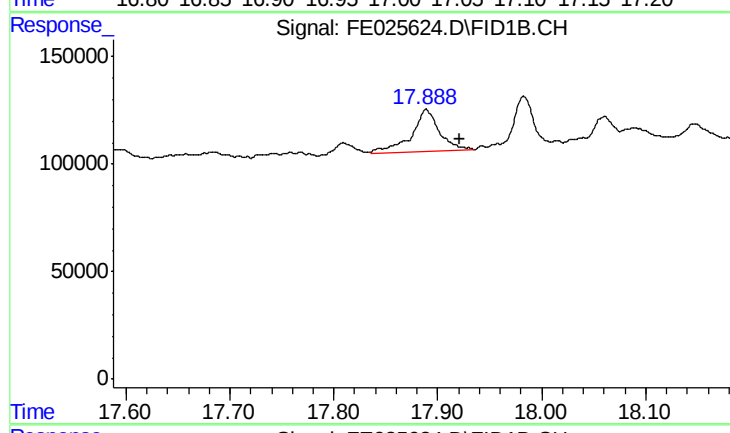


#13 N-TRIACONTANE

R.T.: 17.889 min
Delta R.T.: -0.032 min
Response: 357200
Conc: 2.26 ug/ml

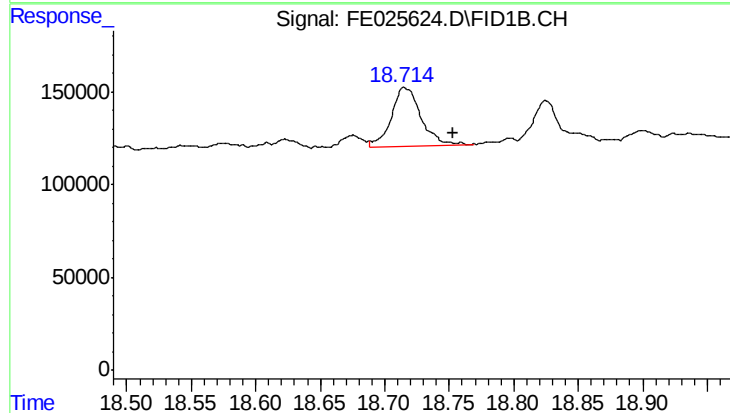

#14 N-DOTRIACONTANE

R.T.: 18.716 min
Delta R.T.: -0.037 min
Response: 503468
Conc: 3.10 ug/ml

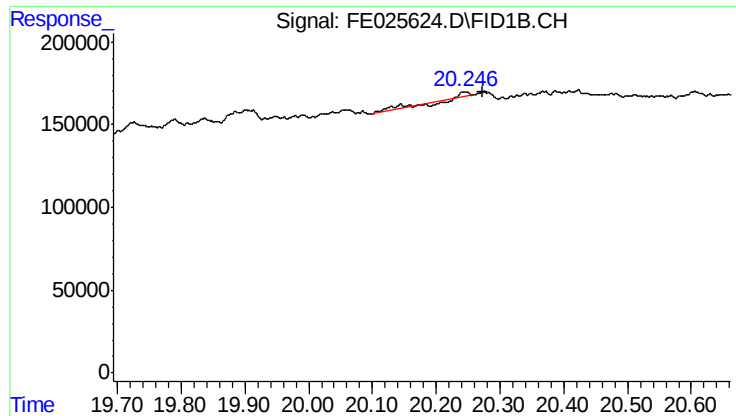

#16 N-HEXATRIACONTANE

R.T.: 20.246 min
Delta R.T.: -0.027 min
Response: 44733
Conc: 0.34 ug/ml

Instrument :
FID_E
ClientSampleId :