

Data Path : P:\HPCHEM1\FID_E\Data\FE011518\
 Data File : FE025629.D
 Signal(s) : FID1B.CH
 Acq On : 16 Jan 2018 8:01
 Operator : UA/AJ
 Sample : J1116-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 09:15:23 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.837	2739311	15.061 ug/ml
Target Compounds			
4) N-TETRADECANE	8.465f	1698865	9.322 ug/ml
10) N-TETRACOSANE	15.086	704450	3.303 ug/ml
11) N-HEXACOSANE	16.061	306656	1.591 ug/ml
12) N-OCTACOSANE	17.020	851920	5.067 ug/ml
13) N-TRIACONTANE	17.904	2180213	13.808 ug/ml
14) N-DOTRIACONTANE	18.733	1060177	6.537 ug/ml
15) N-TETRATRIACONTANE	19.473f	376072	2.421 ug/ml
16) N-HEXATRIACONTANE	20.264	377987	2.844 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE011518\
Data File : FE025629.D
Signal(s) : FID1B.CH
Acq On : 16 Jan 2018 8:01
Operator : UA/AJ
Sample : J1116-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 09:15:23 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

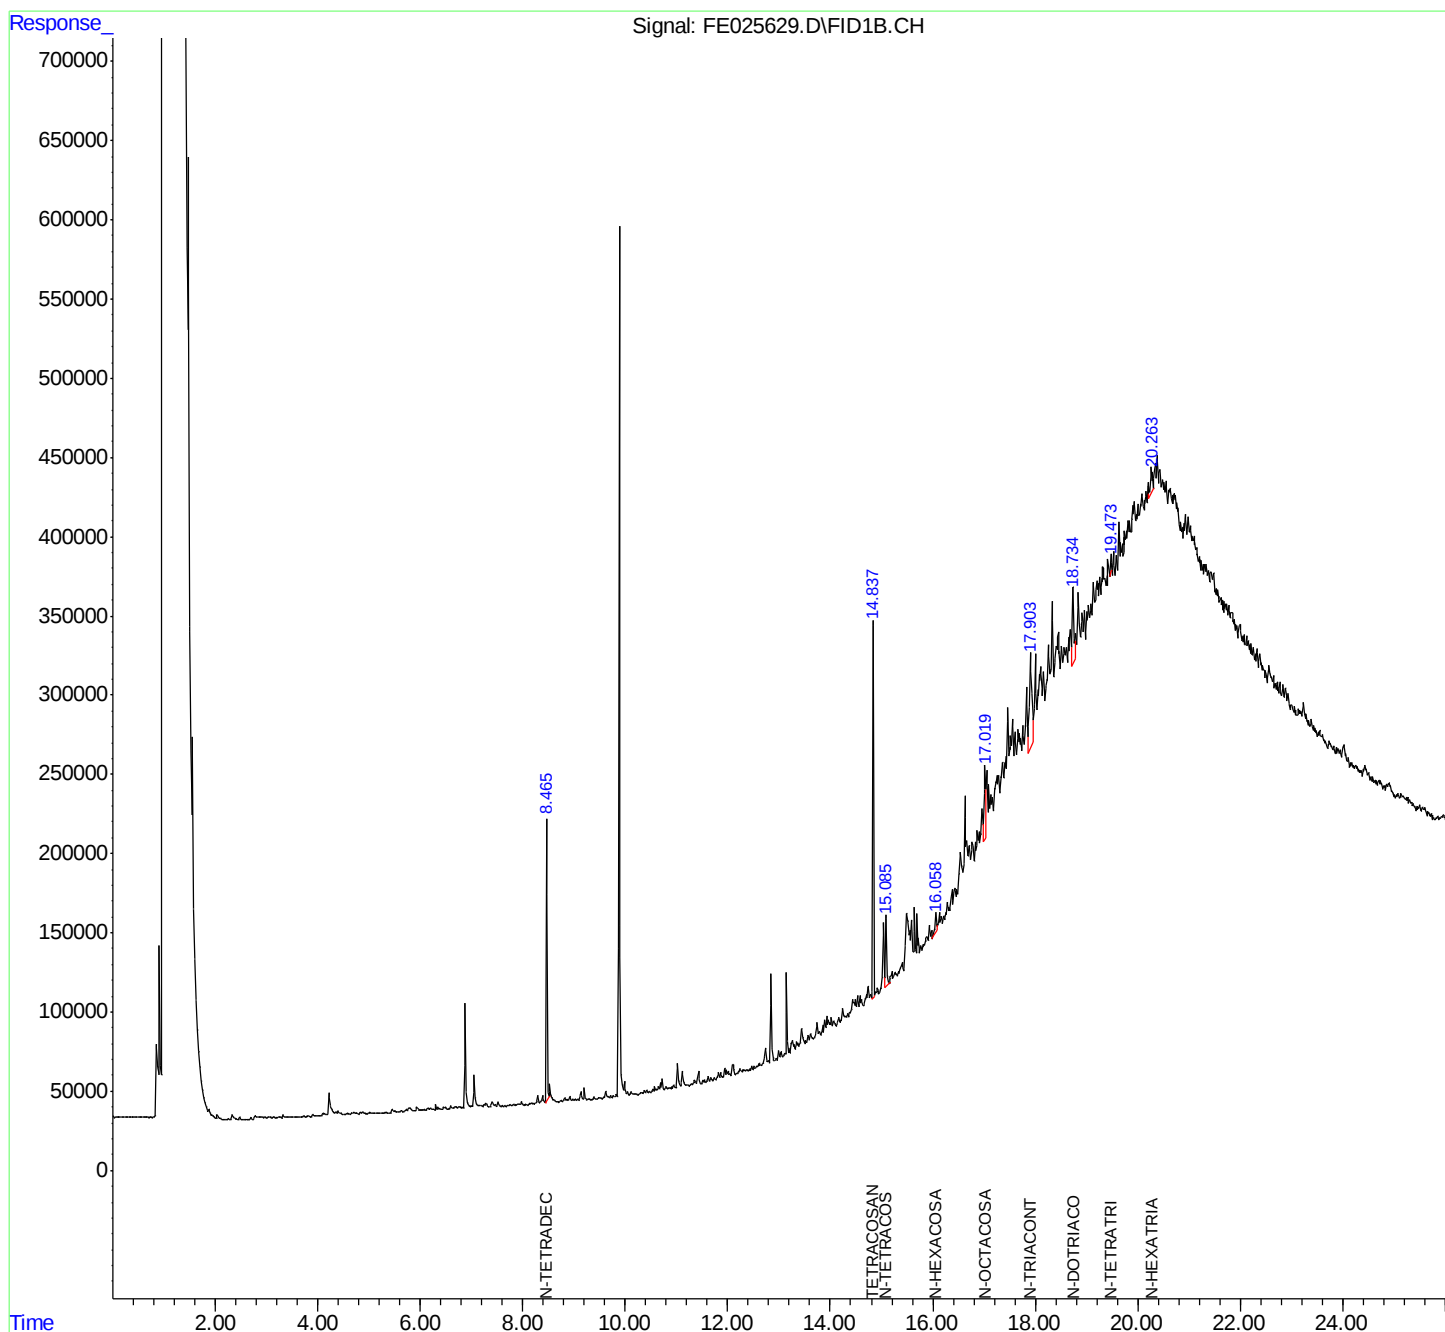


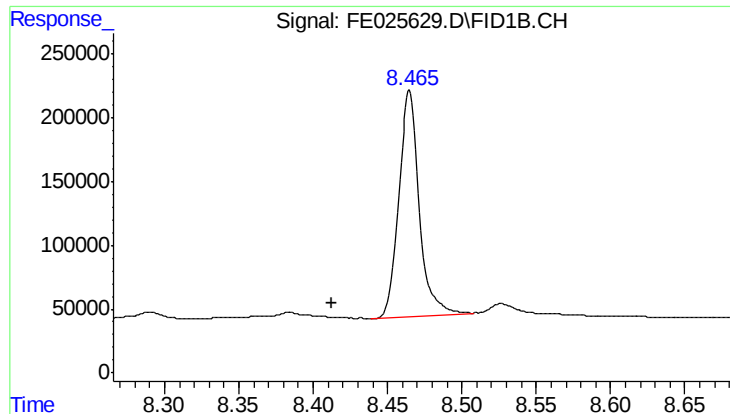

#4 N-TETRADECANE


R.T.: 8.465 min
Delta R.T.: 0.053 min
Response: 1698865
Conc: 9.32 ug/ml

Instrument :
FID_E
ClientSampleId :

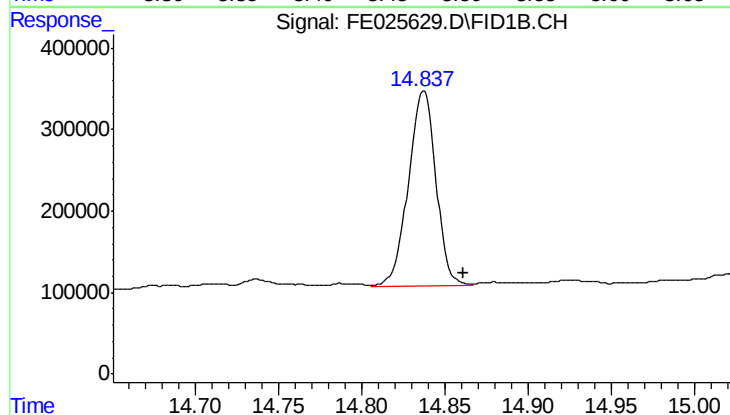


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.837 min
Delta R.T.: -0.024 min
Response: 2739311
Conc: 15.06 ug/ml

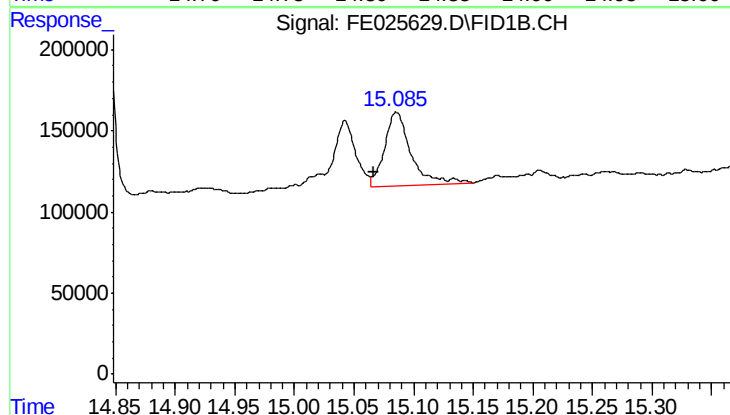


#10 N-TETRACOSANE

R.T.: 15.086 min
Delta R.T.: 0.019 min
Response: 704450
Conc: 3.30 ug/ml

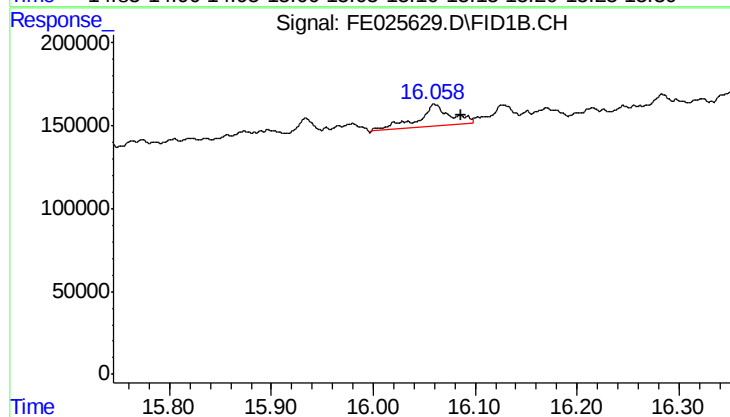

#11 N-HEXACOSANE


R.T.: 16.061 min
Delta R.T.: -0.025 min
Response: 306656
Conc: 1.59 ug/ml

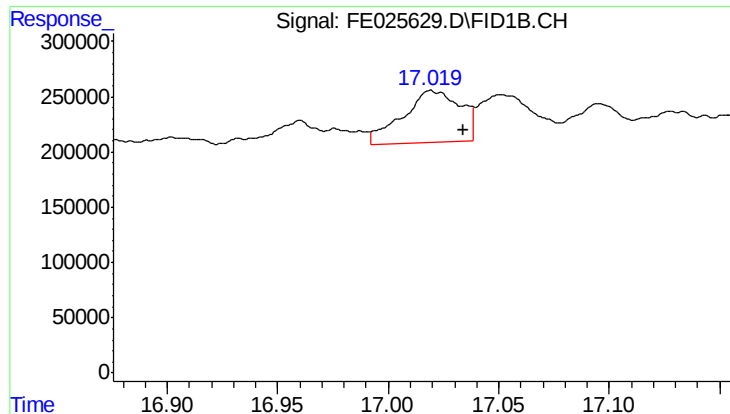

#12 N-OCTACOSANE


R.T.: 17.020 min
Delta R.T.: -0.014 min
Response: 851920
Conc: 5.07 ug/ml

Instrument :
FID_E
ClientSampleId :

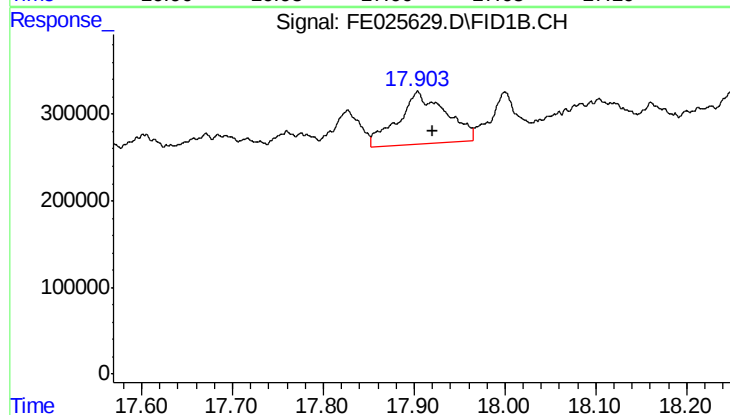


#13 N-TRIACONTANE

R.T.: 17.904 min
Delta R.T.: -0.017 min
Response: 2180213
Conc: 13.81 ug/ml

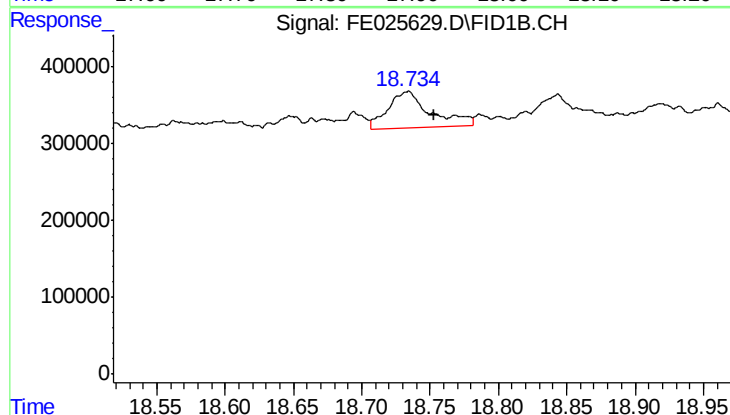


#14 N-DOTRIACONTANE

R.T.: 18.733 min
Delta R.T.: -0.020 min
Response: 1060177
Conc: 6.54 ug/ml

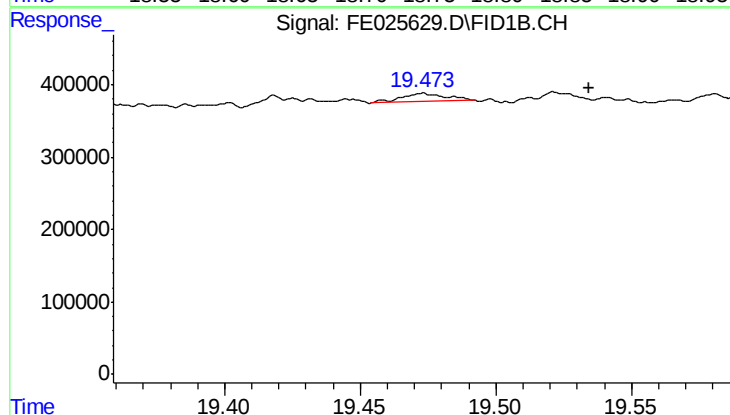

#15 N-TETRATRIACONTANE

R.T.: 19.473 min
Delta R.T.: -0.061 min
Response: 376072
Conc: 2.42 ug/ml

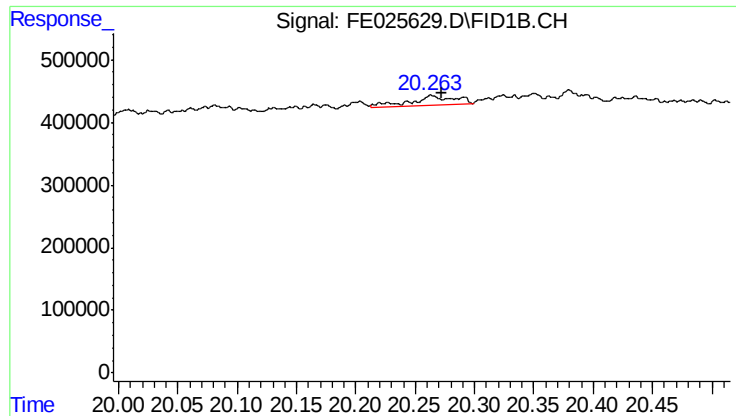

#16 N-HEXATRIACONTANE

R.T.: 20.264 min
Delta R.T.: -0.008 min
Response: 377987
Conc: 2.84 ug/ml

Instrument :
FID_E
ClientSampleId :