

Data Path : P:\HPCHEM1\FID_E\Data\FE011518\
 Data File : FE025631.D
 Signal(s) : FID1B.CH
 Acq On : 16 Jan 2018 9:11
 Operator : UA/AJ
 Sample : J1137-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 09:42:41 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.836	3361749	18.483 ug/ml
Target Compounds			
4) N-TETRADECANE	8.466f	2052397	11.261 ug/ml
7) N-EICOSANE	12.717	663887	2.994 ug/ml
8) N-DOCOSANE	13.914f	417941	1.905 ug/ml
10) N-TETRACOSANE	15.083	3490270	16.366 ug/ml
11) N-HEXACOSANE	16.146f	234031	1.214 ug/ml
12) N-OCTACOSANE	17.007	2643095	15.721 ug/ml
13) N-TRIACONTANE	17.893	671113	4.250 ug/ml
14) N-DOTRIACONTANE	18.719	855032	5.272 ug/ml
16) N-HEXATRIACONTANE	20.245	278370	2.094 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE011518\
Data File : FE025631.D
Signal(s) : FID1B.CH
Acq On : 16 Jan 2018 9:11
Operator : UA/AJ
Sample : J1137-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 09:42:41 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

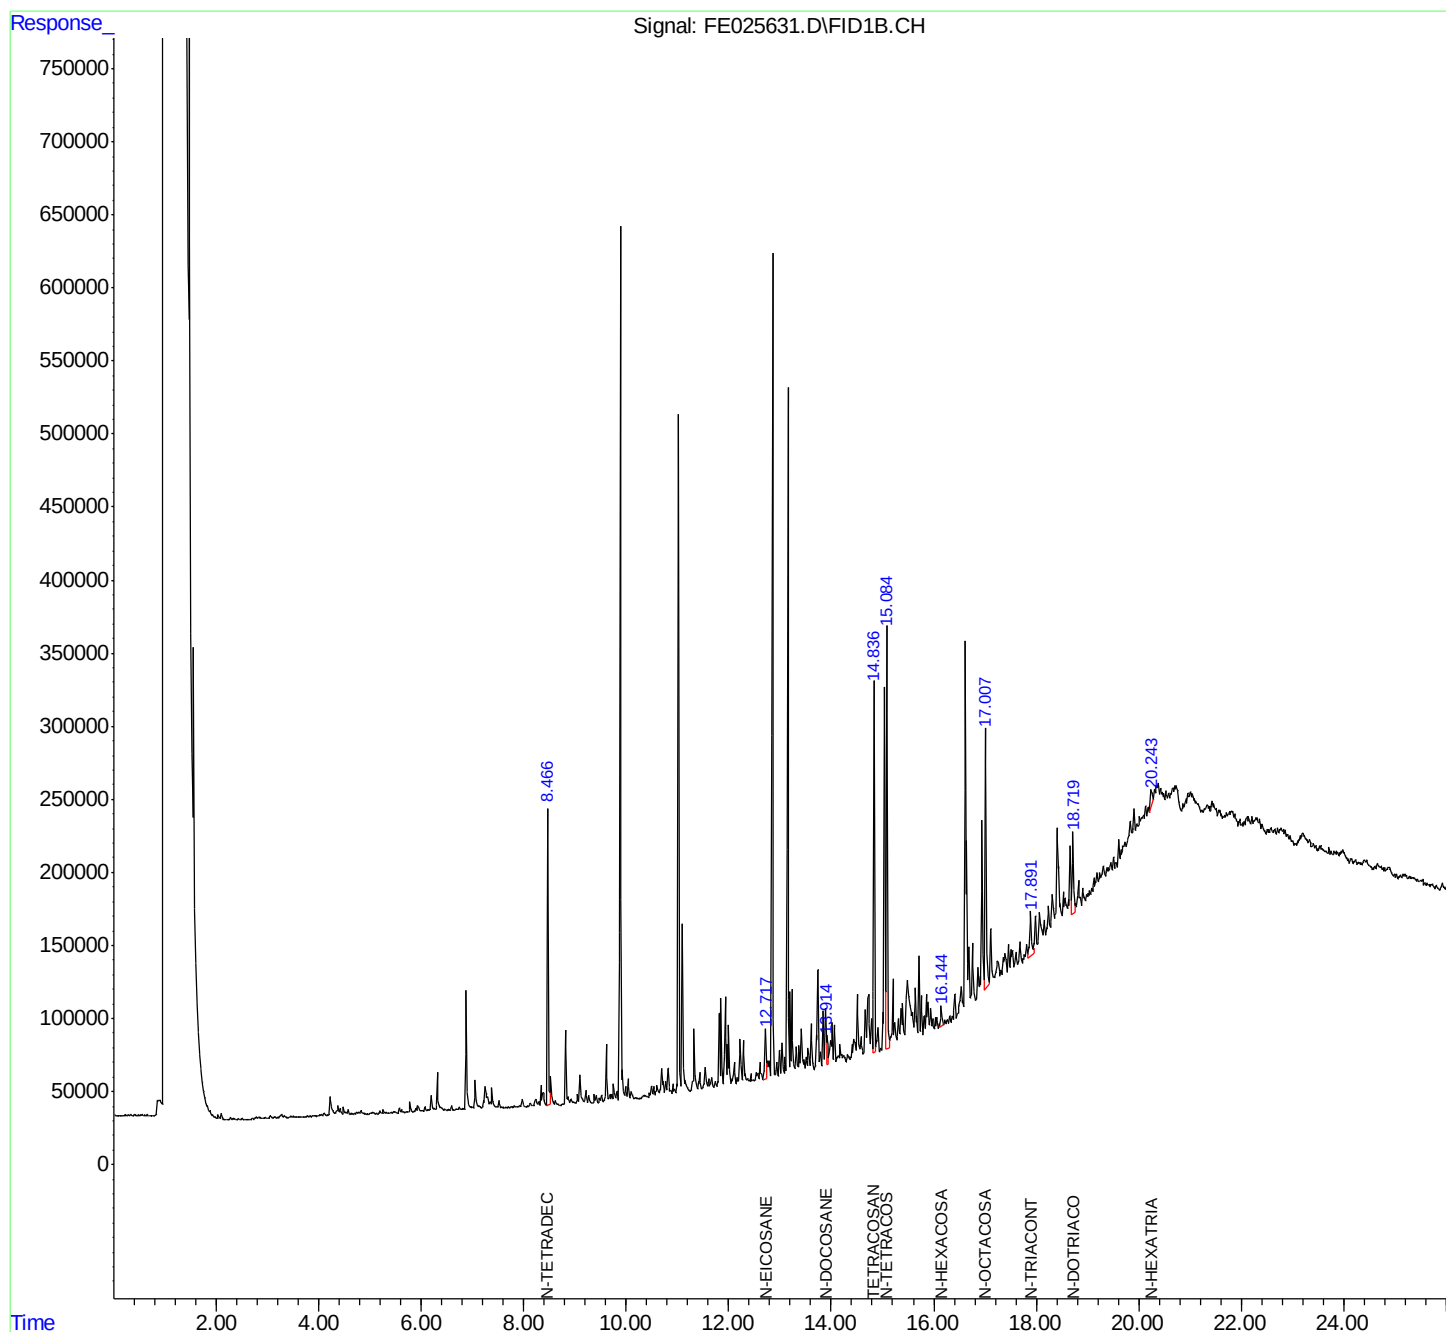


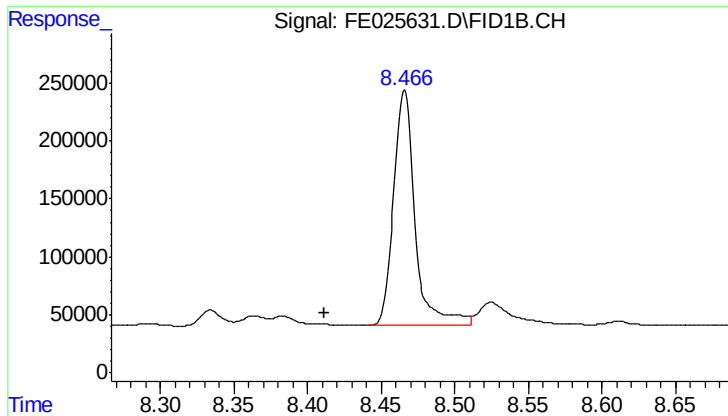

#4 N-TETRADECANE


R.T.: 8.466 min
Delta R.T.: 0.054 min
Response: 2052397
Conc: 11.26 ug/ml

Instrument :
FID_E
ClientSampleId :

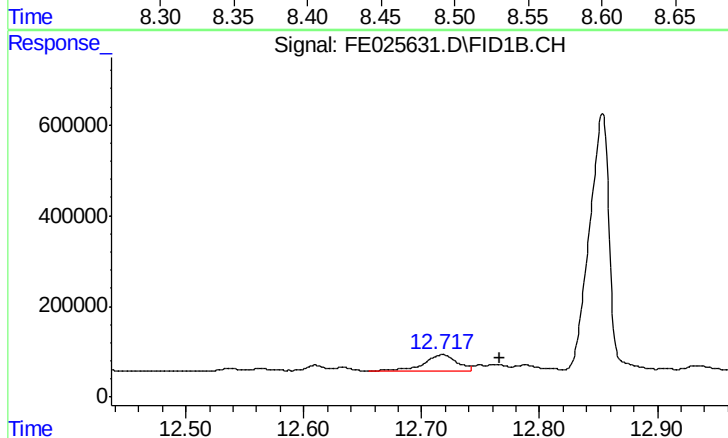


#7 N-EICOSANE

R.T.: 12.717 min
Delta R.T.: -0.049 min
Response: 663887
Conc: 2.99 ug/ml

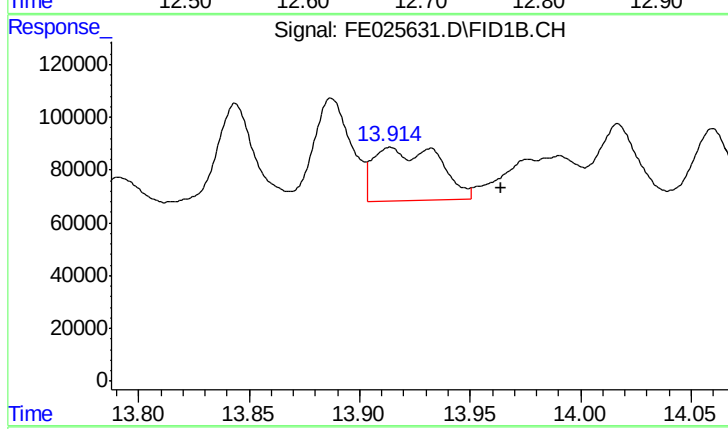


#8 N-DOCOSANE

R.T.: 13.914 min
Delta R.T.: -0.051 min
Response: 417941
Conc: 1.91 ug/ml

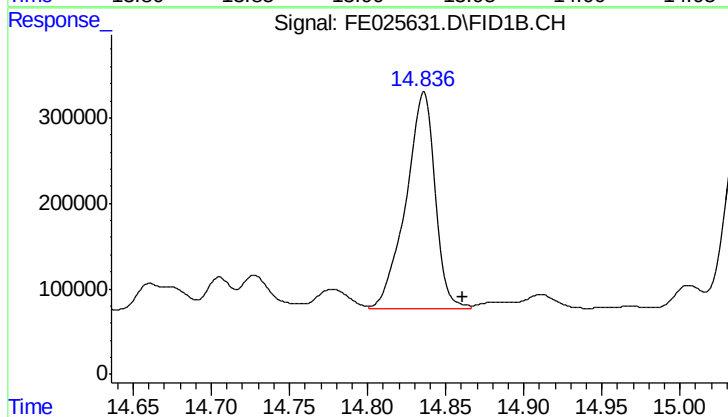

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.836 min
Delta R.T.: -0.026 min
Response: 3361749
Conc: 18.48 ug/ml

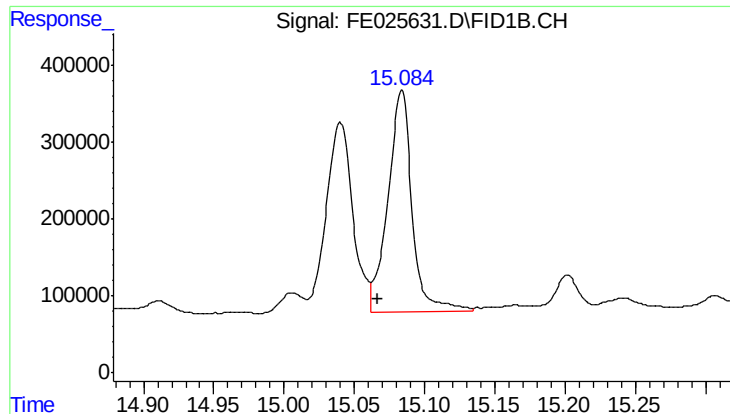

#10 N-TETRACOSANE


R.T.: 15.083 min
Delta R.T.: 0.017 min
Response: 3490270
Conc: 16.37 ug/ml

Instrument :
FID_E
ClientSampleId :

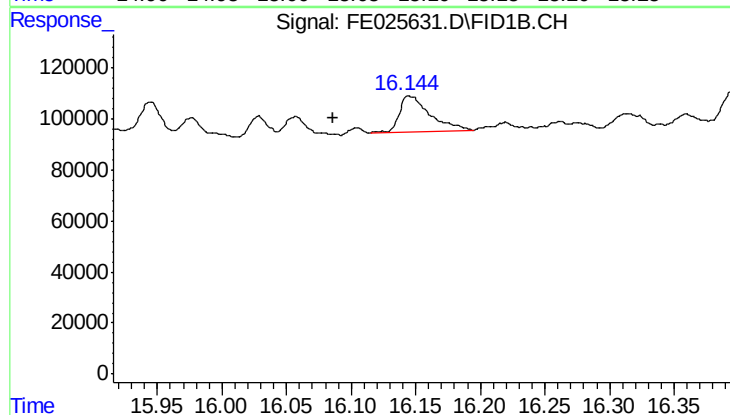


#11 N-HEXACOSANE

R.T.: 16.146 min
Delta R.T.: 0.060 min
Response: 234031
Conc: 1.21 ug/ml

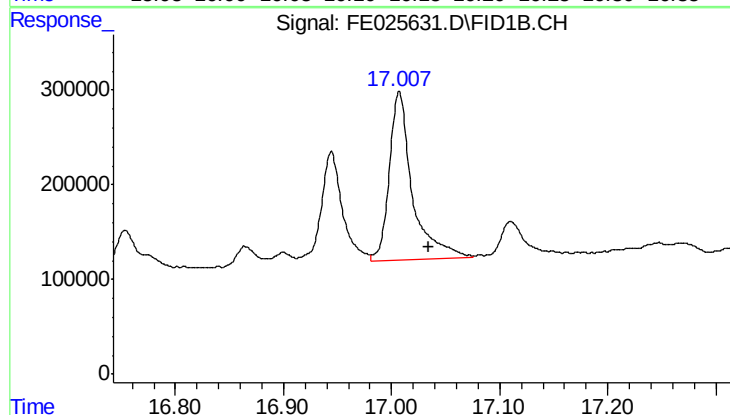


#12 N-OCTACOSANE

R.T.: 17.007 min
Delta R.T.: -0.027 min
Response: 2643095
Conc: 15.72 ug/ml

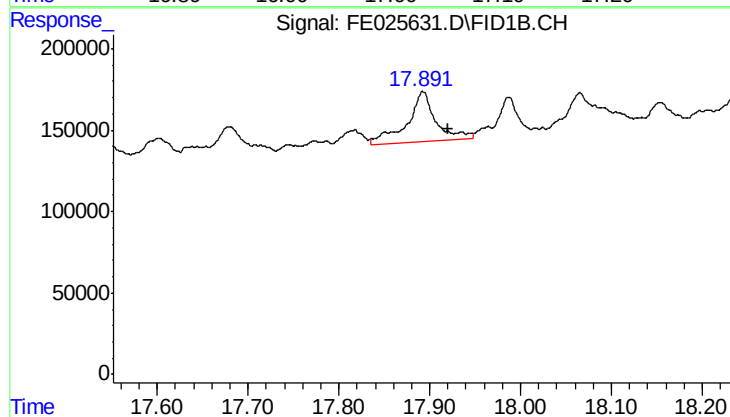

#13 N-TRIACONTANE


R.T.: 17.893 min
Delta R.T.: -0.028 min
Response: 671113
Conc: 4.25 ug/ml

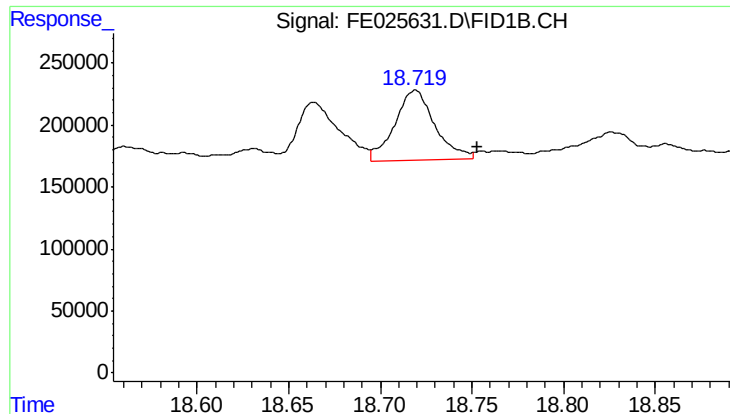

#14 N-DOTRIACONTANE

R.T.: 18.719 min
Delta R.T.: -0.034 min
Response: 855032
Conc: 5.27 ug/ml

Instrument :
FID_E
ClientSampleId :

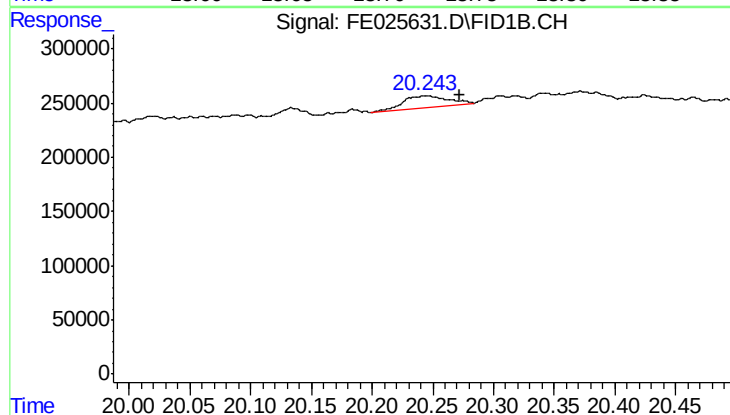

#16 N-HEXATRIACONTANE

R.T.: 20.245 min
Delta R.T.: -0.027 min
Response: 278370
Conc: 2.09 ug/ml