

Data Path : P:\HPCHEM1\FID_E\Data\FE011518\
 Data File : FE025635.D
 Signal(s) : FID1B.CH
 Acq On : 16 Jan 2018 11:31
 Operator : UA/AJ
 Sample : J1115-14 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 16 13:22:37 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
 Quant Title :
 QLast Update : Fri Jan 12 18:22:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.832	657155	3.613 ug/ml
Target Compounds			
4) N-TETRADECANE	8.466f	314381	1.725 ug/ml
7) N-EICOSANE	12.718	415034	1.872 ug/ml
8) N-DOCOSANE	14.017f	372747	1.699 ug/ml
10) N-TETRACOSANE	15.079	1016825	4.768 ug/ml
12) N-OCTACOSANE	17.044	240230	1.429 ug/ml
13) N-TRIACONTANE	17.891	581067	3.680 ug/ml
14) N-DOTRIACONTANE	18.723	277284	1.710 ug/ml
16) N-HEXATRIACONTANE	20.253	61140	0.460 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE011518\
Data File : FE025635.D
Signal(s) : FID1B.CH
Acq On : 16 Jan 2018 11:31
Operator : UA/AJ
Sample : J1115-14 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 13:22:37 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE011218.M
Quant Title :
QLast Update : Fri Jan 12 18:22:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

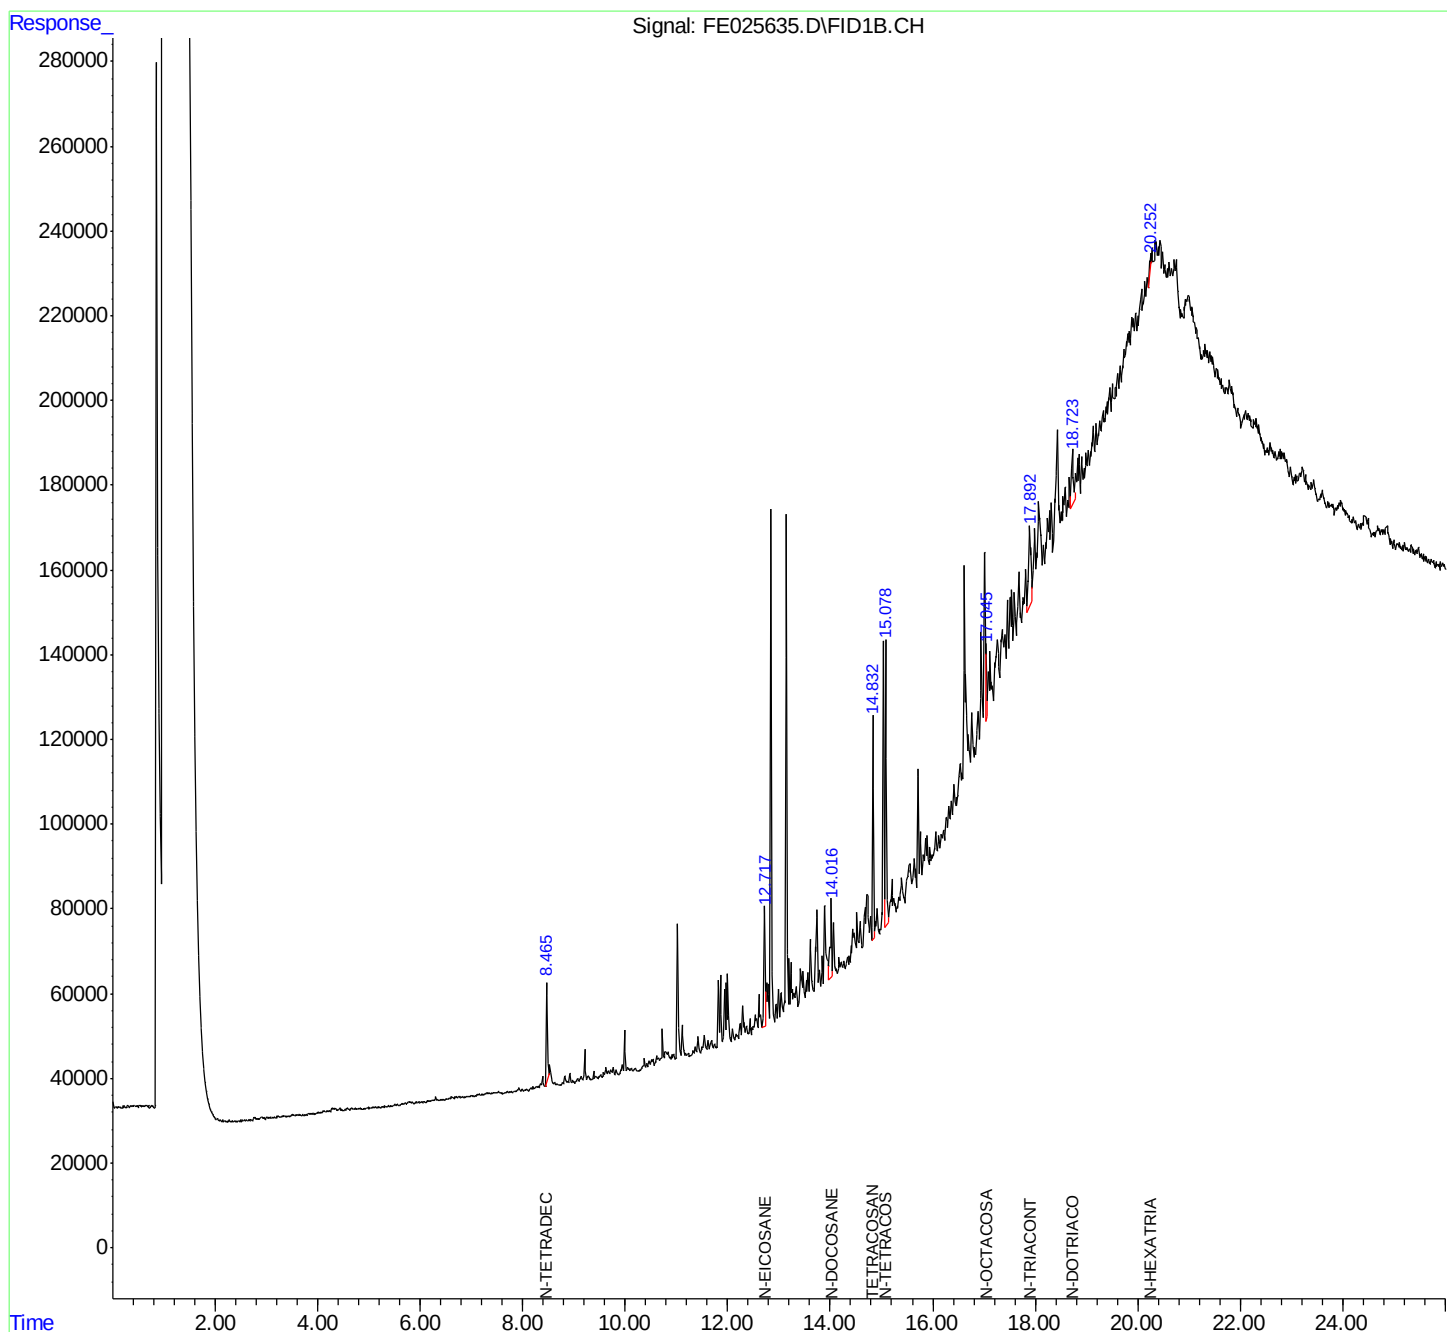


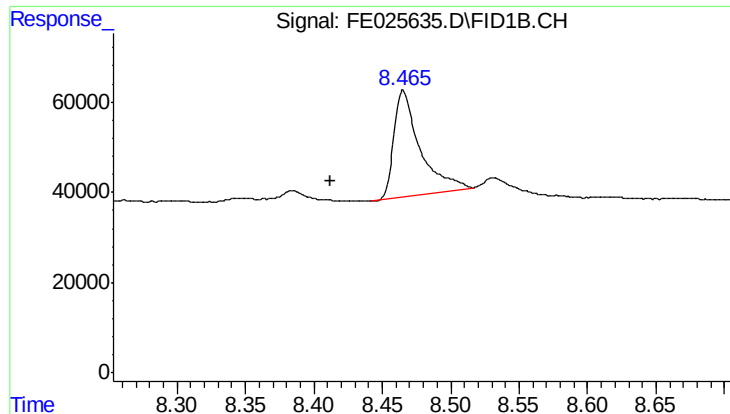

#4 N-TETRADECANE


R.T.: 8.466 min
Delta R.T.: 0.054 min
Response: 314381
Conc: 1.73 ug/ml

Instrument :
FID_E
ClientSampleId :

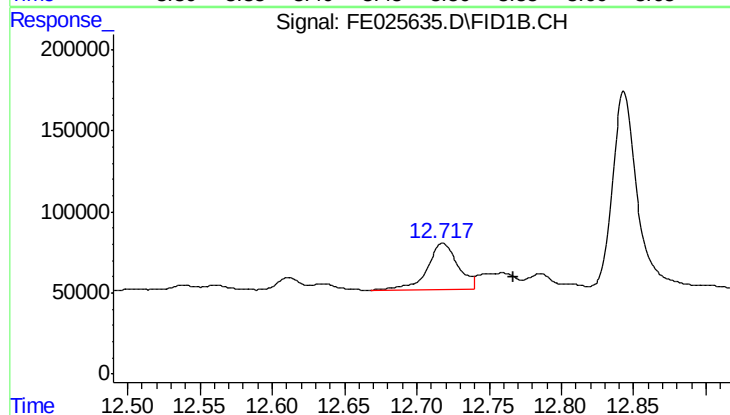


#7 N-EICOSANE

R.T.: 12.718 min
Delta R.T.: -0.048 min
Response: 415034
Conc: 1.87 ug/ml

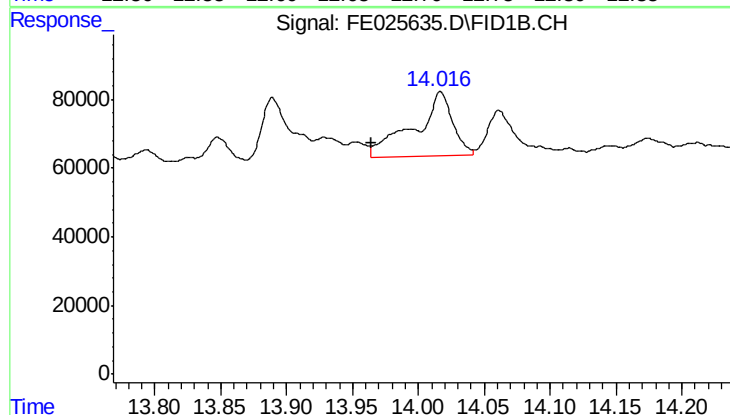


#8 N-DOCOSANE

R.T.: 14.017 min
Delta R.T.: 0.053 min
Response: 372747
Conc: 1.70 ug/ml

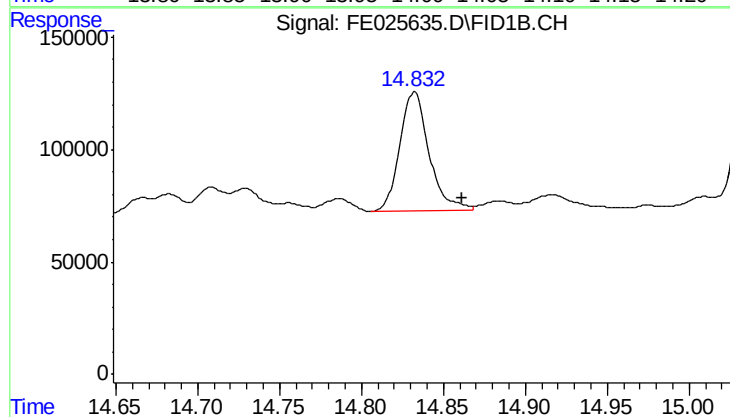

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.832 min
Delta R.T.: -0.029 min
Response: 657155
Conc: 3.61 ug/ml

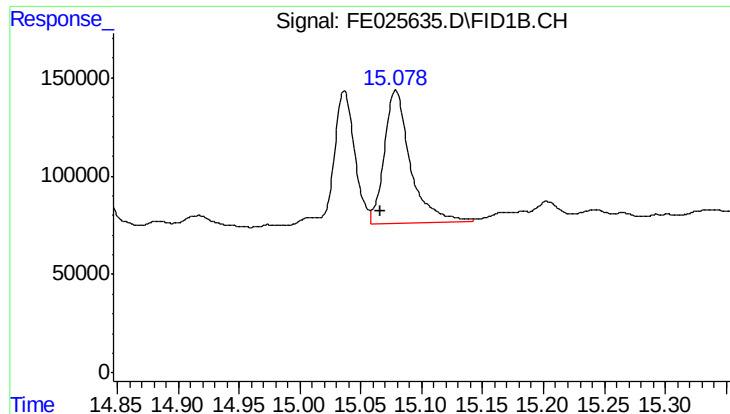

#10 N-TETRACOSANE


R.T.: 15.079 min
Delta R.T.: 0.012 min
Response: 1016825
Conc: 4.77 ug/ml

Instrument :
FID_E
ClientSampleId :

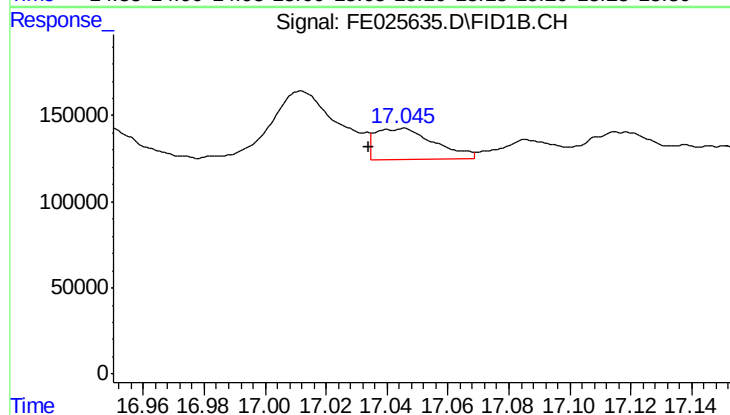


#12 N-OCTACOSANE

R.T.: 17.044 min
Delta R.T.: 0.010 min
Response: 240230
Conc: 1.43 ug/ml

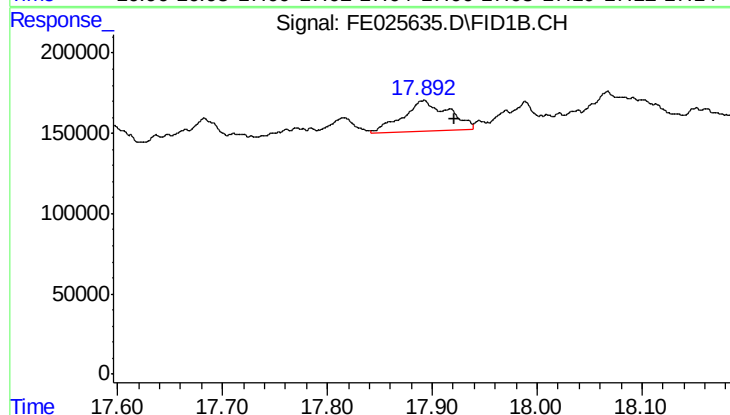


#13 N-TRIACONTANE

R.T.: 17.891 min
Delta R.T.: -0.030 min
Response: 581067
Conc: 3.68 ug/ml

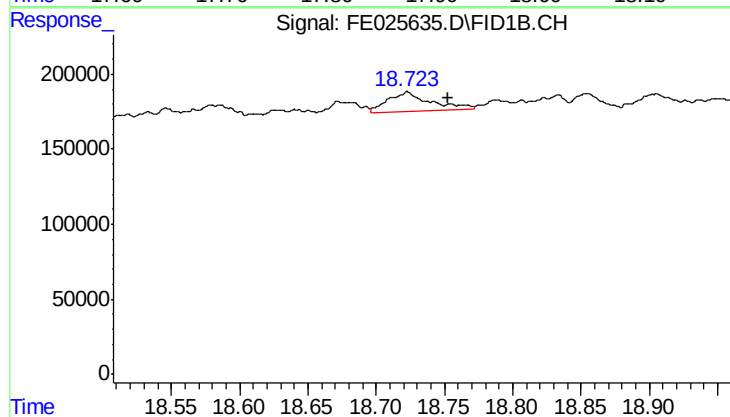

#14 N-DOTRIACONTANE

R.T.: 18.723 min
Delta R.T.: -0.030 min
Response: 277284
Conc: 1.71 ug/ml

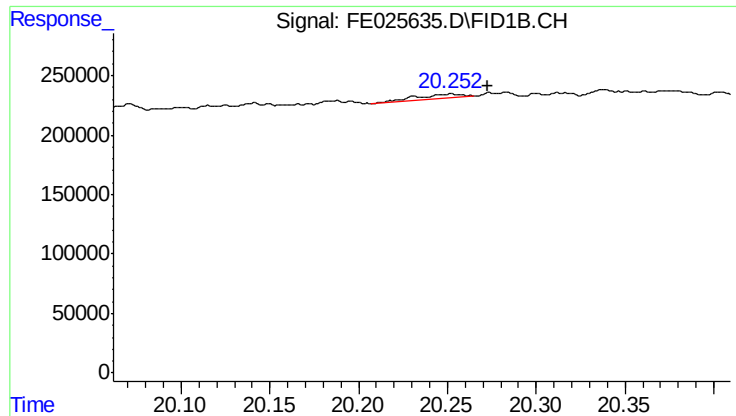

#16 N-HEXATRIACONTANE

R.T.: 20.253 min
Delta R.T.: -0.019 min
Response: 61140
Conc: 0.46 ug/ml

Instrument :
FID_E
ClientSampleId :