

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE011519\  
 Data File : FE029452.D  
 Signal(s) : FID1B.CH  
 Acq On : 15 Jan 2019 15:11  
 Operator : AJ\SJ  
 Sample : K1139-08  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e  
 Quant Time: Jan 16 01:30:52 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE010419.M  
 Quant Title :  
 QLast Update : Fri Jan 04 15:40:11 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.824	2896259	15.104 ug/ml
Target Compounds			
6) N-TETRADECANE	8.435	1139815	6.013 ug/ml
7) N-HEXADECANE	9.958	40025	0.210 ug/ml
8) N-OCTADECANE	11.494	38608	0.202 ug/ml
10) N-TETRACOSANE	15.056	352391	1.857 ug/ml
11) N-OCTACOSANE	17.000	331588	1.776 ug/ml
12) N-DOTRIACONTANE	18.725	355336	2.138 ug/ml
14) N-HEXATRIACONTANE	20.252	159482	1.565 ug/ml
-----			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE011519\  
Data File : FE029452.D  
Signal(s) : FID1B.CH  
Acq On : 15 Jan 2019 15:11  
Operator : AJ\SJ  
Sample : K1139-08  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Integration File: autoint1.e  
Quant Time: Jan 16 01:30:52 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE010419.M  
Quant Title :  
QLast Update : Fri Jan 04 15:40:11 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

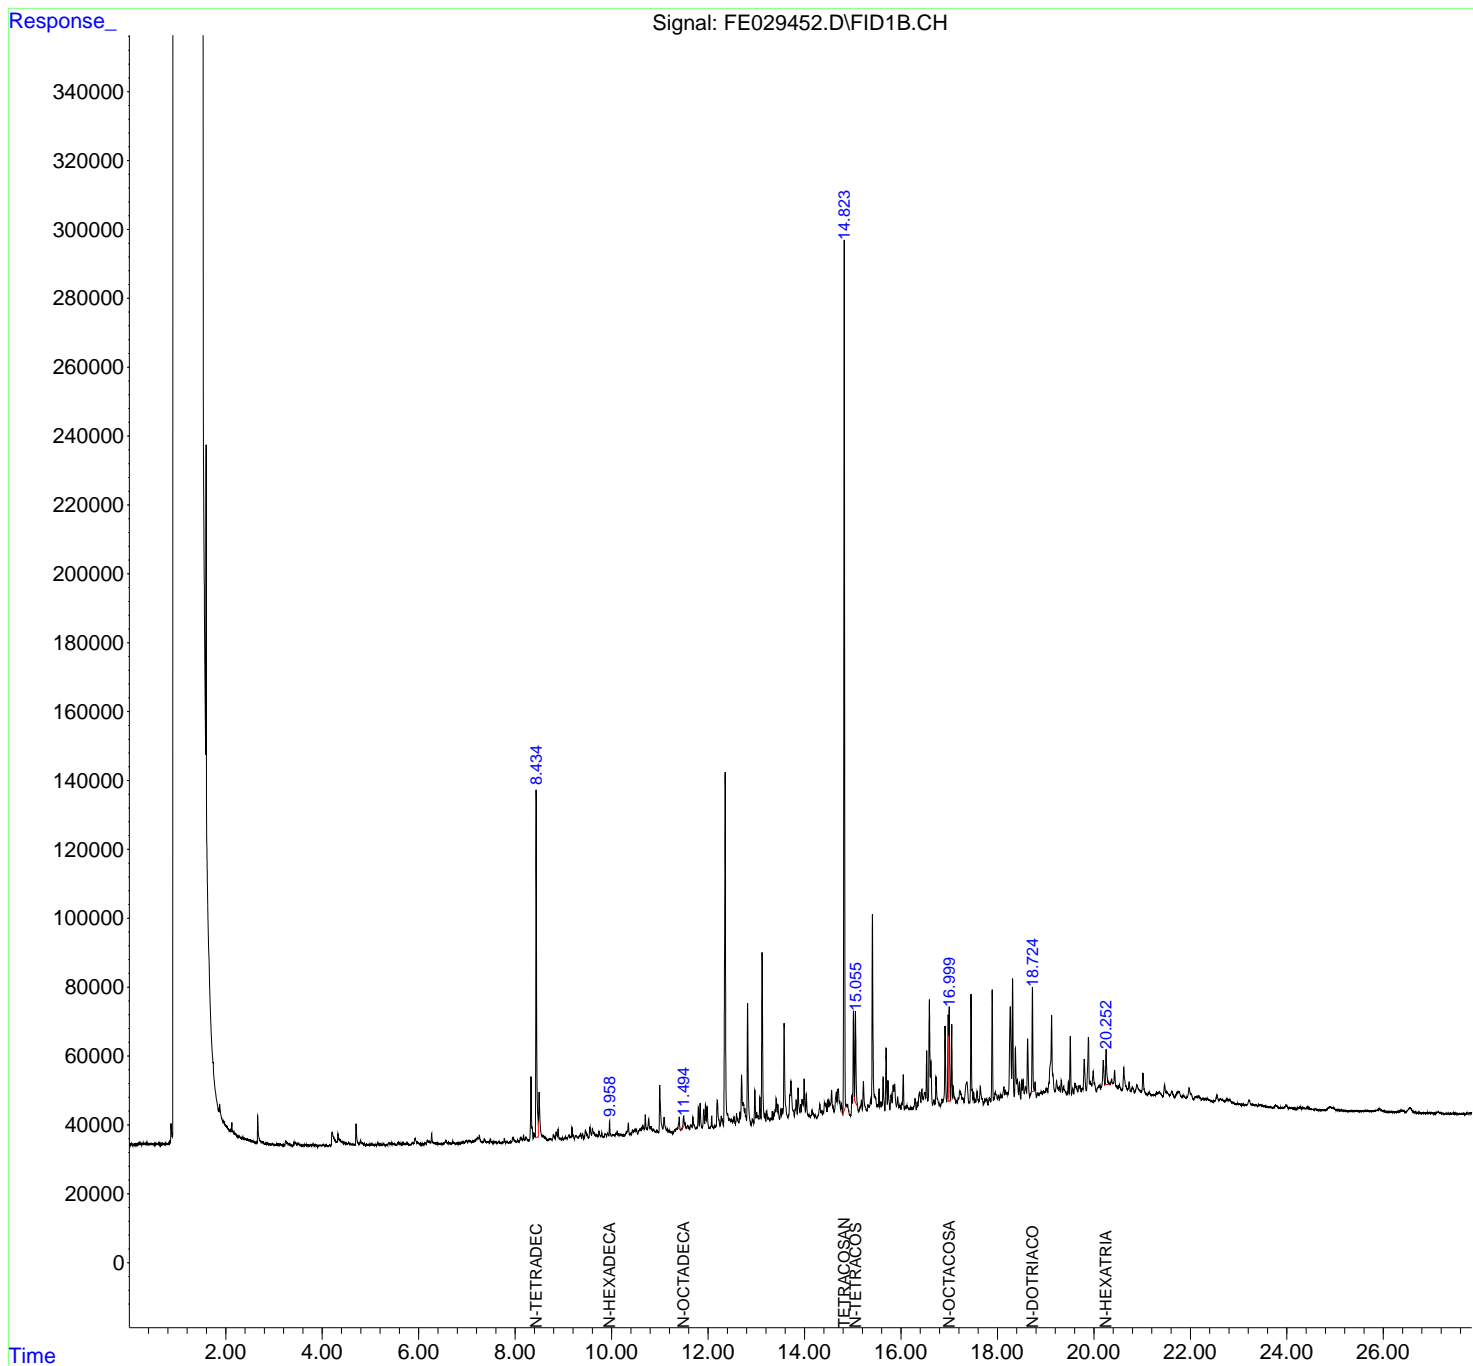


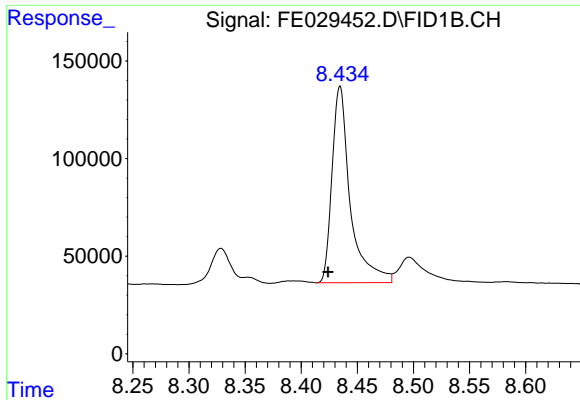


#6 N-TETRADECANE  
R.T.: 8.435 min  
Delta R.T.: 0.011 min  
Response: 1139815  
Conc: 6.01 ug/ml

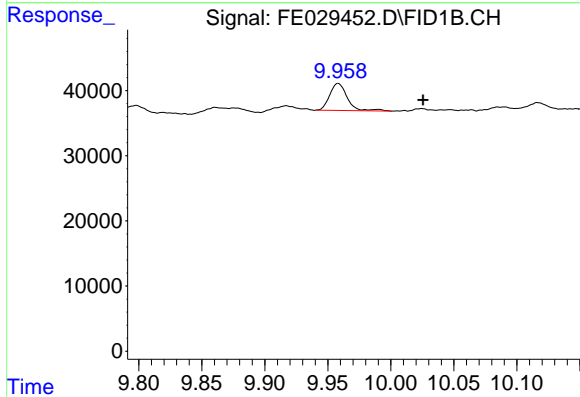


#7 N-HEXADECANE  
R.T.: 9.958 min  
Delta R.T.: -0.067 min  
Response: 40025  
Conc: 0.21 ug/ml

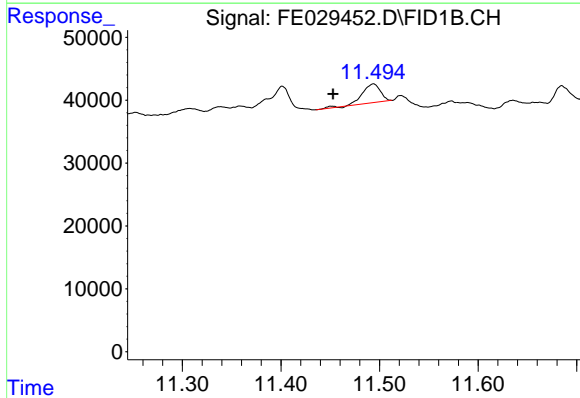

#8 N-OCTADECANE  
R.T.: 11.494 min  
Delta R.T.: 0.041 min  
Response: 38608  
Conc: 0.20 ug/ml

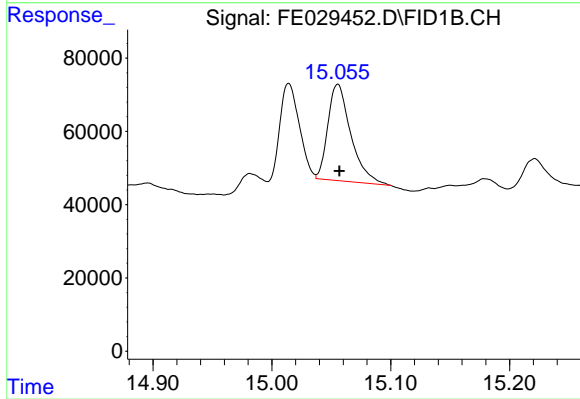


#10 N-TETRACOSANE  
R.T.: 15.056 min  
Delta R.T.: -0.001 min  
Response: 352391  
Conc: 1.86 ug/ml

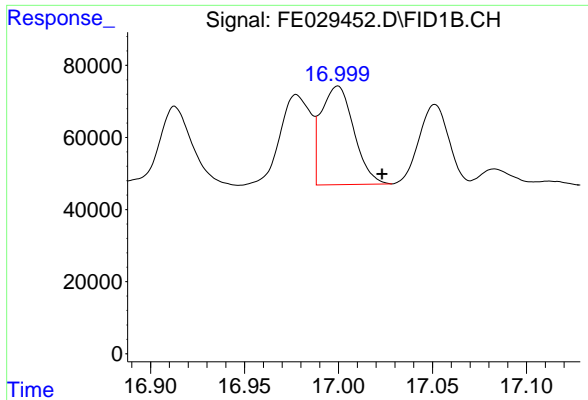


#11 N-OCTACOSANE

R.T.: 17.000 min  
Delta R.T.: -0.024 min  
Response: 331588  
Conc: 1.78 ug/ml

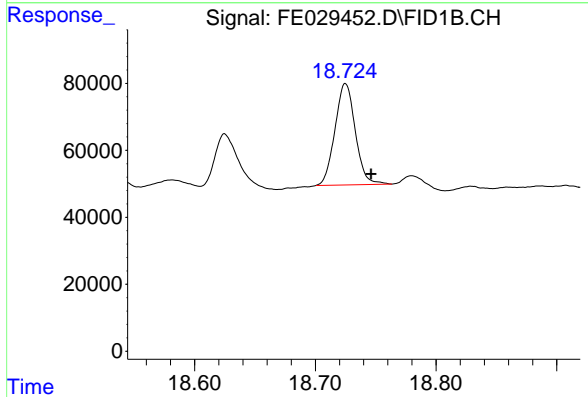


#12 N-DOTRIACONTANE

R.T.: 18.725 min  
Delta R.T.: -0.021 min  
Response: 355336  
Conc: 2.14 ug/ml

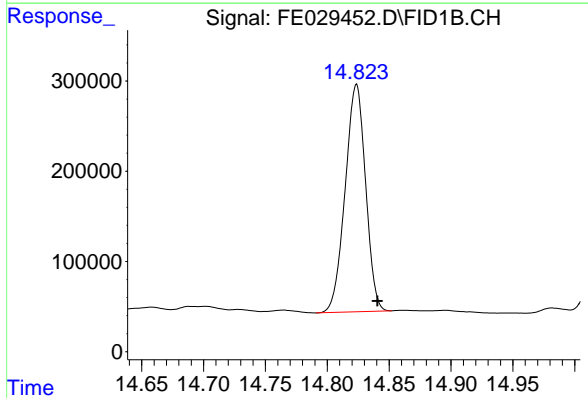

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.824 min  
Delta R.T.: -0.017 min  
Response: 2896259  
Conc: 15.10 ug/ml

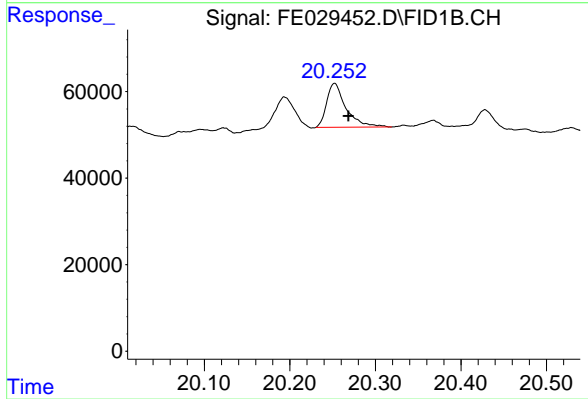

#14 N-HEXATRIACONTANE

R.T.: 20.252 min  
Delta R.T.: -0.016 min  
Response: 159482  
Conc: 1.57 ug/ml