

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011520\
 Data File : FE031132.D
 Signal(s) : FID1B.CH
 Acq On : 15 Jan 2020 17:33
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 16 00:28:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	15711472	47.085 ug/ml
Target Compounds			
2) N-DECANE	4.371	19196031	51.089 ug/ml
3) N-DODECANE	6.381	19505574	55.267 ug/ml
4) N-TETRADECANE	8.176	19209845	50.239 ug/ml
5) N-HEXADECANE	9.779	19021278	49.133 ug/ml
6) N-OCTADECANE	11.223	18538597	48.187 ug/ml
7) N-EICOSANE	12.535	18652650	47.941 ug/ml
8) N-DOCOSANE	13.736	18268616	47.304 ug/ml
10) N-TETRACOSANE	14.841	18009608	46.955 ug/ml
11) N-HEXACOSANE	15.863	17783119	46.493 ug/ml
12) N-OCTACOSANE	16.815	17798718	46.299 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011520\
Data File : FE031132.D
Signal(s) : FID1B.CH
Acq On : 15 Jan 2020 17:33
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 16 00:28:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

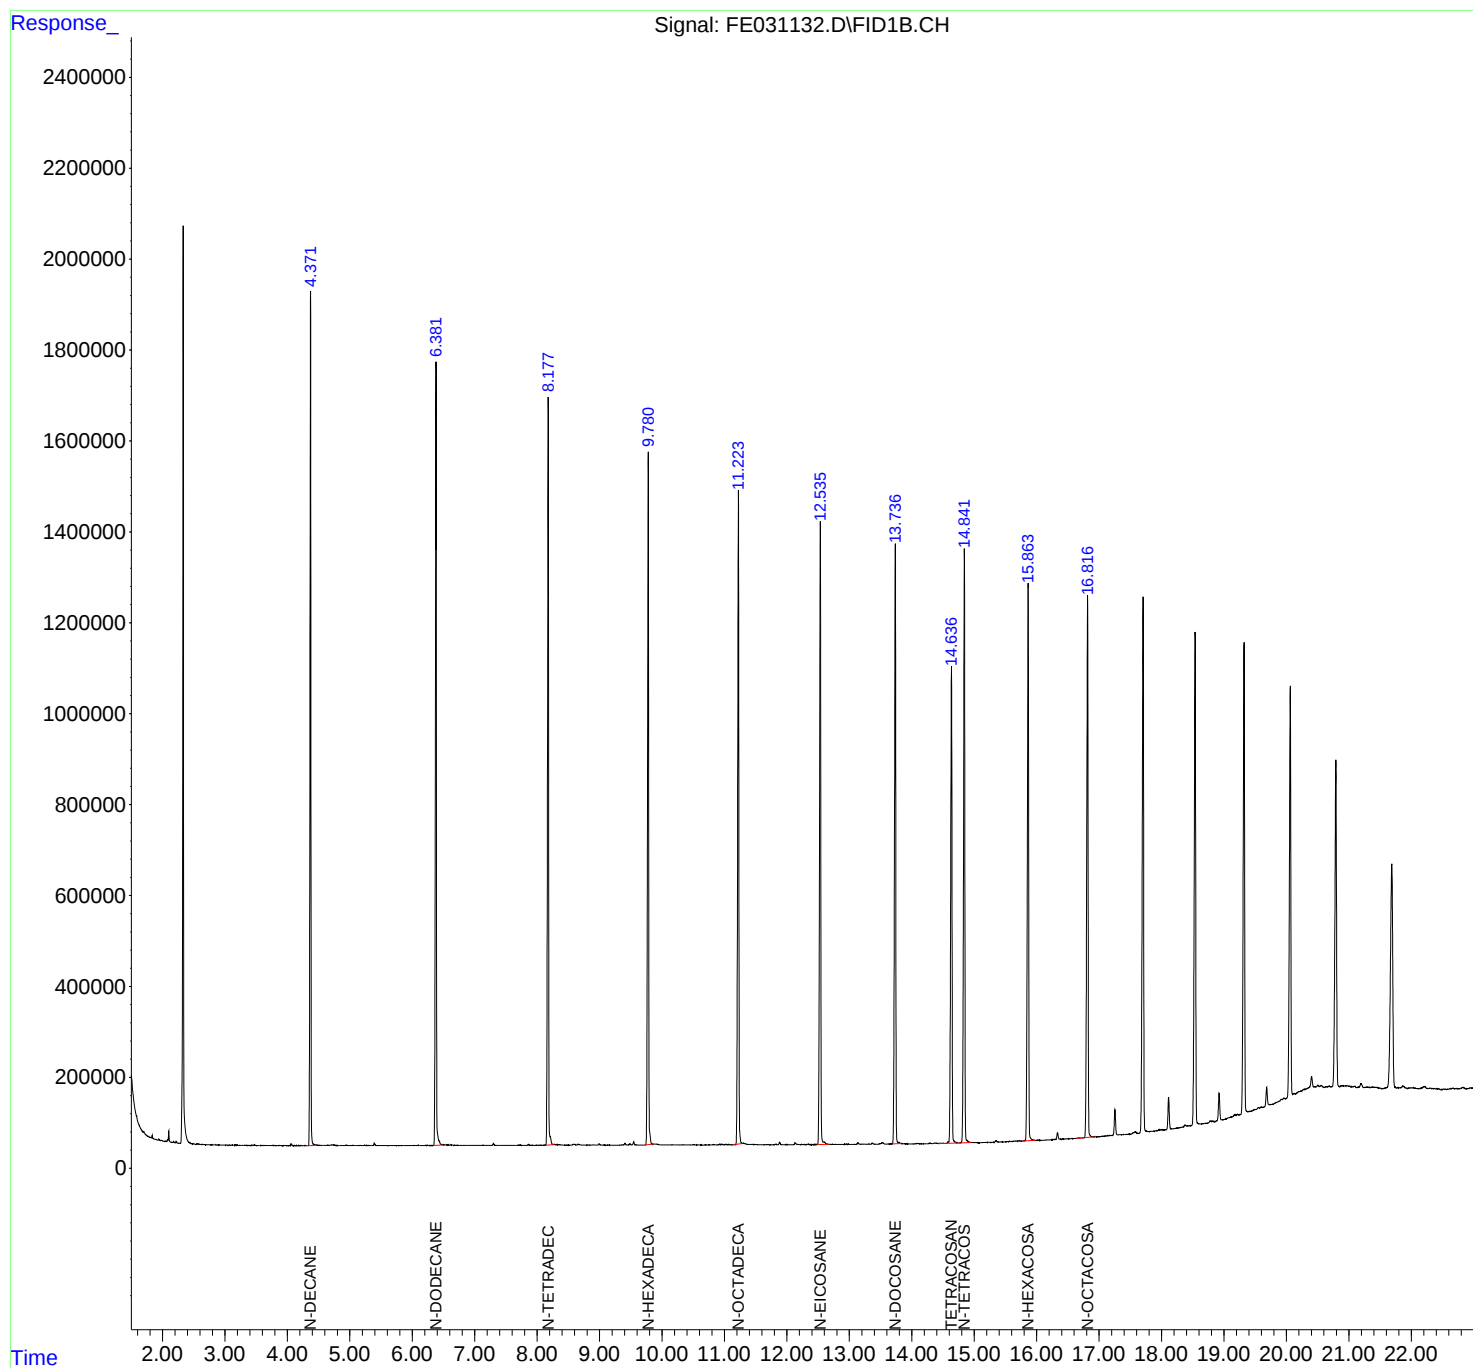

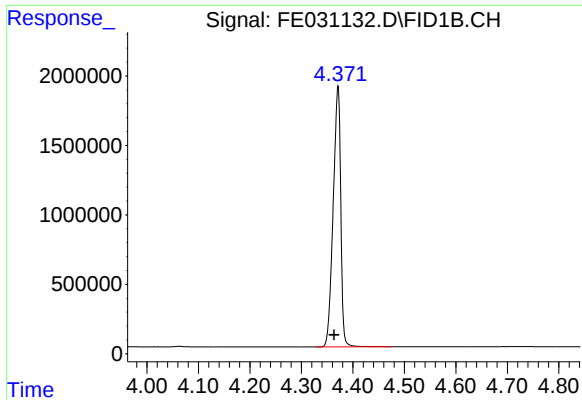


#2 N-DECANE

R.T.: 4.371 min
Delta R.T.: 0.007 min
Response: 19196031
Conc: 51.09 ug/ml

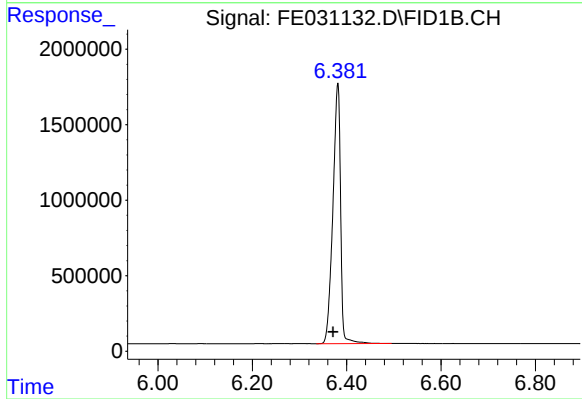


#3 N-DODECANE

R.T.: 6.381 min
Delta R.T.: 0.009 min
Response: 19505574
Conc: 55.27 ug/ml

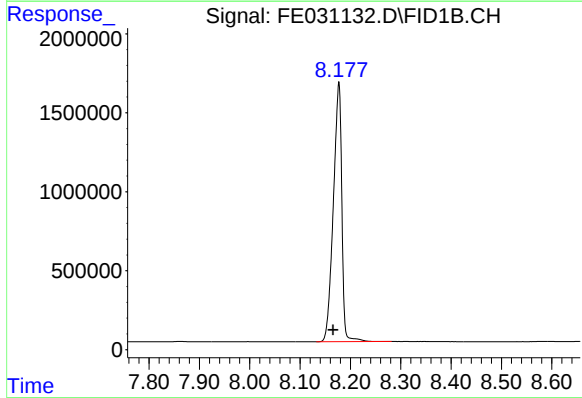


#4 N-TETRADECANE

R.T.: 8.176 min
Delta R.T.: 0.011 min
Response: 19209845
Conc: 50.24 ug/ml

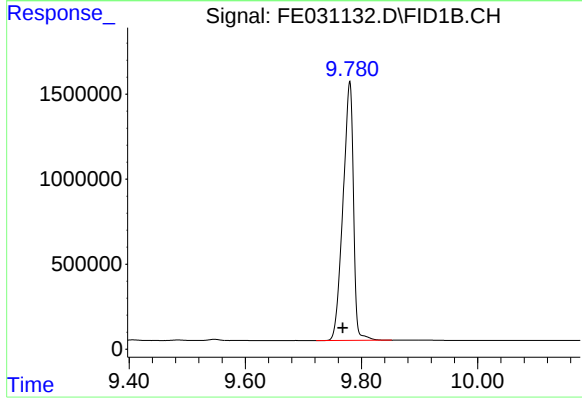


#5 N-HEXADECANE

R.T.: 9.779 min
Delta R.T.: 0.011 min
Response: 19021278
Conc: 49.13 ug/ml

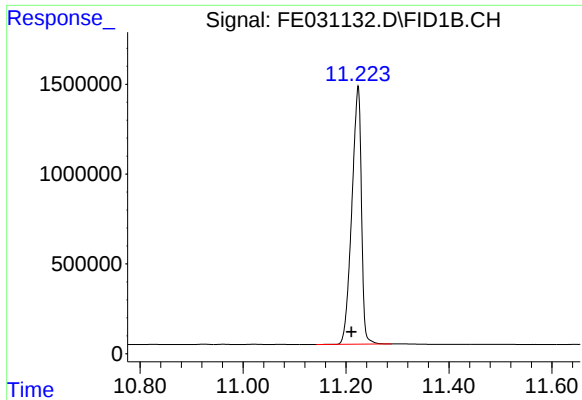


#6 N-OCTADECANE

R.T.: 11.223 min
Delta R.T.: 0.013 min
Response: 18538597
Conc: 48.19 ug/ml

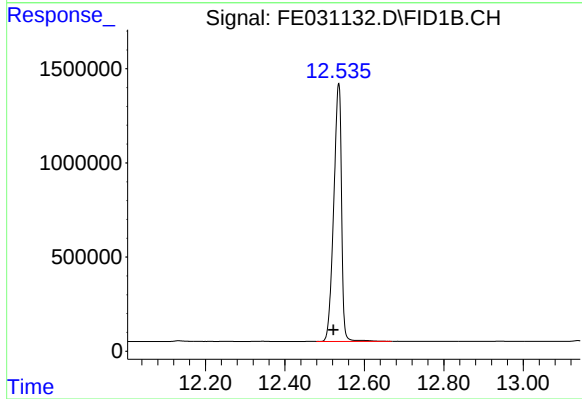


#7 N-EICOSANE

R.T.: 12.535 min
Delta R.T.: 0.013 min
Response: 18652650
Conc: 47.94 ug/ml

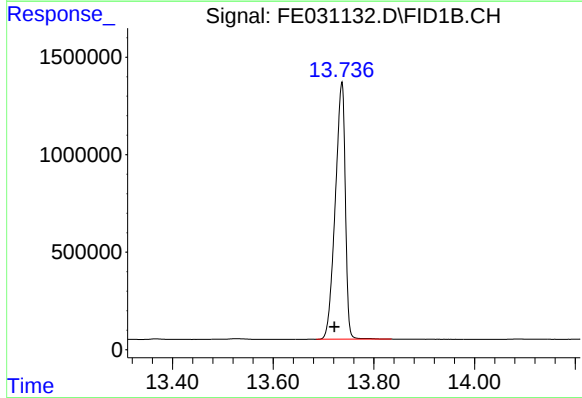


#8 N-DOCOSANE

R.T.: 13.736 min
Delta R.T.: 0.014 min
Response: 18268616
Conc: 47.30 ug/ml

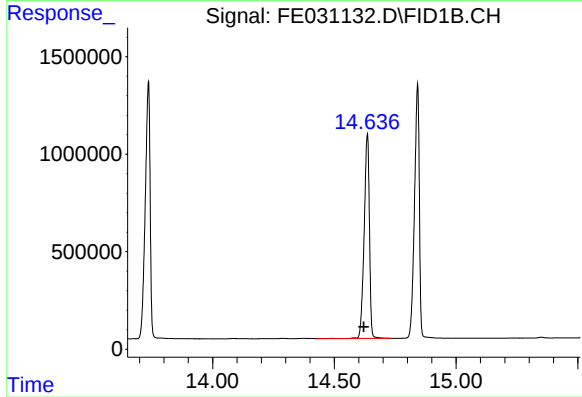


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min
Delta R.T.: 0.014 min
Response: 15711472
Conc: 47.08 ug/ml

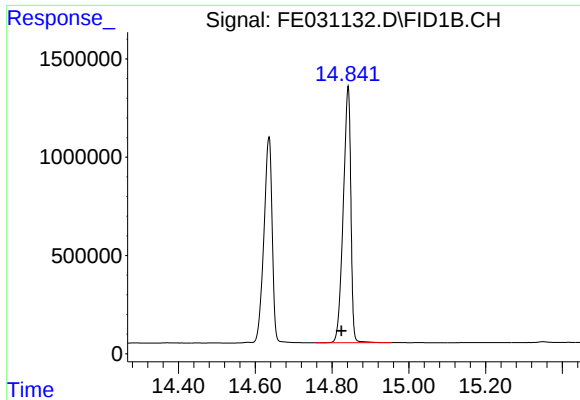


#10 N-TETRACOSANE

R.T.: 14.841 min
Delta R.T.: 0.016 min
Response: 18009608
Conc: 46.96 ug/ml

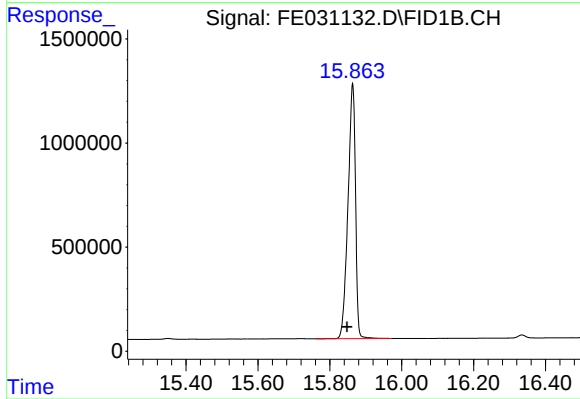

#11 N-HEXACOSANE

R.T.: 15.863 min
Delta R.T.: 0.015 min
Response: 17783119
Conc: 46.49 ug/ml

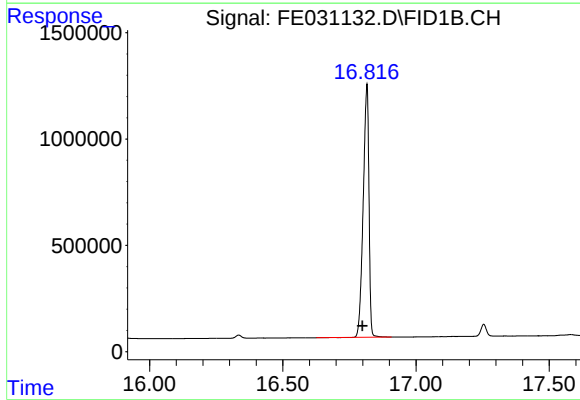

#12 N-OCTACOSANE

R.T.: 16.815 min
Delta R.T.: 0.016 min
Response: 17798718
Conc: 46.30 ug/ml