

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011524AL\
Data File : FE046215.D
Signal(s) : FID1B.ch
Acq On : 15 Jan 2024 09:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 02:32:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.005	8437	0.057 ug/ml
18) T	n-Dotriacontane (C32)	18.850	14135	0.095 ug/ml
21) T	n-Octatriacontane (C38)	21.122	33235	0.225 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011524AL\
Data File : FE046215.D
Signal(s) : FID1B.ch
Acq On : 15 Jan 2024 09:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 02:32:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

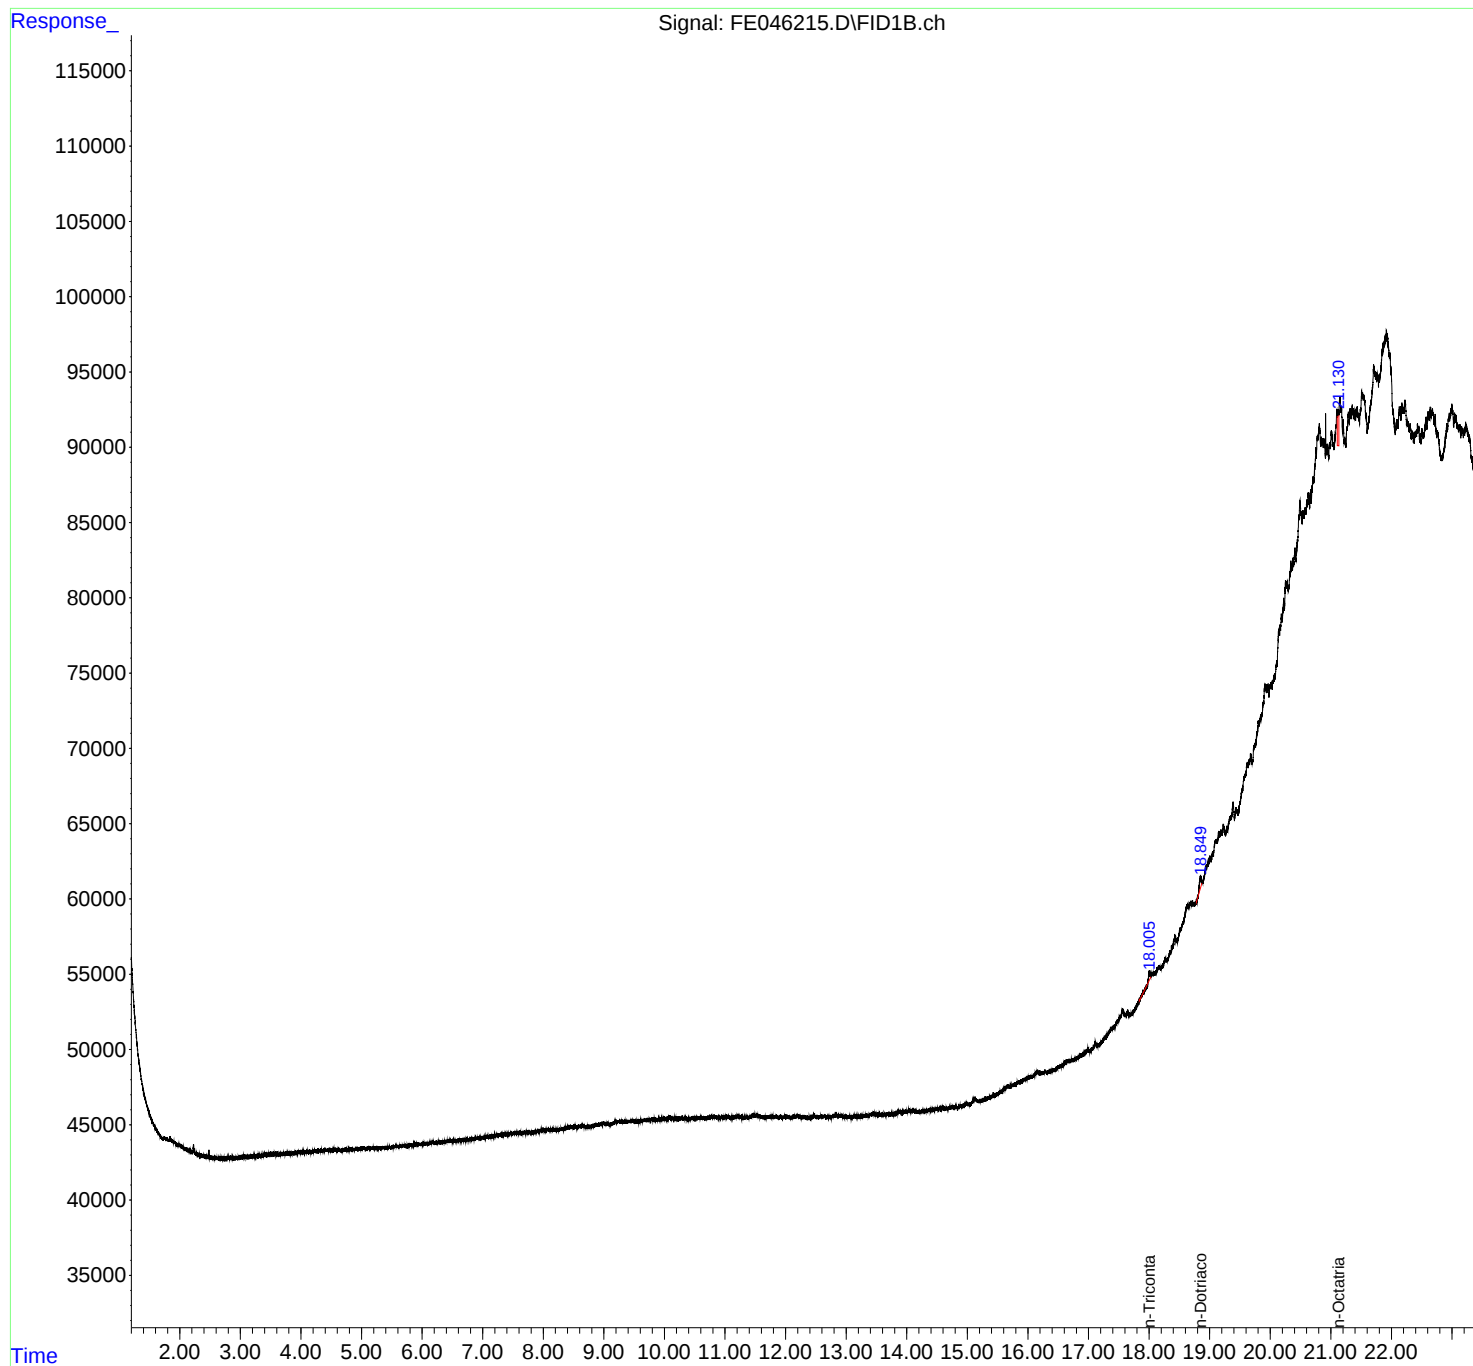


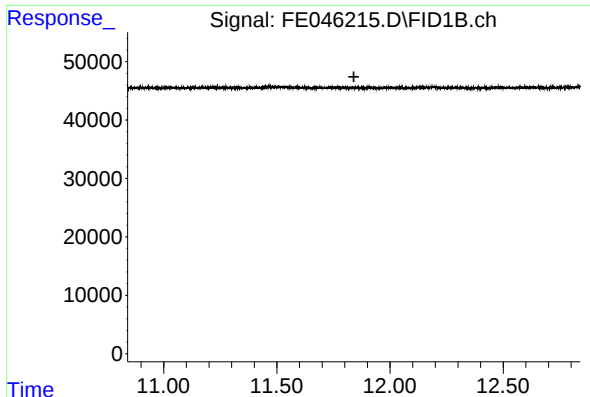

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

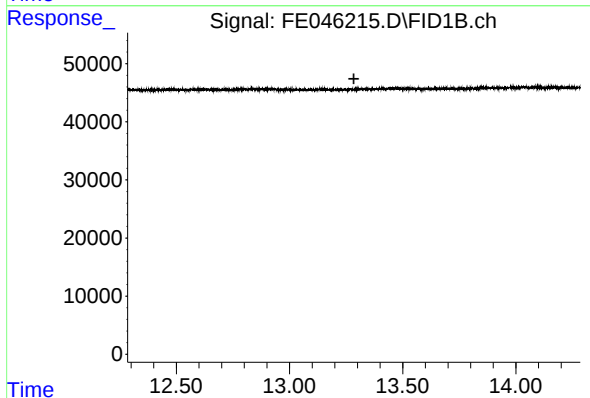


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

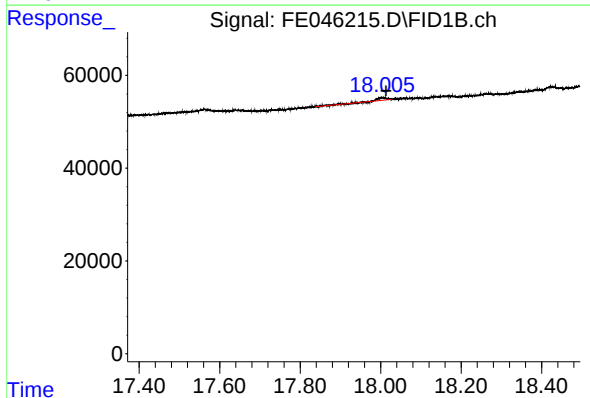


#17 n-Tricontane (C30)

R.T.: 18.005 min
Delta R.T.: -0.009 min
Response: 8437
Conc: 0.06 ug/ml

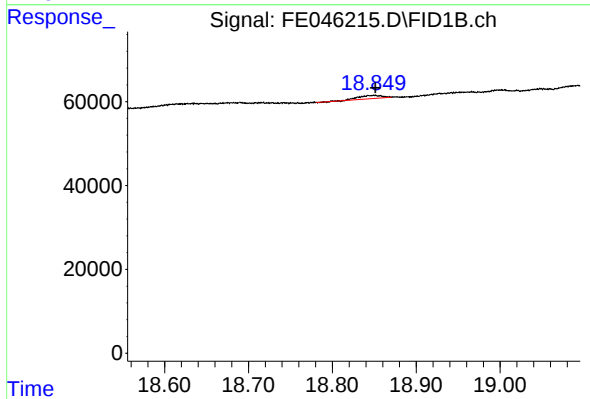

#18 n-Dotriacontane (C32)

R.T.: 18.850 min
Delta R.T.: -0.001 min
Response: 14135
Conc: 0.09 ug/ml

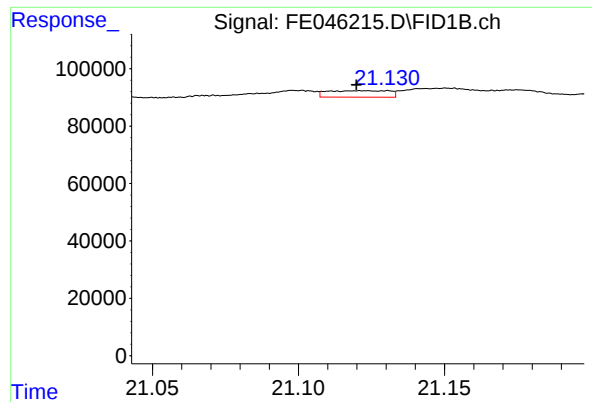

#21 n-Octatriacontane (C38)

R.T.: 21.122 min
Delta R.T.: 0.002 min
Response: 33235
Conc: 0.23 ug/ml

Instrument :
FID_E
ClientSampleId :