

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011524AL\
Data File : FE046242.D
Signal(s) : FID1B.ch
Acq On : 16 Jan 2024 00:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 02:38:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	17.996	20200	0.136 ug/ml
18) T	n-Dotriacontane (C32)	18.832	42658	0.285 ug/ml
19) T	n-Tetratriacontane (C34)	19.620	21739	0.152 ug/ml
21) T	n-Octatriacontane (C38)	21.160	7247	0.049 ug/ml
22) T	n-Tetracontane (C40)	21.965f	32699	0.209 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011524AL\
Data File : FE046242.D
Signal(s) : FID1B.ch
Acq On : 16 Jan 2024 00:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 16 02:38:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

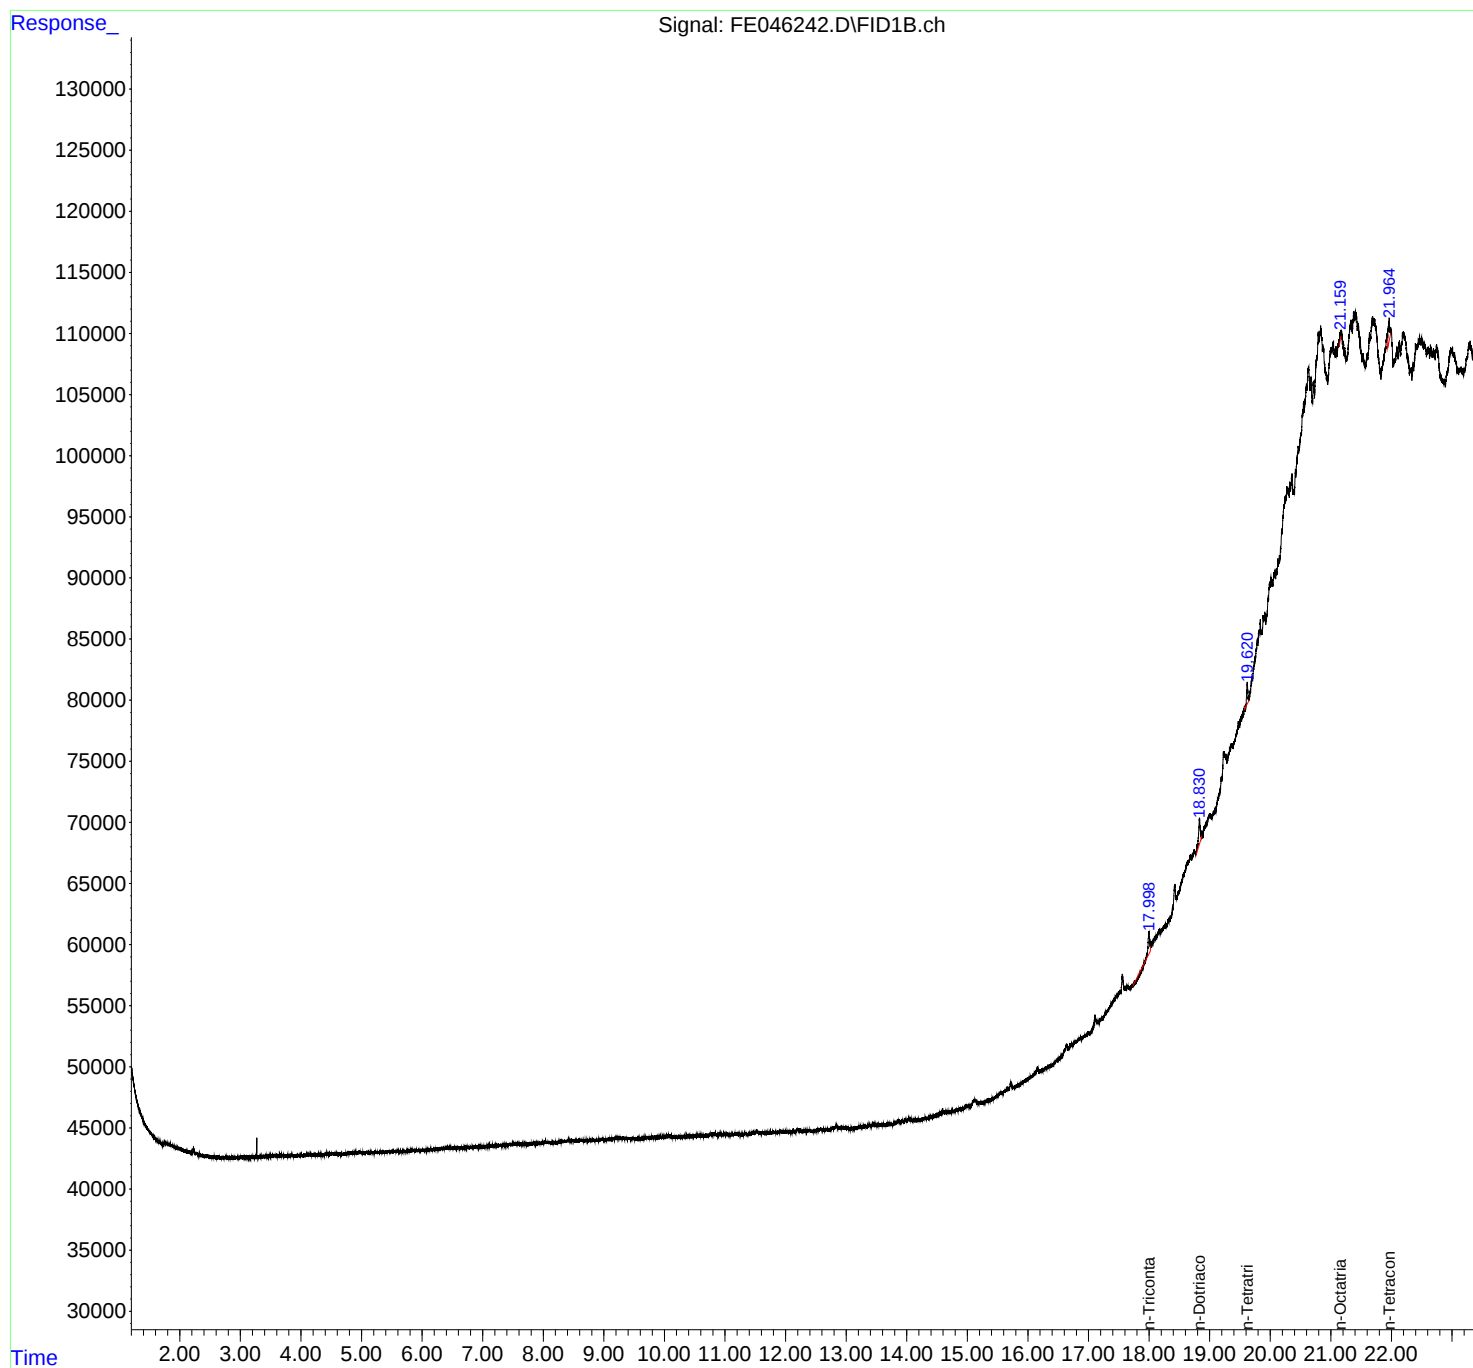


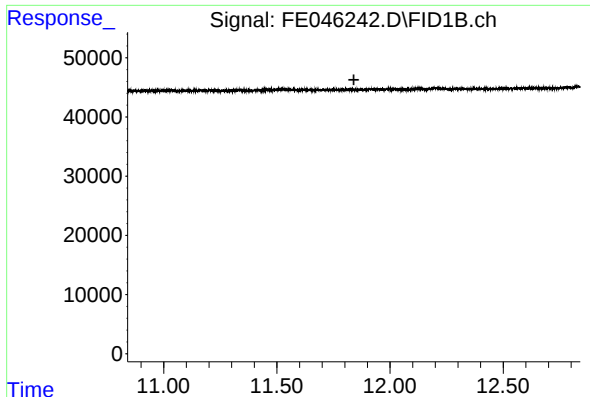

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

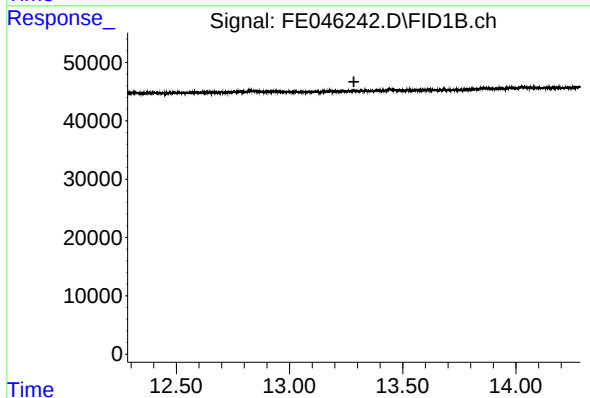


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

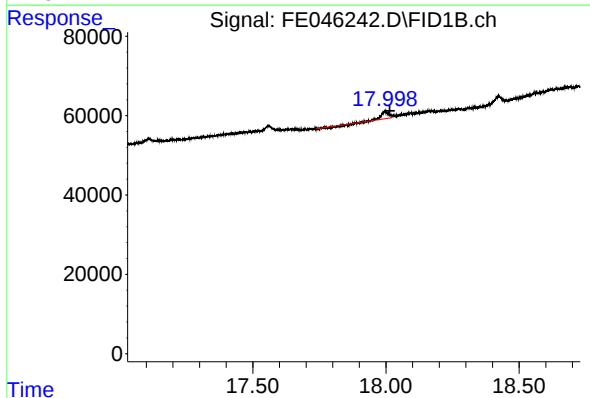


#17 n-Tricontane (C30)

R.T.: 17.996 min
Delta R.T.: -0.018 min
Response: 20200
Conc: 0.14 ug/ml

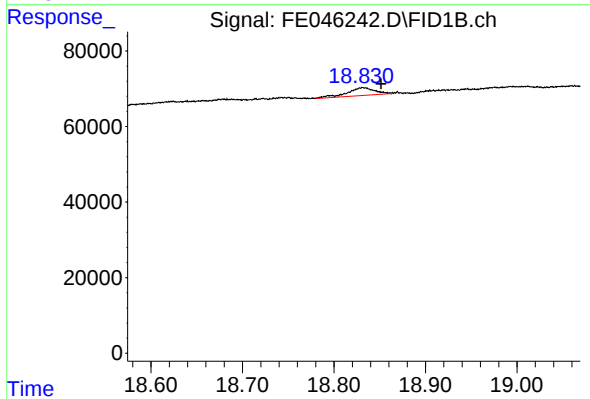

#18 n-Dotriacontane (C32)


R.T.: 18.832 min
Delta R.T.: -0.019 min
Response: 42658
Conc: 0.29 ug/ml

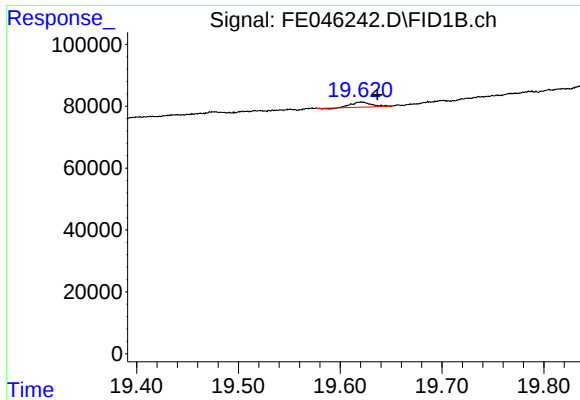

#19 n-Tetratriacontane (C34)


R.T.: 19.620 min
Delta R.T.: -0.016 min
Response: 21739
Conc: 0.15 ug/ml

Instrument :
FID_E
ClientSampleId :

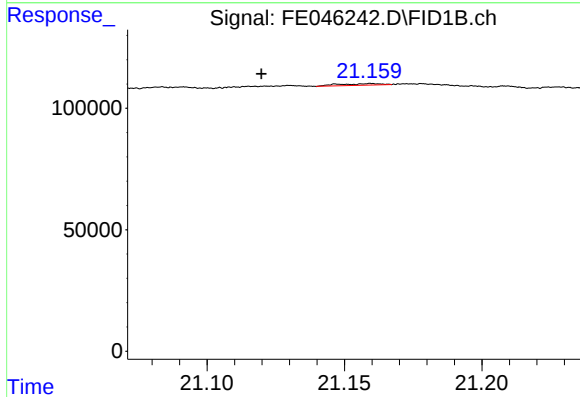

#21 n-Octatriacontane (C38)

R.T.: 21.160 min
Delta R.T.: 0.040 min
Response: 7247
Conc: 0.05 ug/ml

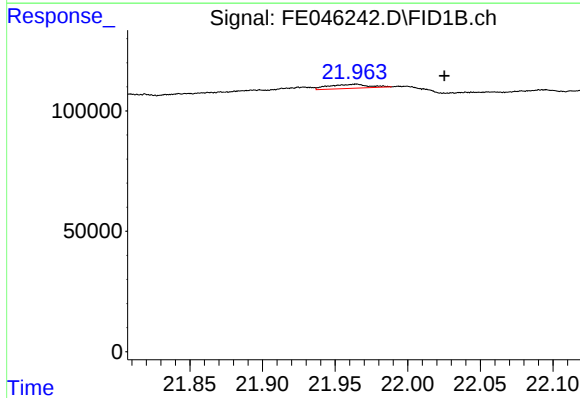

#22 n-Tetracontane (C40)

R.T.: 21.965 min
Delta R.T.: -0.061 min
Response: 32699
Conc: 0.21 ug/ml