

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011624AL\
 Data File : FE046244.D
 Signal(s) : FID1B.ch
 Acq On : 16 Jan 2024 09:25
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 17 01:16:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:49:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.001	27796	0.187 ug/ml
18) T n-Dotriacontane (C32)	18.836	35927	0.240 ug/ml
19) T n-Tetratriacontane (C34)	19.620	44615	0.311 ug/ml
22) T n-Tetracontane (C40)	21.983	51503	0.329 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011624AL\
Data File : FE046244.D
Signal(s) : FID1B.ch
Acq On : 16 Jan 2024 09:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 01:16:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

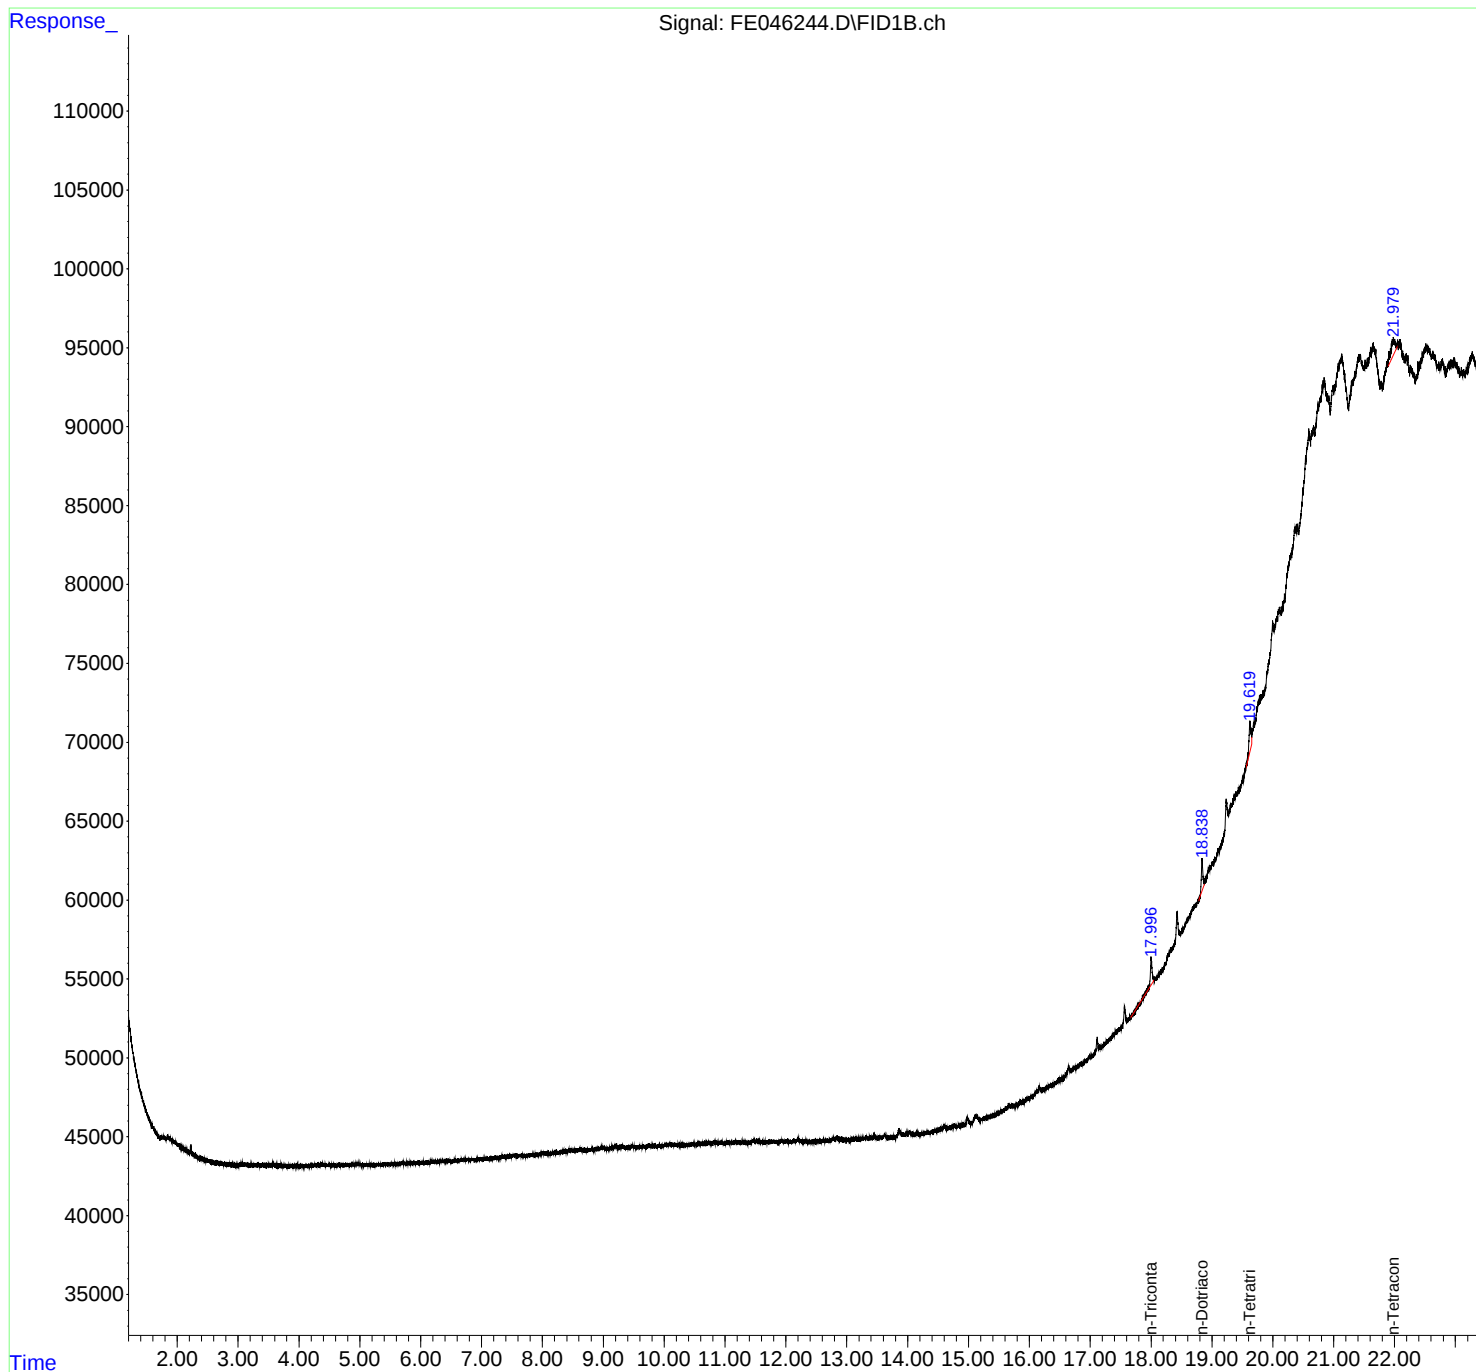


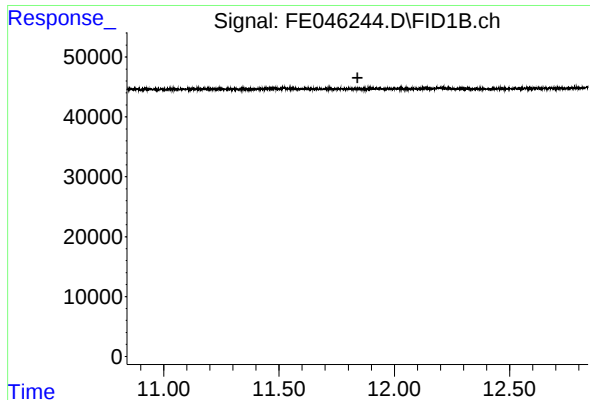

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

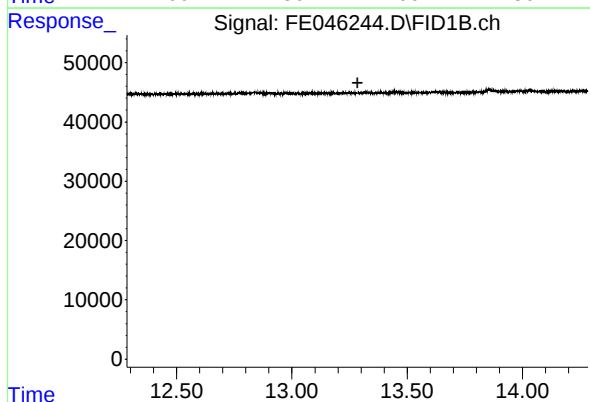


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

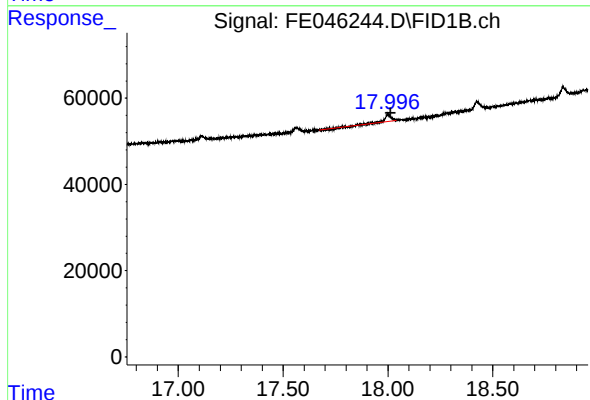


#17 n-Tricontane (C30)

R.T.: 18.001 min
Delta R.T.: -0.013 min
Response: 27796
Conc: 0.19 ug/ml

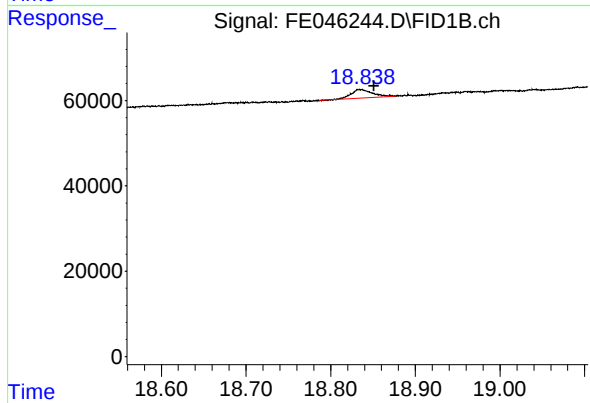

#18 n-Dotriacontane (C32)


R.T.: 18.836 min
Delta R.T.: -0.016 min
Response: 35927
Conc: 0.24 ug/ml

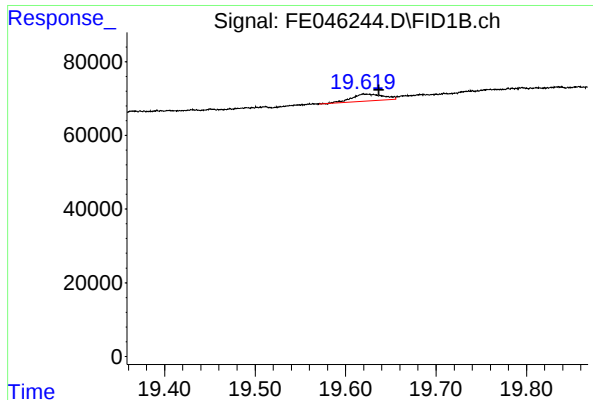

#19 n-Tetratriacontane (C34)

R.T.: 19.620 min
Delta R.T.: -0.017 min
Response: 44615
Conc: 0.31 ug/ml

Instrument :
FID_E
ClientSampleId :

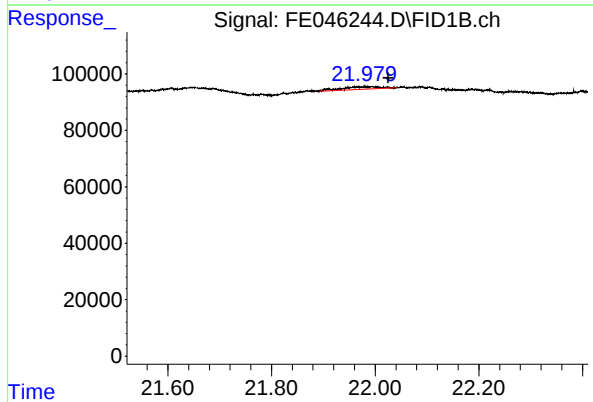

#22 n-Tetracontane (C40)

R.T.: 21.983 min
Delta R.T.: -0.043 min
Response: 51503
Conc: 0.33 ug/ml