

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011624AL\
Data File : FE046249.D
Signal(s) : FID1B.ch
Acq On : 16 Jan 2024 11:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 01:17:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.999	32598	0.219 ug/ml
18) T	n-Dotriacontane (C32)	18.837	40721	0.272 ug/ml
19) T	n-Tetratriacontane (C34)	19.622	28530	0.199 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011624AL\
Data File : FE046249.D
Signal(s) : FID1B.ch
Acq On : 16 Jan 2024 11:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 17 01:17:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

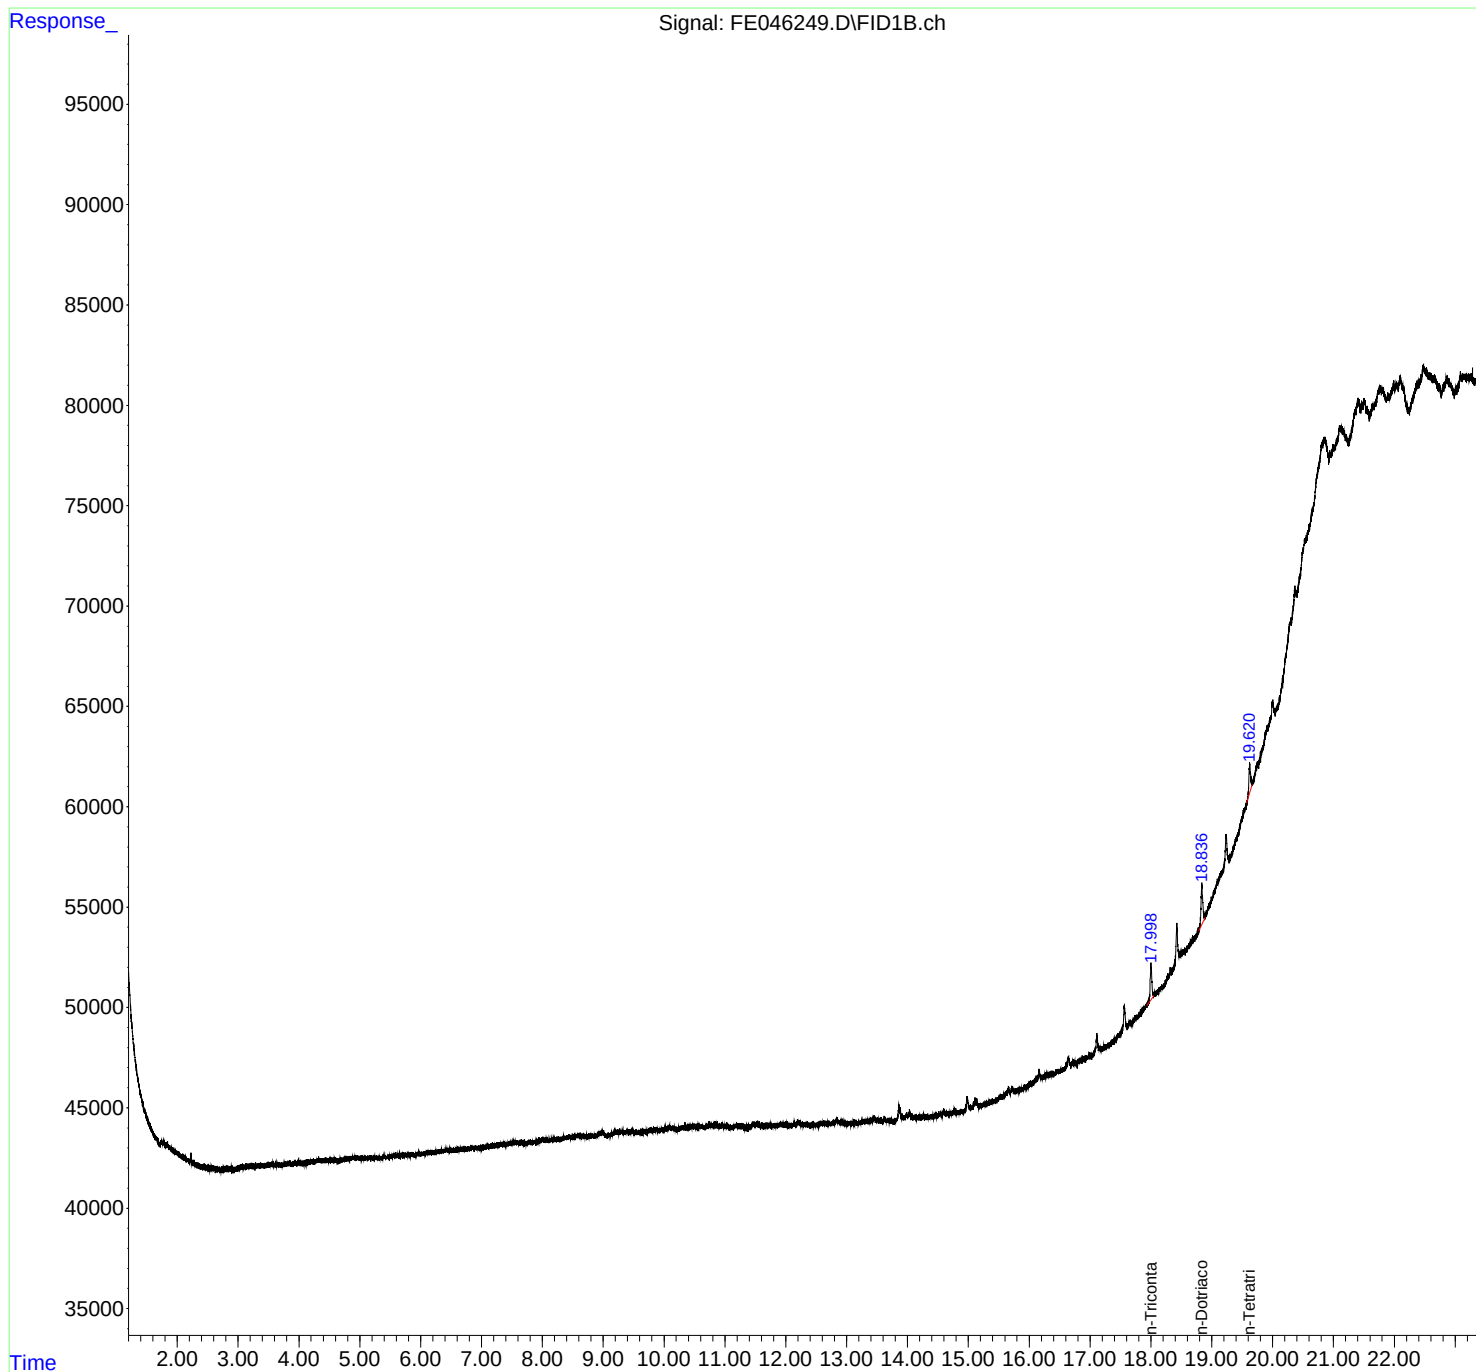


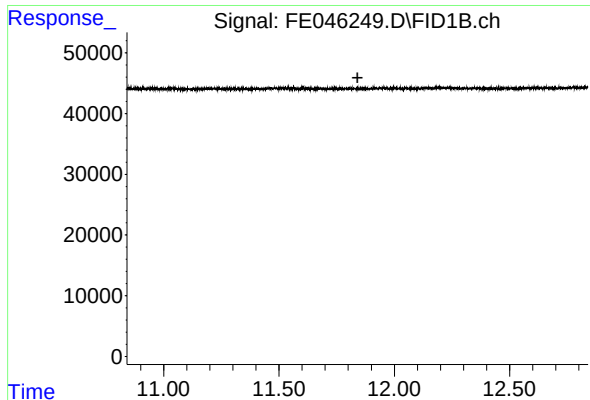

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

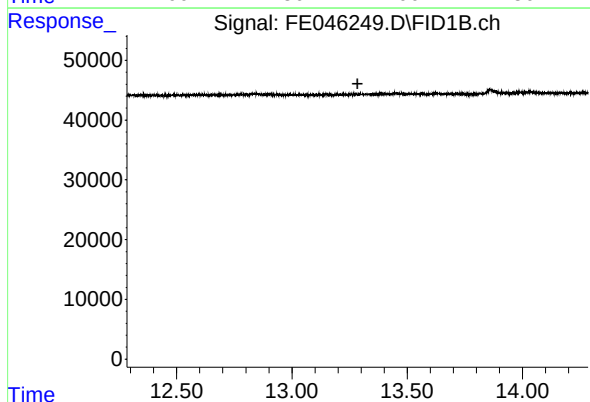


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

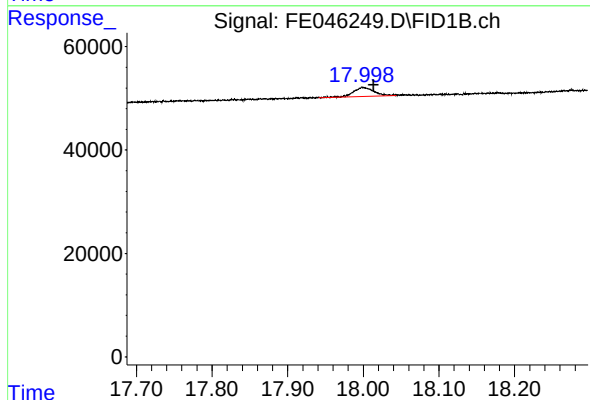


#17 n-Tricontane (C30)

R.T.: 17.999 min
Delta R.T.: -0.015 min
Response: 32598
Conc: 0.22 ug/ml

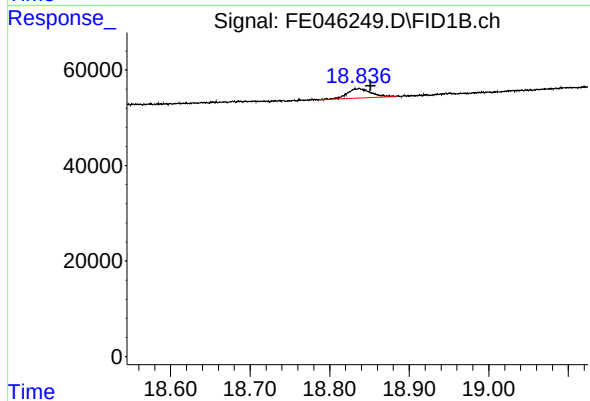

#18 n-Dotriacontane (C32)

R.T.: 18.837 min
Delta R.T.: -0.014 min
Response: 40721
Conc: 0.27 ug/ml

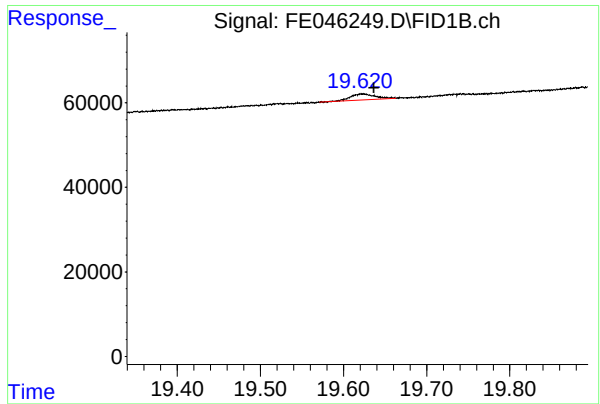

#19 n-Tetratriacontane (C34)

R.T.: 19.622 min
Delta R.T.: -0.014 min
Response: 28530
Conc: 0.20 ug/ml

Instrument :
FID_E
ClientSampleId :