

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011824AL\
 Data File : FE046296.D
 Signal(s) : FID1B.ch
 Acq On : 18 Jan 2024 21:41
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 00:13:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:49:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	17.106	25311	0.176 ug/ml
18) T n-Dotriacontane (C32)	18.832	60552	0.405 ug/ml
19) T n-Tetratriacontane (C34)	19.624	47249	0.330 ug/ml
20) T n-Hexatriacontane (C36)	20.388	4198	0.029 ug/ml
21) T n-Octatriacontane (C38)	21.126	103489	0.702 ug/ml
22) T n-Tetracontane (C40)	22.059	22838	0.146 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011824AL\
Data File : FE046296.D
Signal(s) : FID1B.ch
Acq On : 18 Jan 2024 21:41
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 00:13:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

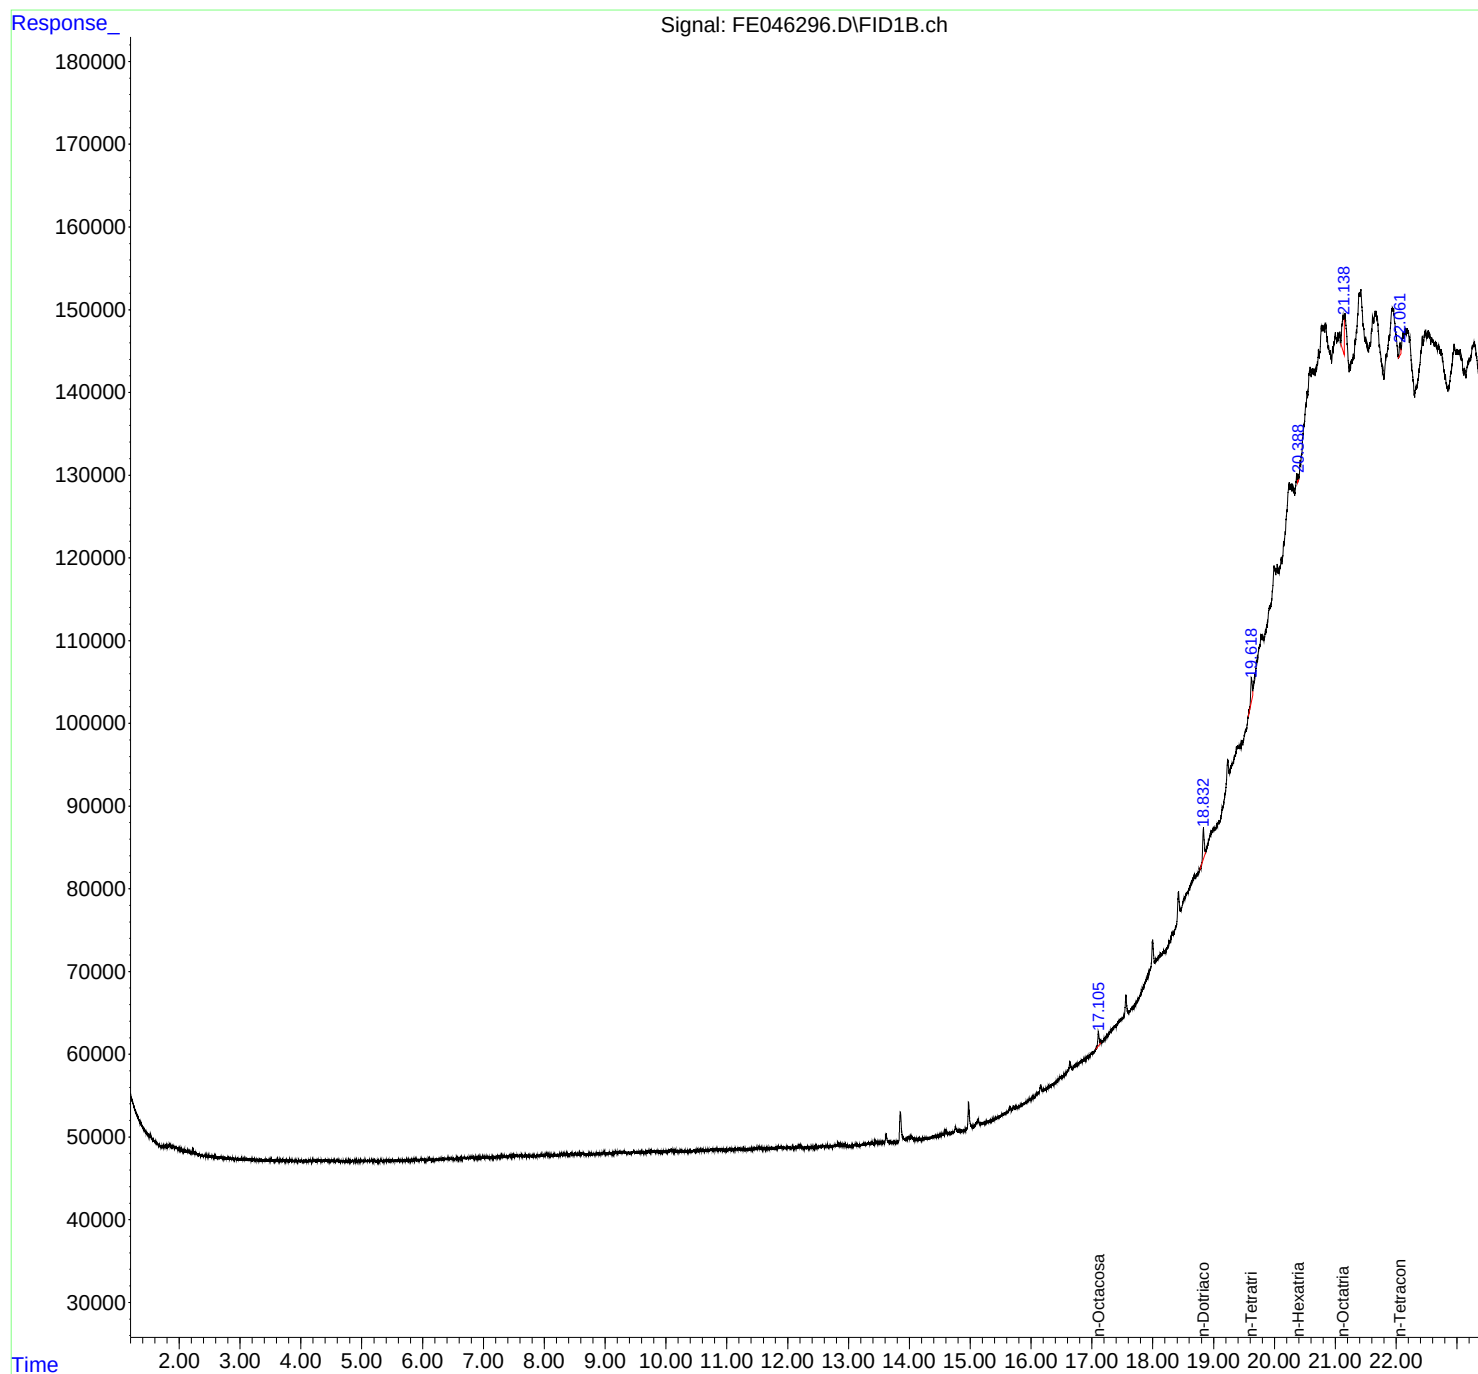


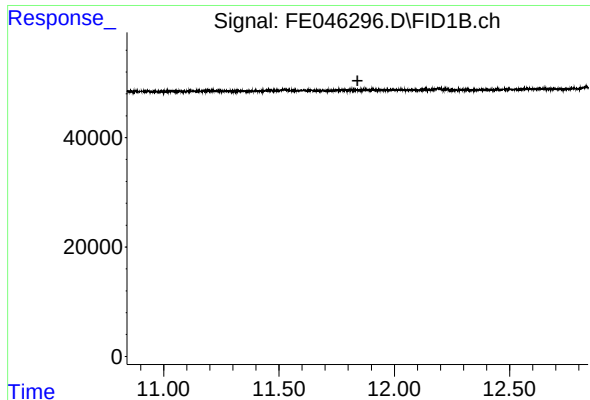

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

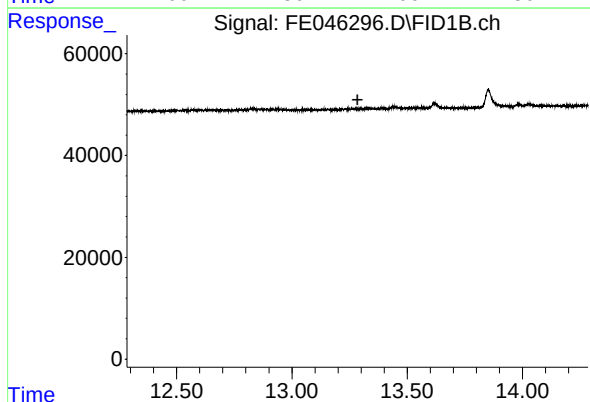


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

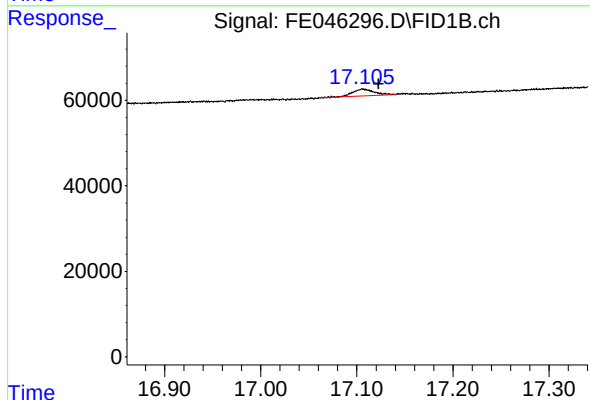


#16 n-Octacosane (C28)

R.T.: 17.106 min
Delta R.T.: -0.016 min
Response: 25311
Conc: 0.18 ug/ml

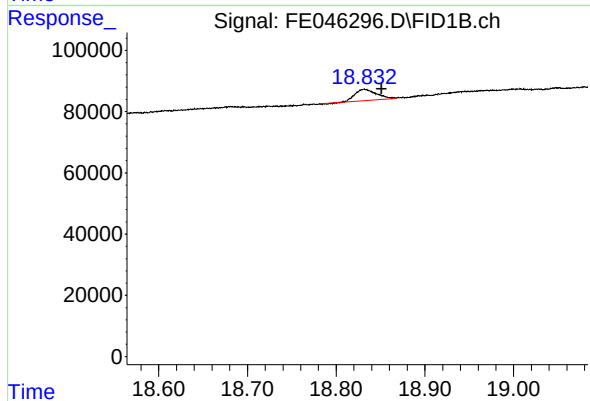

#18 n-Dotriacontane (C32)

R.T.: 18.832 min
Delta R.T.: -0.019 min
Response: 60552
Conc: 0.40 ug/ml

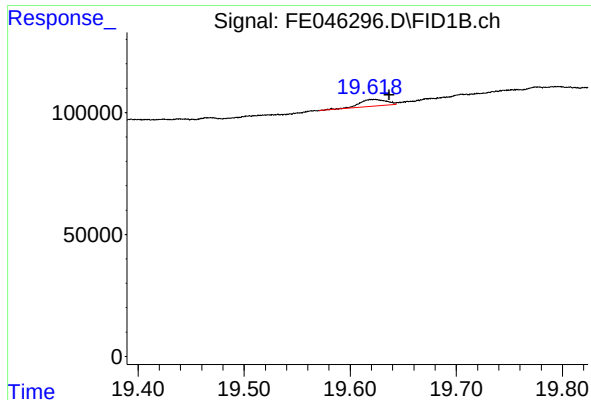


#19 n-Tetratriacontane (C34)

R.T.: 19.624 min
Delta R.T.: -0.013 min
Response: 47249
Conc: 0.33 ug/ml

Instrument :


FID_E

ClientSampleId :

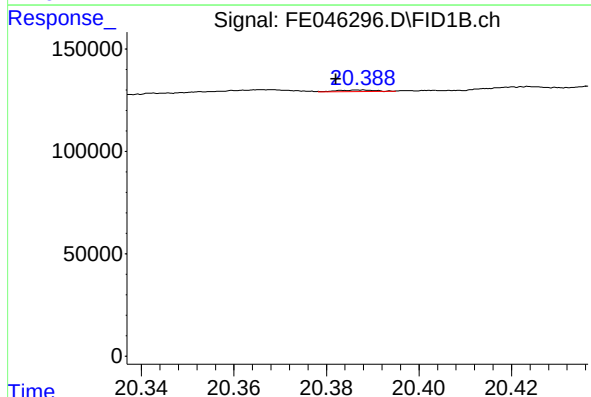


#20 n-Hexatriacontane (C36)

R.T.: 20.388 min
Delta R.T.: 0.006 min
Response: 4198
Conc: 0.03 ug/ml

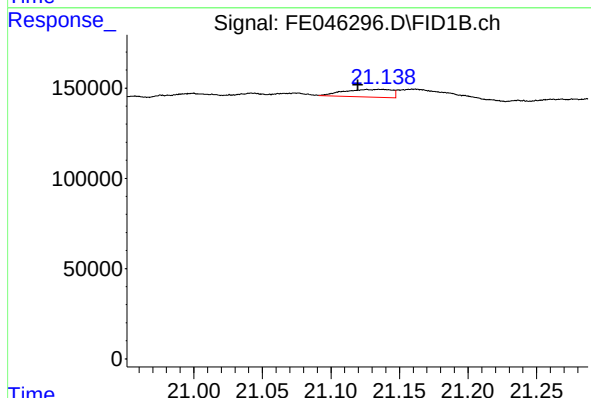

#21 n-Octatriacontane (C38)

R.T.: 21.126 min
Delta R.T.: 0.006 min
Response: 103489
Conc: 0.70 ug/ml

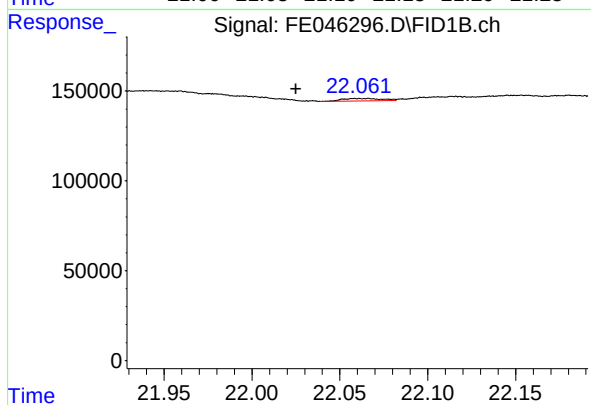

#22 n-Tetracontane (C40)

R.T.: 22.059 min
Delta R.T.: 0.034 min
Response: 22838
Conc: 0.15 ug/ml