

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011924AL\
 Data File : FE046298.D
 Signal(s) : FID1B.ch
 Acq On : 19 Jan 2024 09:08
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 19 22:07:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:49:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	17.111	27997	0.195 ug/ml
17) T n-Tricontane (C30)	18.002	73597	0.495 ug/ml
18) T n-Dotriacontane (C32)	18.838	90256	0.603 ug/ml
19) T n-Tetratriacontane (C34)	19.622	79098	0.552 ug/ml
20) T n-Hexatriacontane (C36)	20.369	31311	0.215 ug/ml
21) T n-Octatriacontane (C38)	21.091	26234	0.178 ug/ml
22) T n-Tetracontane (C40)	22.025	3367	0.022 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE011924AL\
Data File : FE046298.D
Signal(s) : FID1B.ch
Acq On : 19 Jan 2024 09:08
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 19 22:07:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

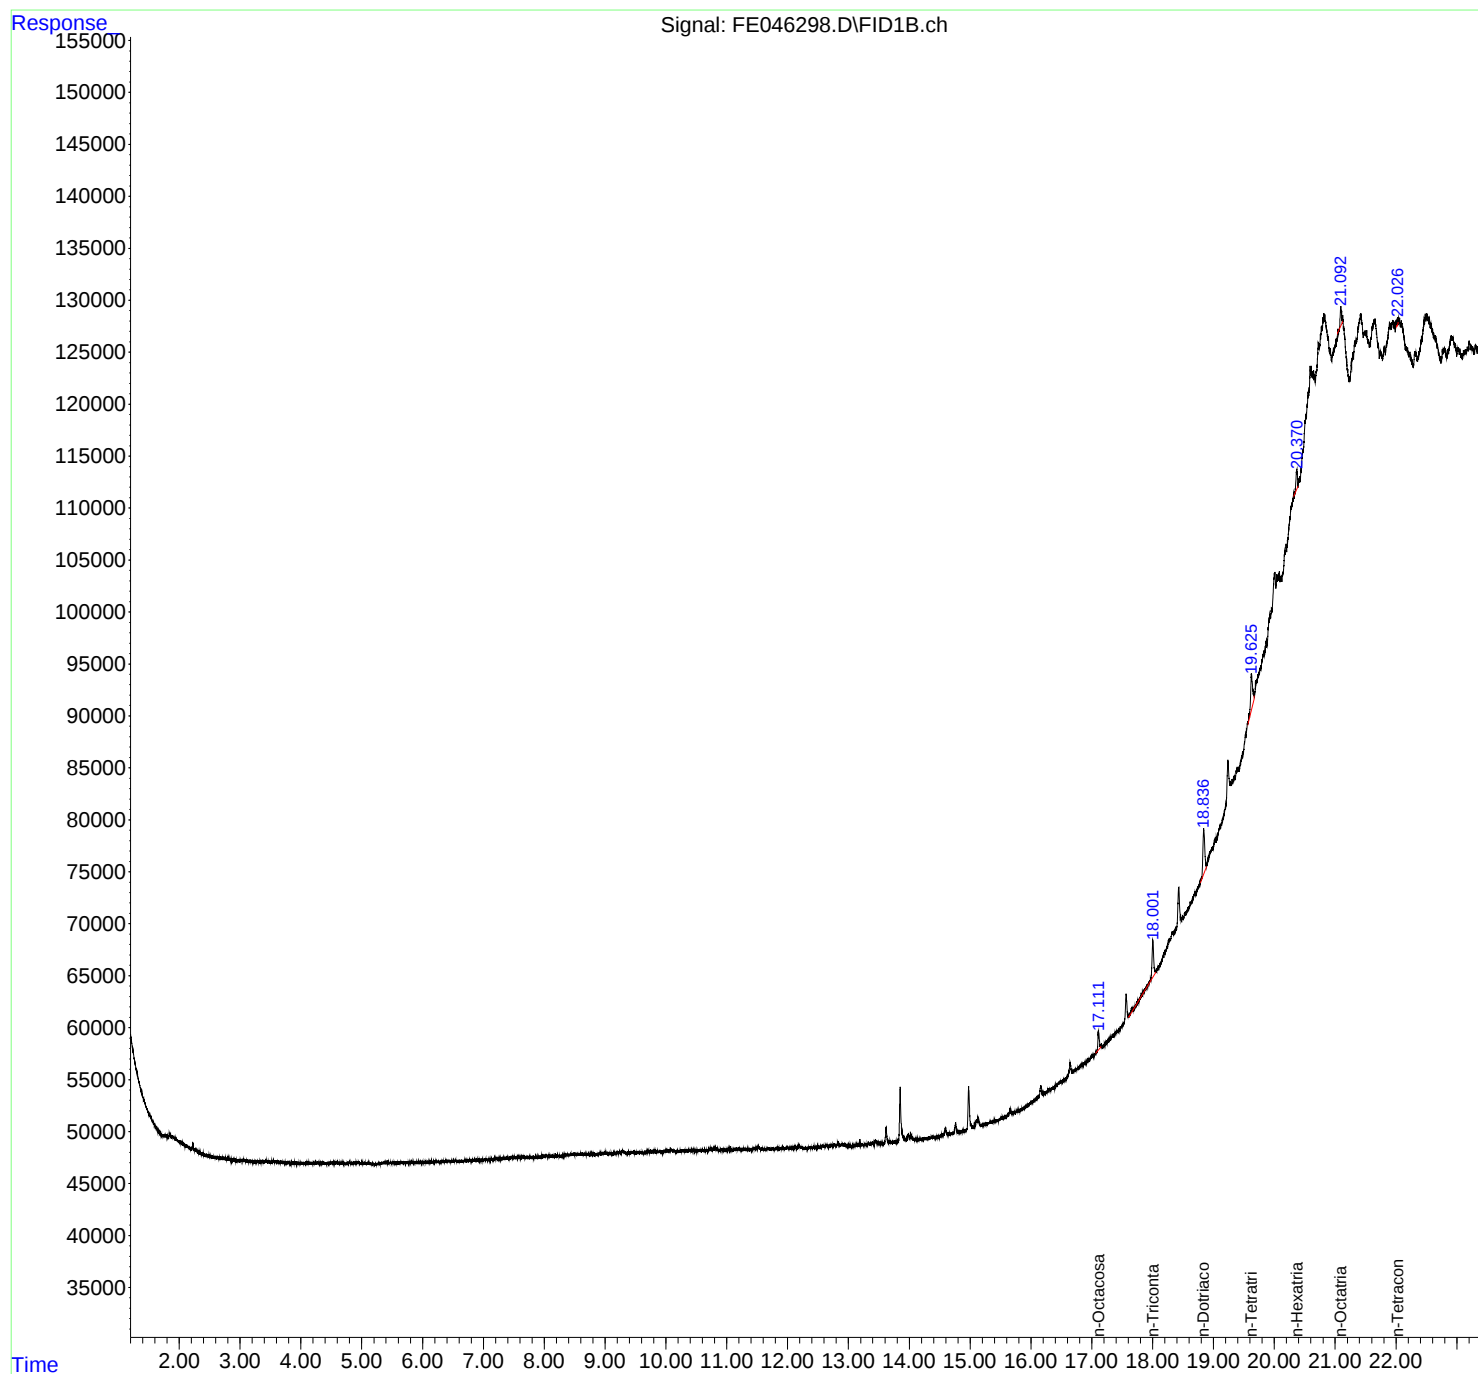


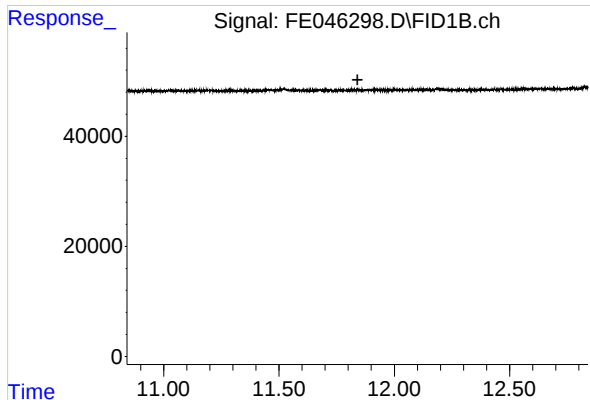

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

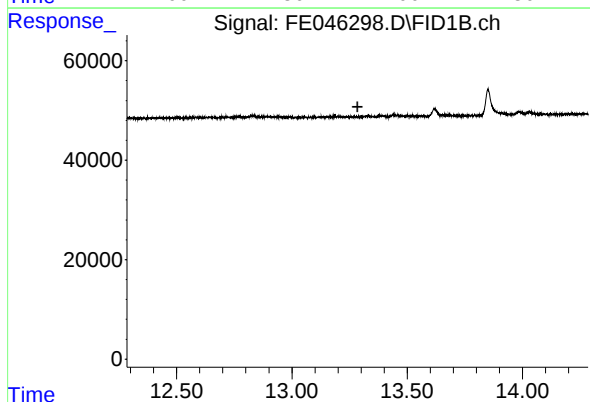


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

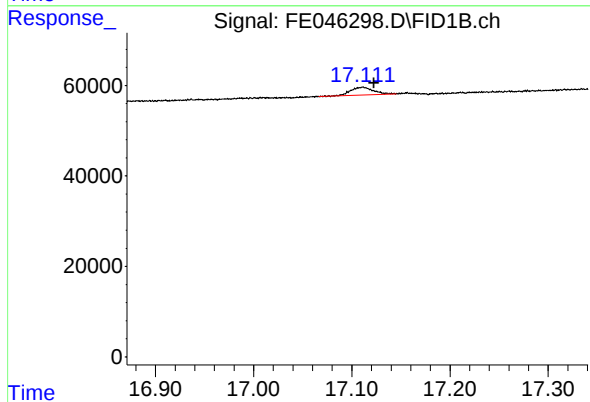


#16 n-Octacosane (C28)

R.T.: 17.111 min
Delta R.T.: -0.011 min
Response: 27997
Conc: 0.20 ug/ml

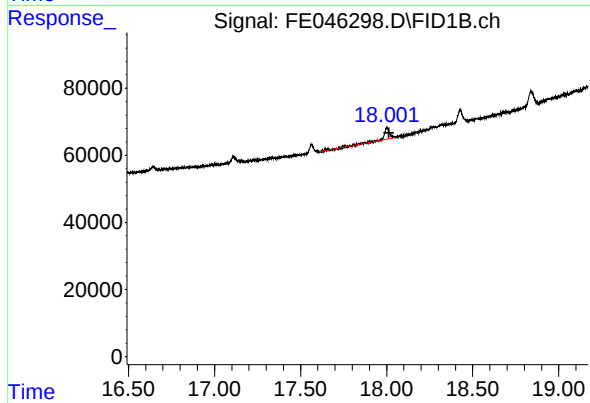

#17 n-Tricontane (C30)


R.T.: 18.002 min
Delta R.T.: -0.012 min
Response: 73597
Conc: 0.50 ug/ml

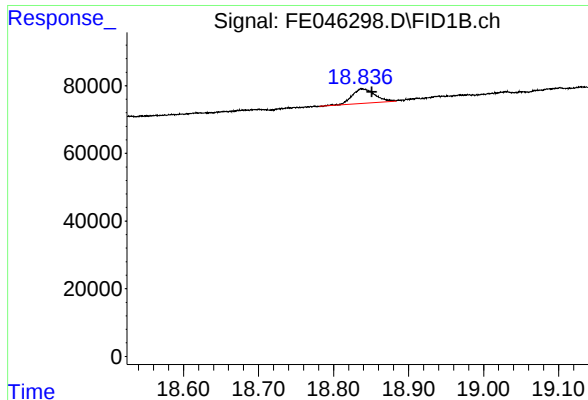

#18 n-Dotriacontane (C32)


R.T.: 18.838 min
Delta R.T.: -0.014 min
Response: 90256
Conc: 0.60 ug/ml

Instrument :
FID_E
ClientSampleId :

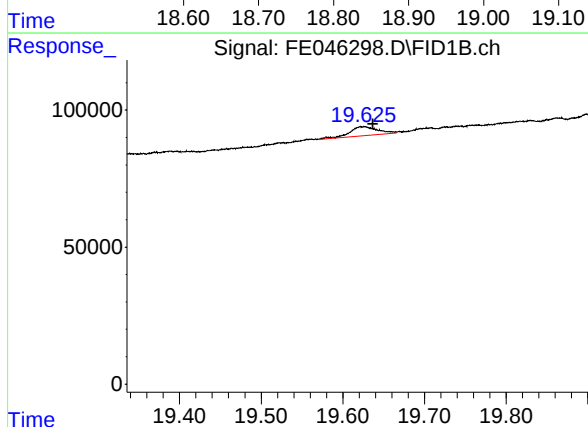


#19 n-Tetratriacontane (C34)

R.T.: 19.622 min
Delta R.T.: -0.015 min
Response: 79098
Conc: 0.55 ug/ml

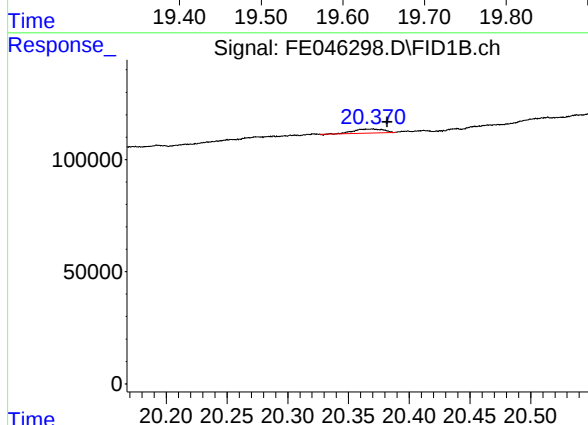


#20 n-Hexatriacontane (C36)

R.T.: 20.369 min
Delta R.T.: -0.013 min
Response: 31311
Conc: 0.21 ug/ml

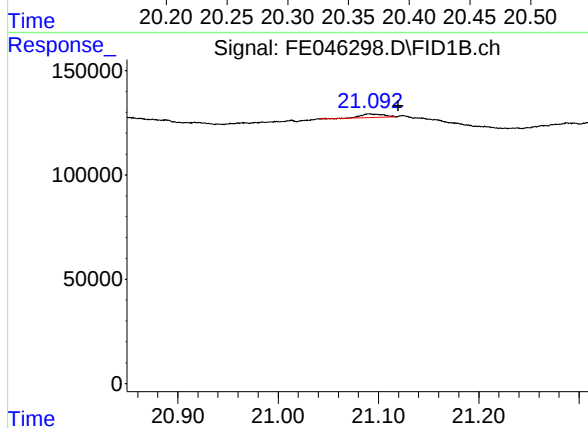

#21 n-Octatriacontane (C38)

R.T.: 21.091 min
Delta R.T.: -0.029 min
Response: 26234
Conc: 0.18 ug/ml

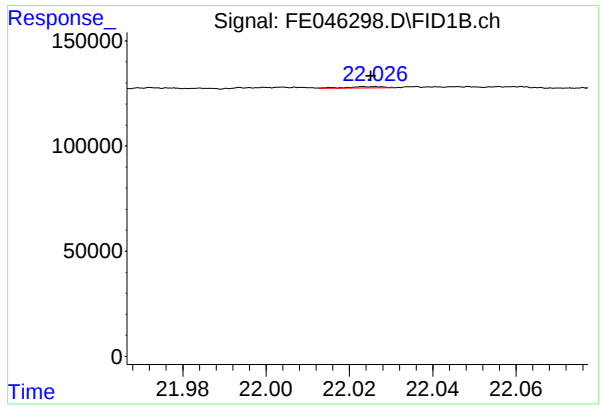

#22 n-Tetracontane (C40)

R.T.: 22.025 min
Delta R.T.: 0.000 min
Response: 3367
Conc: 0.02 ug/ml

Instrument :

FID_E

ClientSampleId :