

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012020\
 Data File : FE031144.D
 Signal(s) : FID1B.CH
 Acq On : 20 Jan 2020 18:37
 Operator : DD\AJ
 Sample : L1165-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 03:03:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	6742544	20.206 ug/ml
Target Compounds			
4) N-TETRADECANE	8.229f	536782	1.404 ug/ml
8) N-DOCOSANE	13.725	192716	0.499 ug/ml
10) N-TETRACOSANE	14.831	337189	0.879 ug/ml
11) N-HEXACOSANE	15.854	755430	1.975 ug/ml
12) N-OCTACOSANE	16.806	1516762	3.946 ug/ml
13) N-TRIACONTANE	17.696	1617611	4.220 ug/ml
14) N-DOTRIACONTANE	18.528	980358	2.711 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012020\
Data File : FE031144.D
Signal(s) : FID1B.CH
Acq On : 20 Jan 2020 18:37
Operator : DD\AJ
Sample : L1165-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:03:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

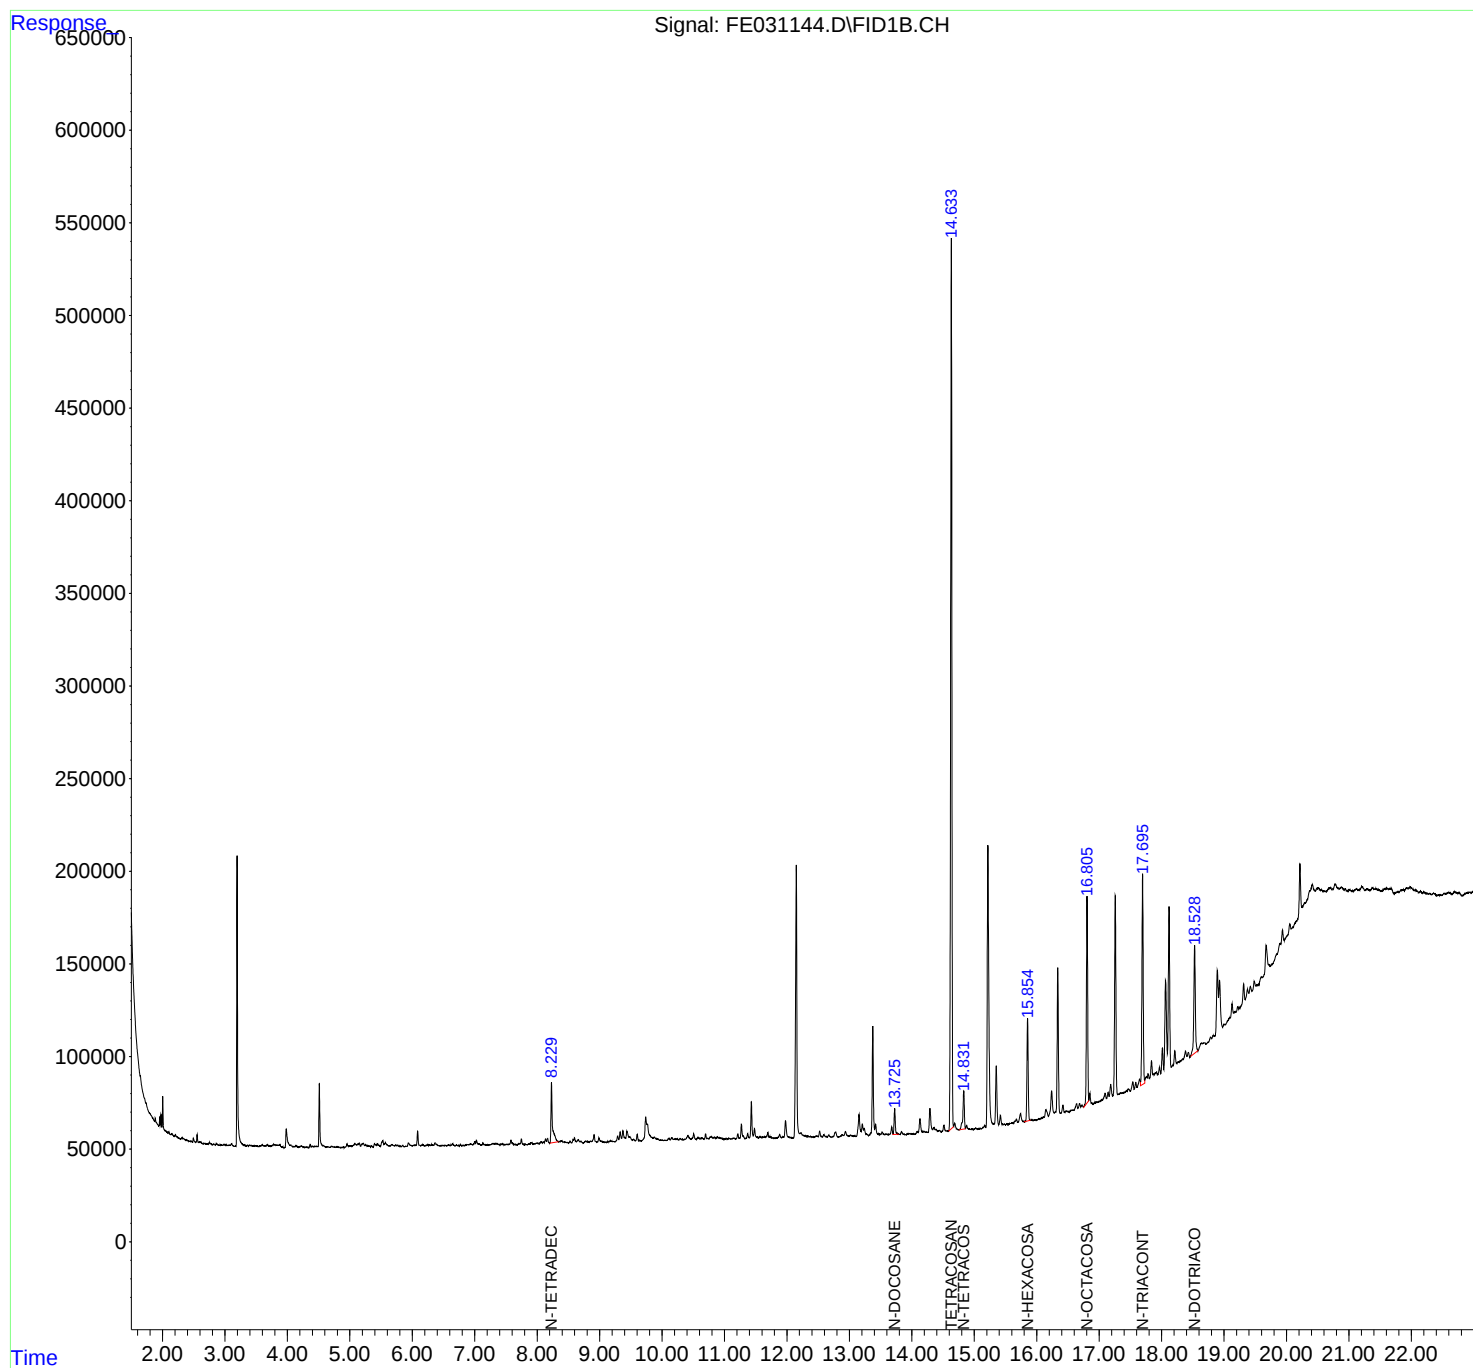


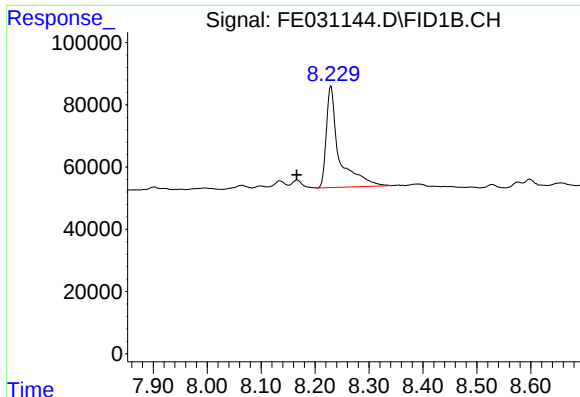

#4 N-TETRADECANE


R.T.: 8.229 min
Delta R.T.: 0.064 min
Response: 536782
Conc: 1.40 ug/ml

Instrument :
FID_E
ClientSampleId :

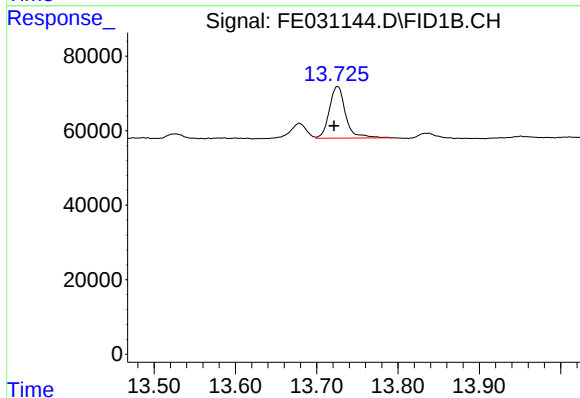


#8 N-DOCOSANE

R.T.: 13.725 min
Delta R.T.: 0.004 min
Response: 192716
Conc: 0.50 ug/ml

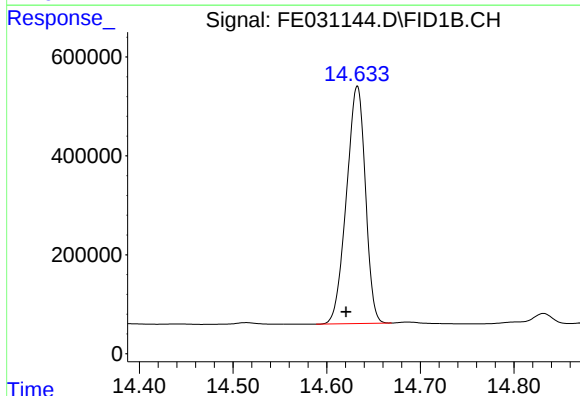


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: 0.012 min
Response: 6742544
Conc: 20.21 ug/ml

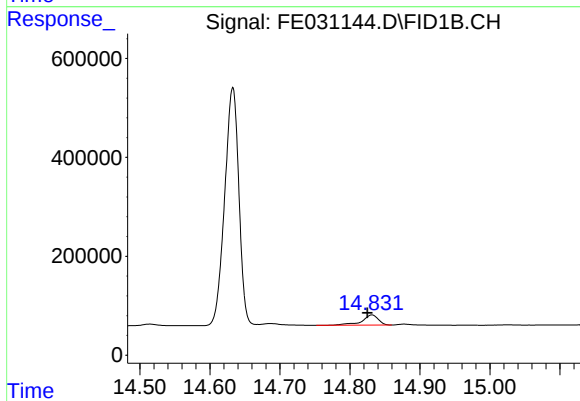

#10 N-TETRACOSANE


R.T.: 14.831 min
Delta R.T.: 0.006 min
Response: 337189
Conc: 0.88 ug/ml

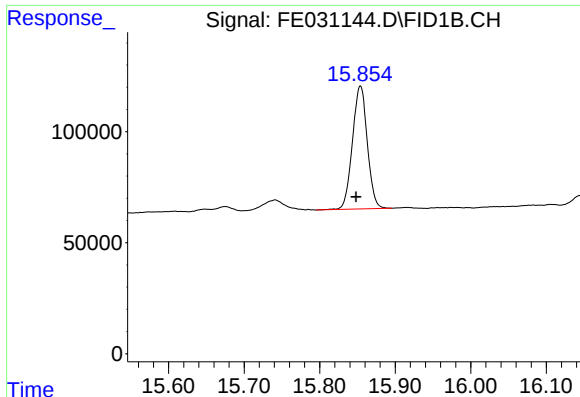

#11 N-HEXACOSANE


R.T.: 15.854 min
Delta R.T.: 0.006 min
Response: 755430
Conc: 1.98 ug/ml

Instrument :
FID_E
ClientSampleId :

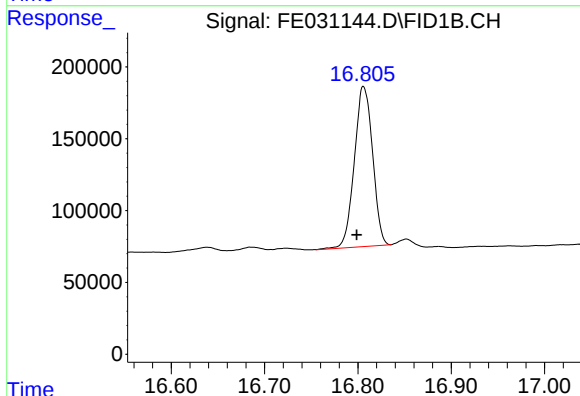


#12 N-OCTACOSANE

R.T.: 16.806 min
Delta R.T.: 0.008 min
Response: 1516762
Conc: 3.95 ug/ml

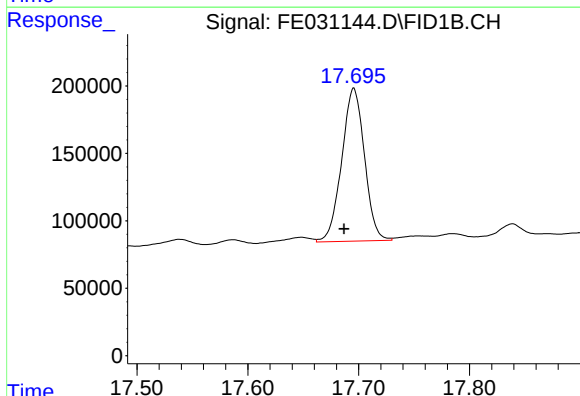

#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: 0.009 min
Response: 1617611
Conc: 4.22 ug/ml

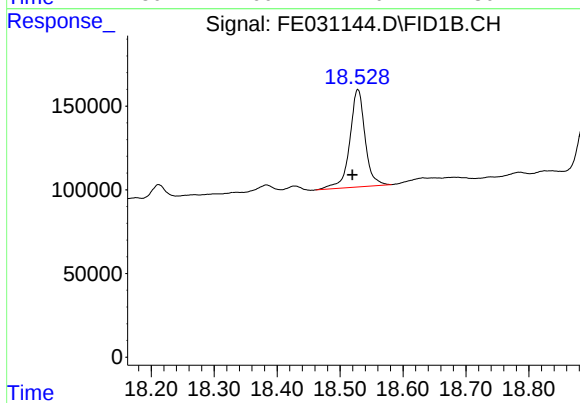

#14 N-DOTRIACONTANE

R.T.: 18.528 min
Delta R.T.: 0.009 min
Response: 980358
Conc: 2.71 ug/ml