

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012020\
 Data File : FE031145.D
 Signal(s) : FID1B.CH
 Acq On : 20 Jan 2020 19:10
 Operator : DD\AJ
 Sample : L1166-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 21 03:03:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.631	6926859	20.759 ug/ml
Target Compounds			
4) N-TETRADECANE	8.229f	585097	1.530 ug/ml
8) N-DOCOSANE	13.724	204463	0.529 ug/ml
10) N-TETRACOSANE	14.831	346552	0.904 ug/ml
11) N-HEXACOSANE	15.853	856689	2.240 ug/ml
12) N-OCTACOSANE	16.806	1829747	4.760 ug/ml
13) N-TRIACONTANE	17.696	1976058	5.155 ug/ml
14) N-DOTRIACONTANE	18.528	1230696	3.403 ug/ml
15) N-TETRATRIACONTANE	19.313	134130	0.402 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012020\
Data File : FE031145.D
Signal(s) : FID1B.CH
Acq On : 20 Jan 2020 19:10
Operator : DD\AJ
Sample : L1166-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 21 03:03:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

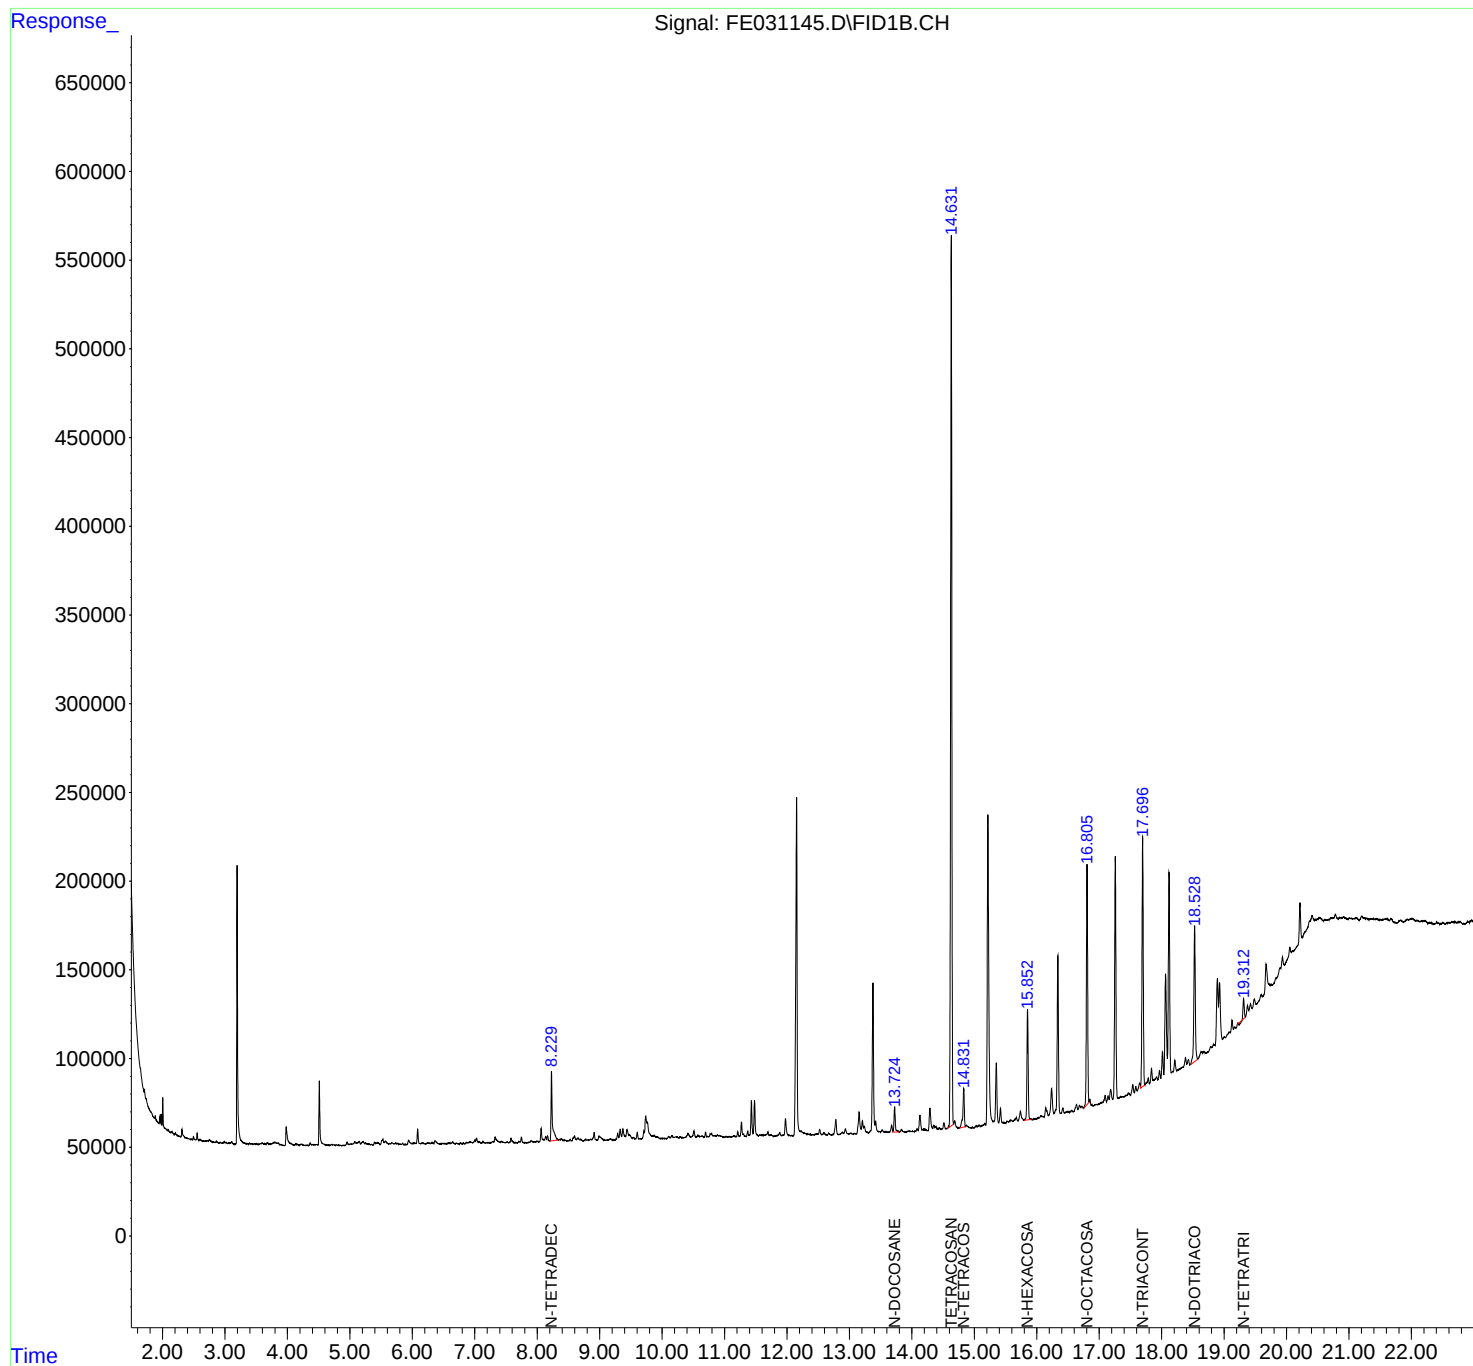


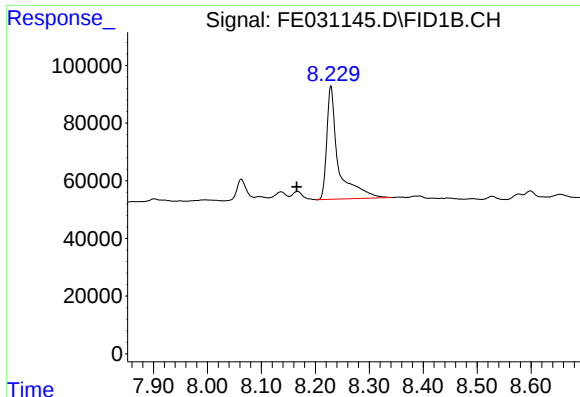

#4 N-TETRADECANE


R.T.: 8.229 min
Delta R.T.: 0.063 min
Response: 585097
Conc: 1.53 ug/ml

Instrument :
FID_E
ClientSampleId :

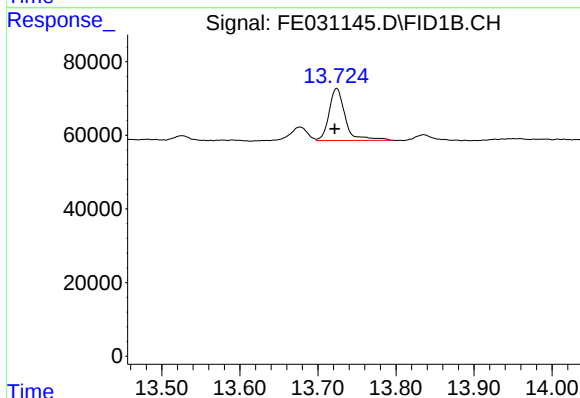


#8 N-DOCOSANE

R.T.: 13.724 min
Delta R.T.: 0.003 min
Response: 204463
Conc: 0.53 ug/ml

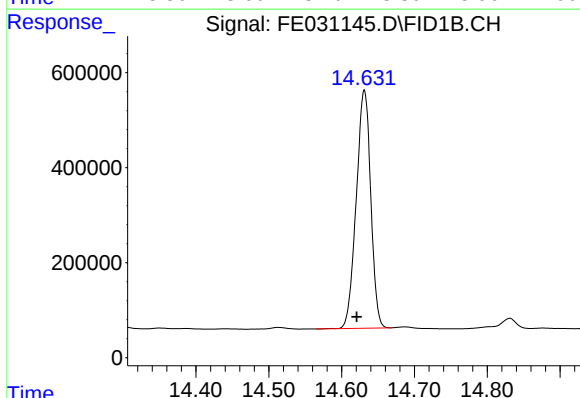


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.631 min
Delta R.T.: 0.010 min
Response: 6926859
Conc: 20.76 ug/ml

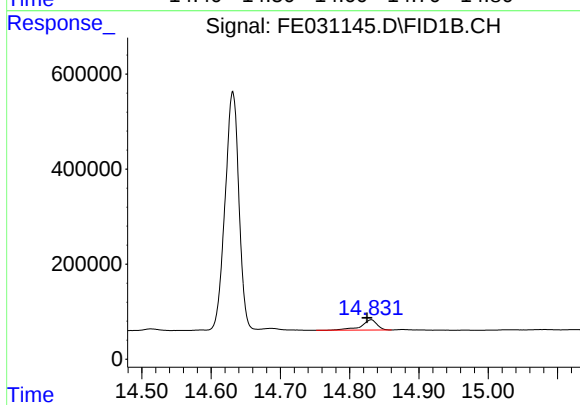

#10 N-TETRACOSANE


R.T.: 14.831 min
Delta R.T.: 0.006 min
Response: 346552
Conc: 0.90 ug/ml

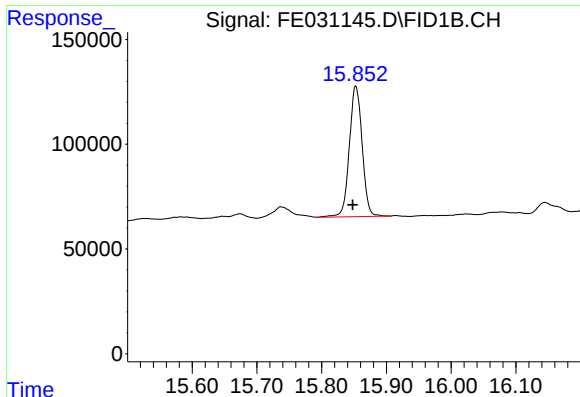

#11 N-HEXACOSANE


R.T.: 15.853 min
Delta R.T.: 0.005 min
Response: 856689
Conc: 2.24 ug/ml

Instrument :
FID_E
ClientSampleId :

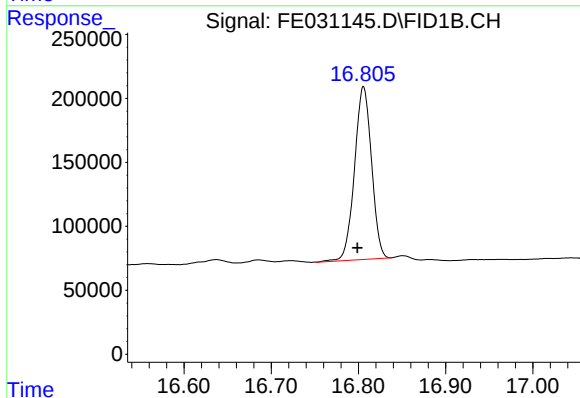


#12 N-OCTACOSANE

R.T.: 16.806 min
Delta R.T.: 0.007 min
Response: 1829747
Conc: 4.76 ug/ml

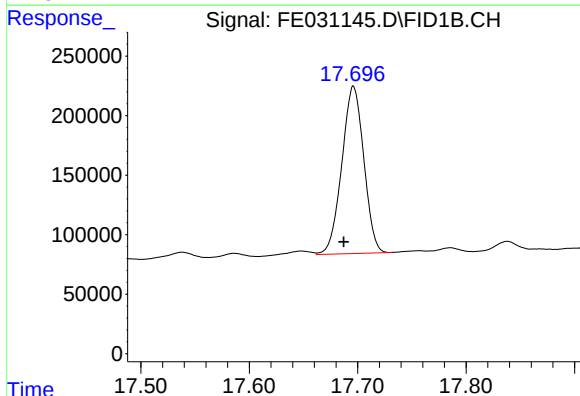


#13 N-TRIACONTANE

R.T.: 17.696 min
Delta R.T.: 0.009 min
Response: 1976058
Conc: 5.15 ug/ml

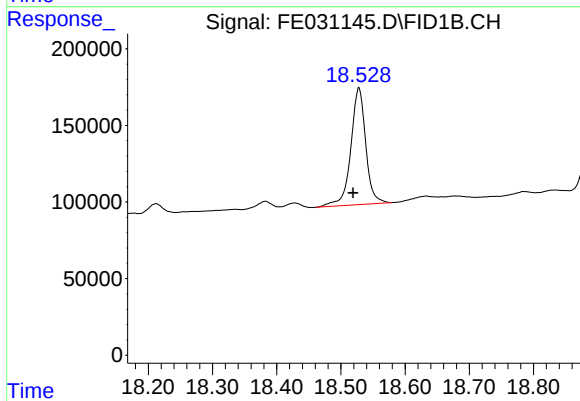

#14 N-DOTRIACONTANE

R.T.: 18.528 min
Delta R.T.: 0.009 min
Response: 1230696
Conc: 3.40 ug/ml

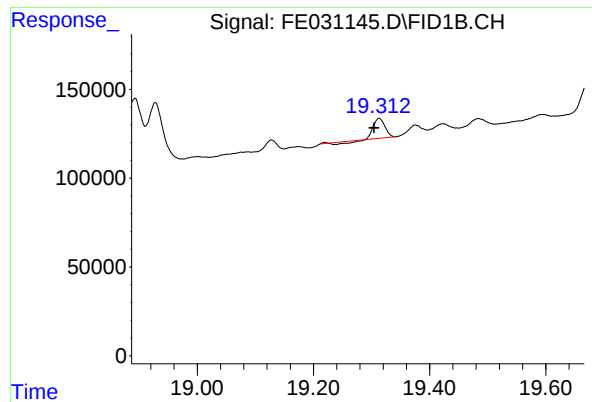

#15 N-TETRATRIACONTANE

R.T.: 19.313 min

Delta R.T.: 0.009 min

Response: 134130

Conc: 0.40 ug/ml

Instrument :
FID_E
ClientSampleId :