

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012120\
 Data File : FE031161.D
 Signal(s) : FID1B.CH
 Acq On : 21 Jan 2020 17:13
 Operator : DD\AJ
 Sample : L1210-06 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 22 00:30:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	867962	2.601 ug/ml
Target Compounds			
8) N-DOCOSANE	13.733	120350	0.312 ug/ml
10) N-TETRACOSANE	14.826	594485	1.550 ug/ml
11) N-HEXACOSANE	15.865	523815	1.369 ug/ml
12) N-OCTACOSANE	16.822	845640	2.200 ug/ml
13) N-TRIACONTANE	17.711	1608478	4.196 ug/ml
14) N-DOTRIACONTANE	18.546	832835	2.303 ug/ml
15) N-TETRATRIACONTANE	19.337	683254	2.049 ug/ml
16) N-HEXATRIACONTANE	20.081	485380	1.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012120\
Data File : FE031161.D
Signal(s) : FID1B.CH
Acq On : 21 Jan 2020 17:13
Operator : DD\AJ
Sample : L1210-06 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 00:30:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

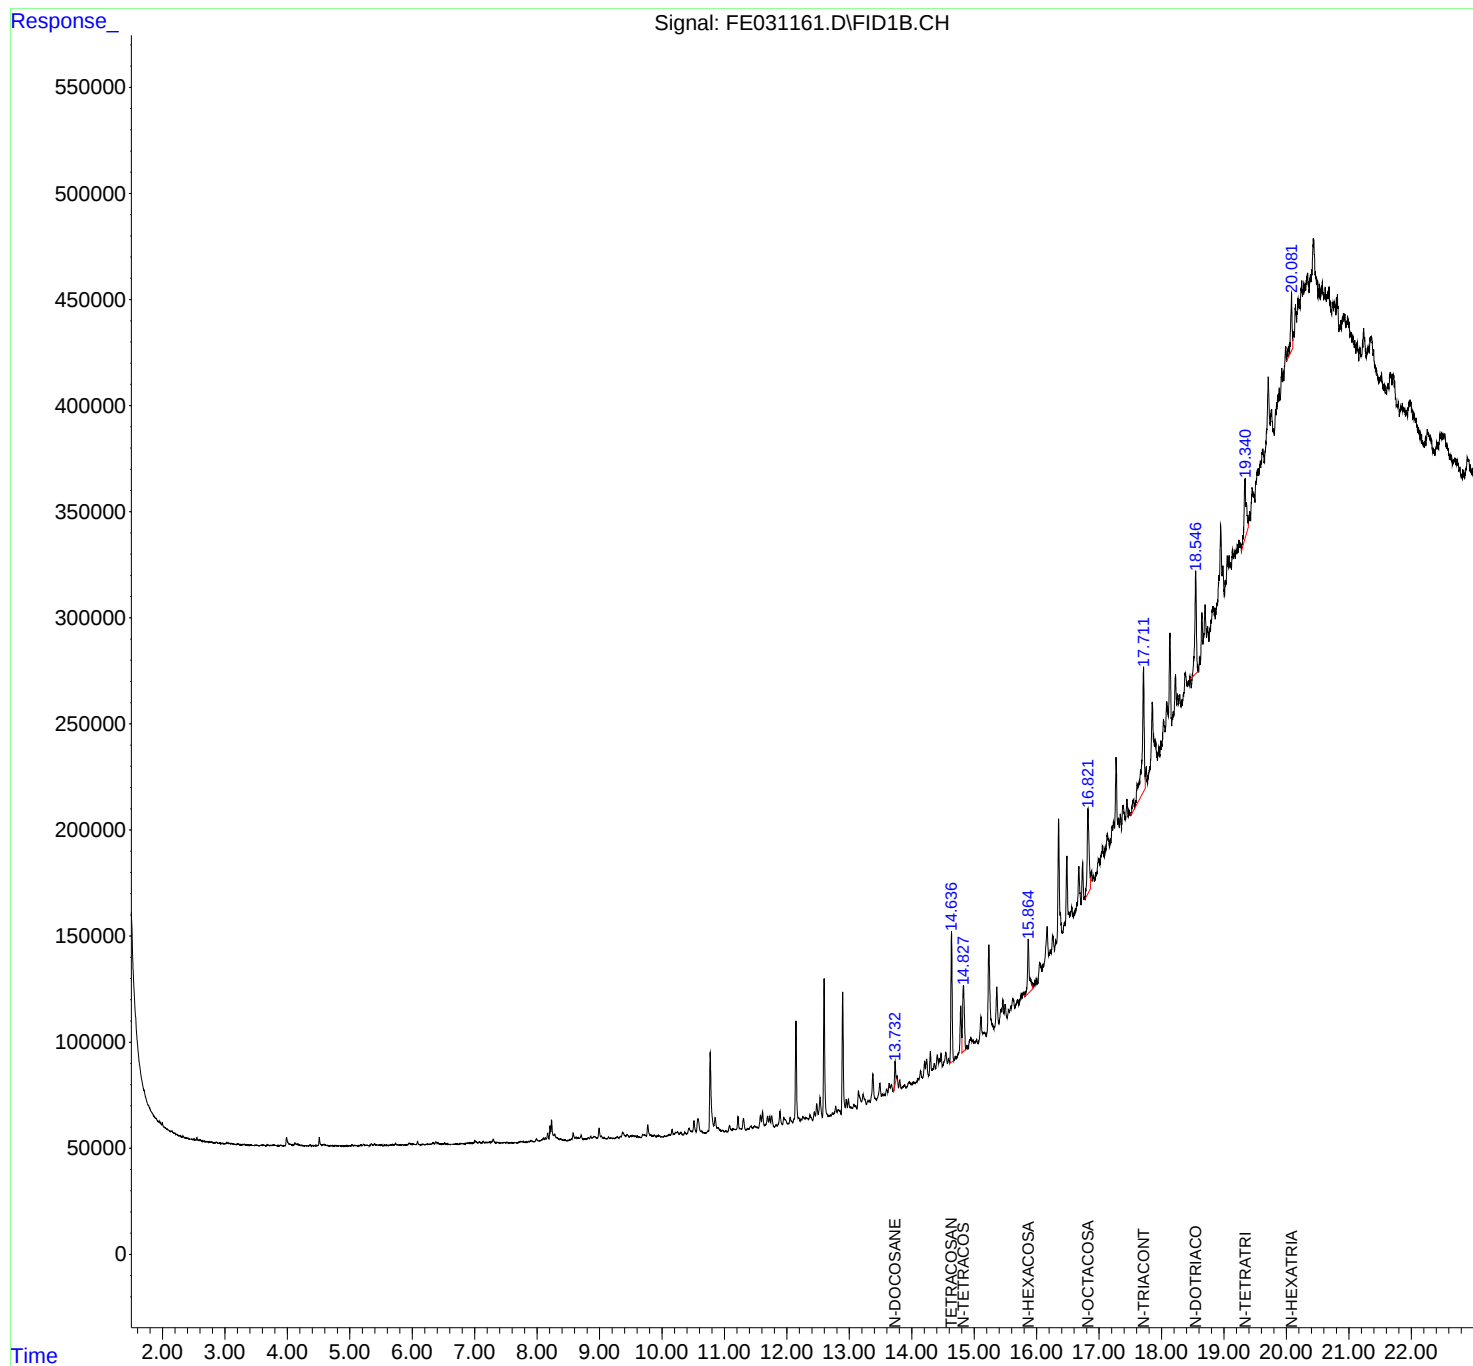


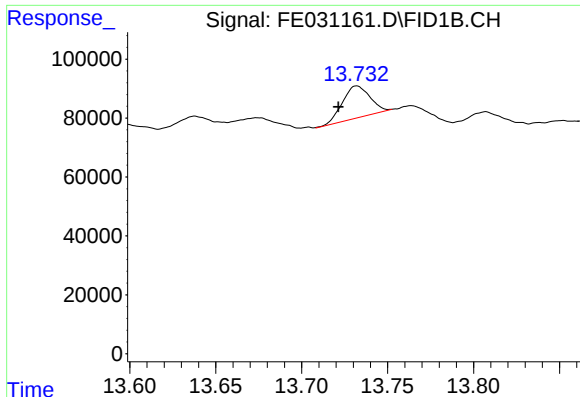

#8 N-DOCOSANE


R.T.: 13.733 min
Delta R.T.: 0.011 min
Response: 120350
Conc: 0.31 ug/ml

Instrument :
FID_E
ClientSampleId :

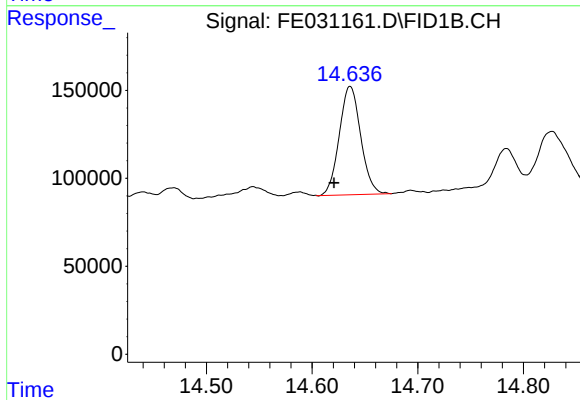


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: 0.015 min
Response: 867962
Conc: 2.60 ug/ml

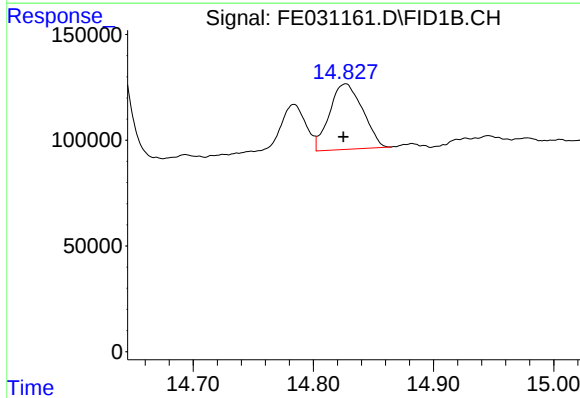


#10 N-TETRACOSANE

R.T.: 14.826 min
Delta R.T.: 0.001 min
Response: 594485
Conc: 1.55 ug/ml

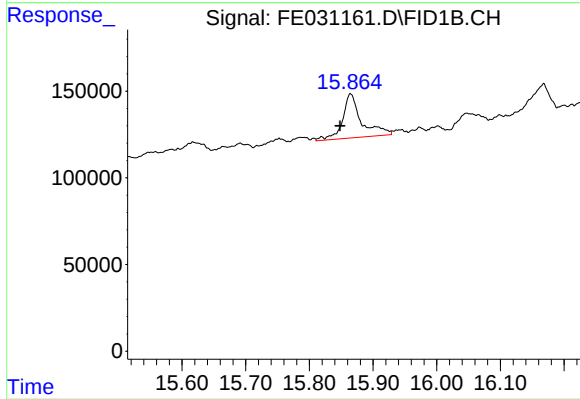

#11 N-HEXACOSANE


R.T.: 15.865 min
Delta R.T.: 0.017 min
Response: 523815
Conc: 1.37 ug/ml

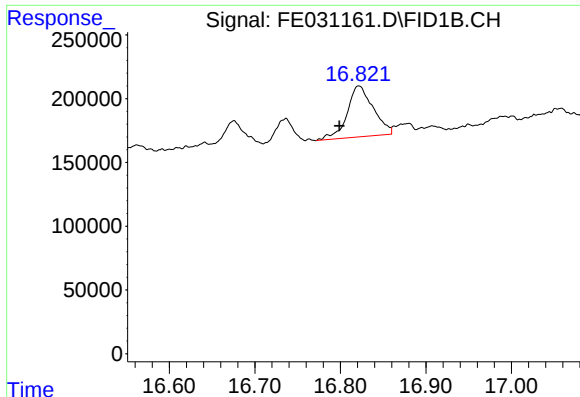

#12 N-OCTACOSANE


R.T.: 16.822 min
Delta R.T.: 0.023 min
Response: 845640
Conc: 2.20 ug/ml

Instrument :
FID_E
ClientSampleId :

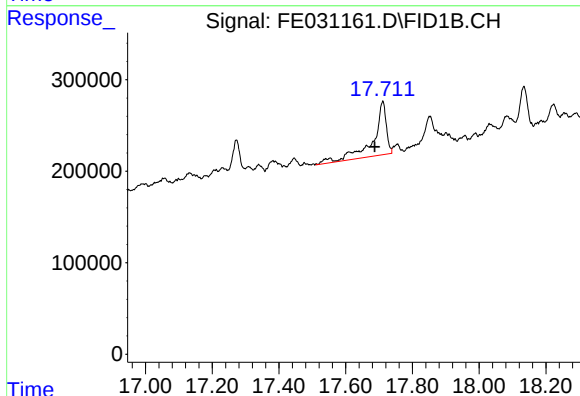


#13 N-TRIACONTANE

R.T.: 17.711 min
Delta R.T.: 0.024 min
Response: 1608478
Conc: 4.20 ug/ml

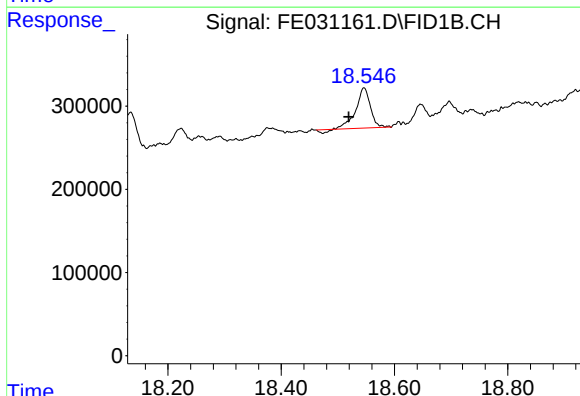


#14 N-DOTRIACONTANE

R.T.: 18.546 min
Delta R.T.: 0.027 min
Response: 832835
Conc: 2.30 ug/ml

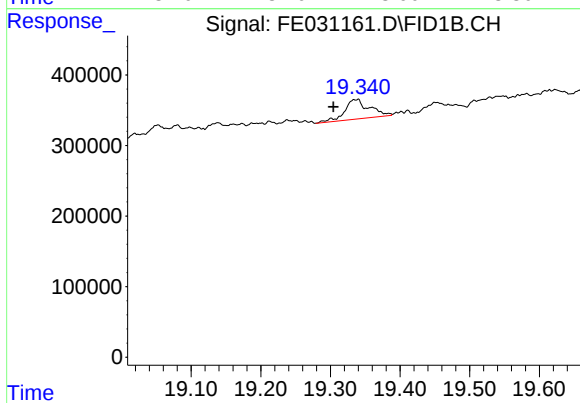

#15 N-TETRATRIACONTANE

R.T.: 19.337 min
Delta R.T.: 0.033 min
Response: 683254
Conc: 2.05 ug/ml

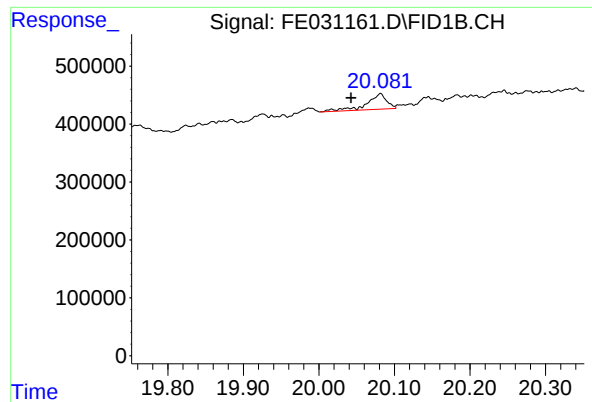

#16 N-HEXATRIACONTANE

R.T.: 20.081 min
Delta R.T.: 0.039 min
Response: 485380
Conc: 1.64 ug/ml

Instrument :
FID_E
ClientSampleId :