

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012320\
 Data File : FE031198.D
 Signal(s) : FID1B.CH
 Acq On : 23 Jan 2020 21:40
 Operator : DD\AJ
 Sample : L1216-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 24 01:27:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.624	5507737	16.506 ug/ml
Target Compounds			
4) N-TETRADECANE	8.219f	1947603	5.093 ug/ml
7) N-EICOSANE	12.582f	183160	0.471 ug/ml
8) N-DOCOSANE	13.717	203370	0.527 ug/ml
10) N-TETRACOSANE	14.822	462402	1.206 ug/ml
11) N-HEXACOSANE	15.846	544040	1.422 ug/ml
12) N-OCTACOSANE	16.797	1046781	2.723 ug/ml
13) N-TRIACONTANE	17.687	991044	2.585 ug/ml
14) N-DOTRIACONTANE	18.519	727627	2.012 ug/ml
15) N-TETRATRIACONTANE	19.306	156574	0.470 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012320\
Data File : FE031198.D
Signal(s) : FID1B.CH
Acq On : 23 Jan 2020 21:40
Operator : DD\AJ
Sample : L1216-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 01:27:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

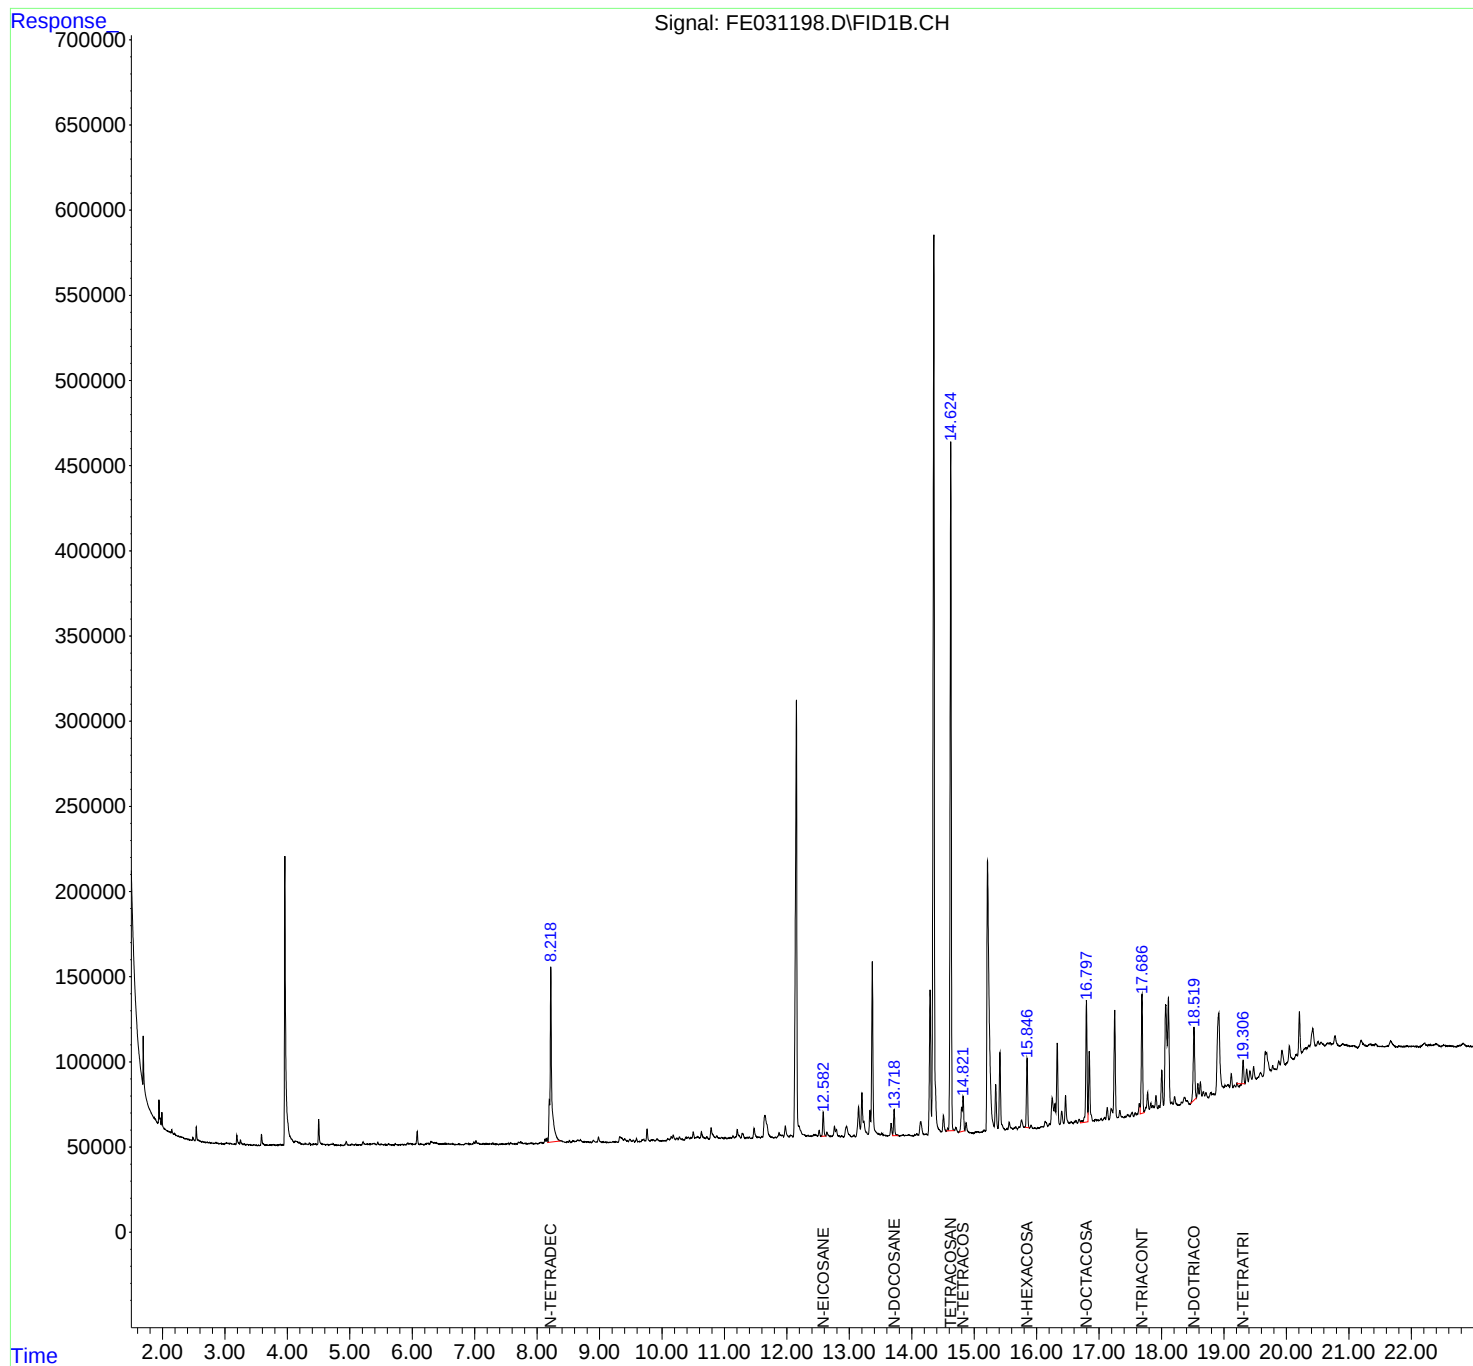


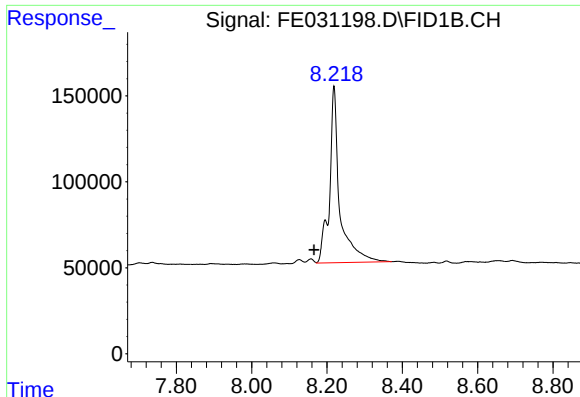

#4 N-TETRADECANE


R.T.: 8.219 min
Delta R.T.: 0.053 min
Response: 1947603
Conc: 5.09 ug/ml

Instrument :
FID_E
ClientSampleId :

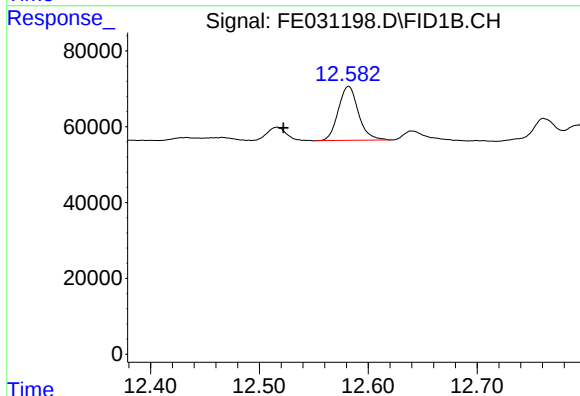


#7 N-EICOSANE

R.T.: 12.582 min
Delta R.T.: 0.060 min
Response: 183160
Conc: 0.47 ug/ml

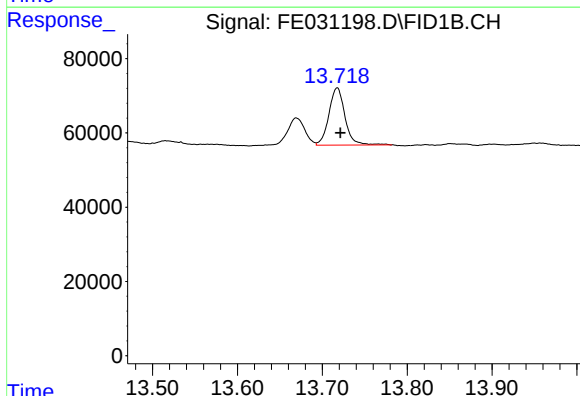


#8 N-DOCOSANE

R.T.: 13.717 min
Delta R.T.: -0.004 min
Response: 203370
Conc: 0.53 ug/ml

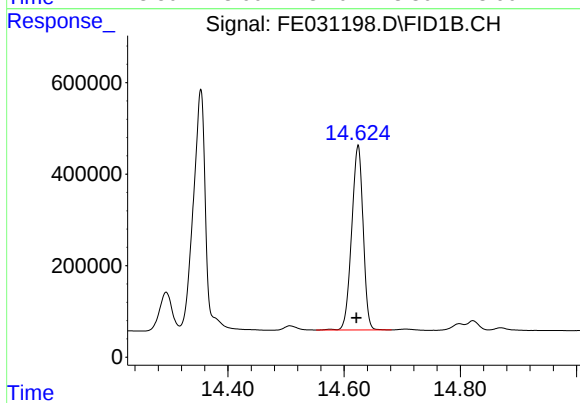

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.624 min
Delta R.T.: 0.003 min
Response: 5507737
Conc: 16.51 ug/ml

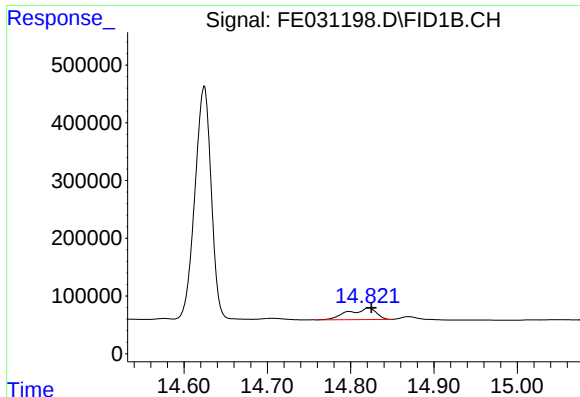

#10 N-TETRACOSANE


R.T.: 14.822 min
Delta R.T.: -0.003 min
Response: 462402
Conc: 1.21 ug/ml

Instrument :
FID_E
ClientSampleId :

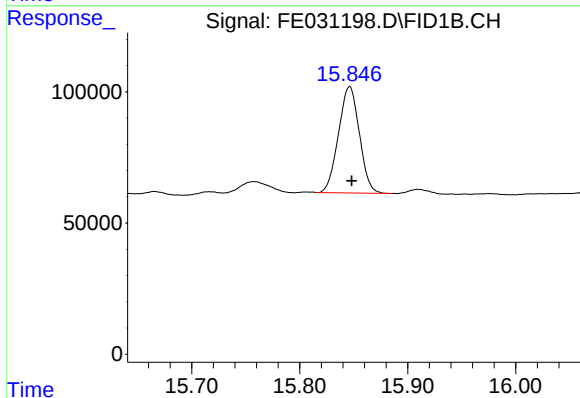


#11 N-HEXACOSANE

R.T.: 15.846 min
Delta R.T.: -0.002 min
Response: 544040
Conc: 1.42 ug/ml

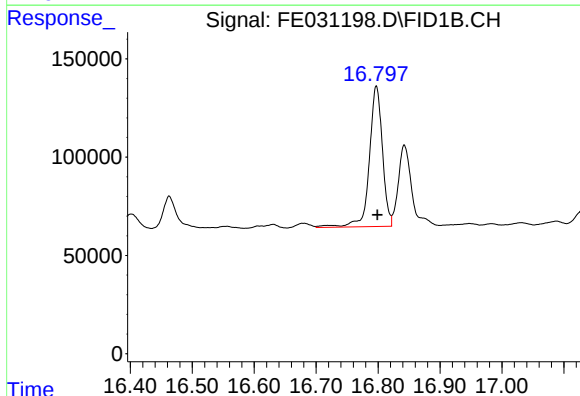


#12 N-OCTACOSANE

R.T.: 16.797 min
Delta R.T.: -0.002 min
Response: 1046781
Conc: 2.72 ug/ml

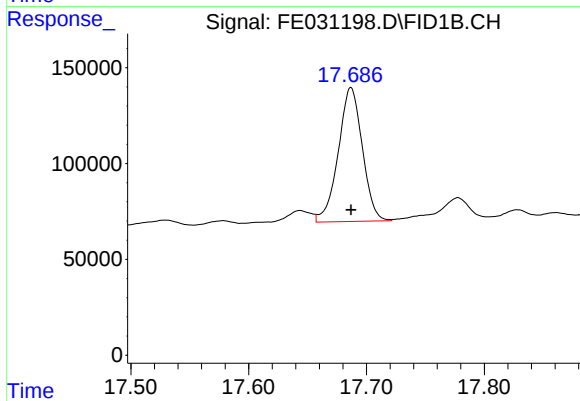

#13 N-TRIACONTANE


R.T.: 17.687 min
Delta R.T.: 0.000 min
Response: 991044
Conc: 2.59 ug/ml

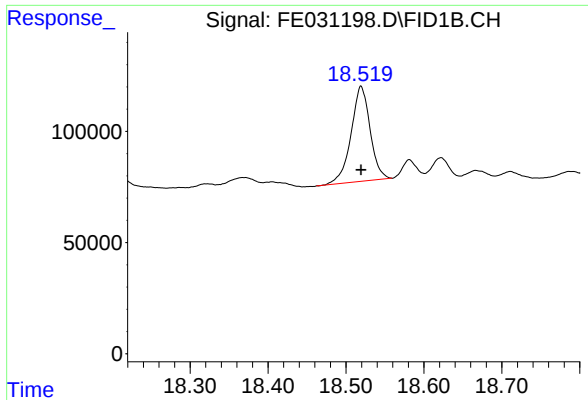

#14 N-DOTRIACONTANE

R.T.: 18.519 min
Delta R.T.: 0.000 min
Response: 727627
Conc: 2.01 ug/ml

Instrument :
FID_E
ClientSampleId :

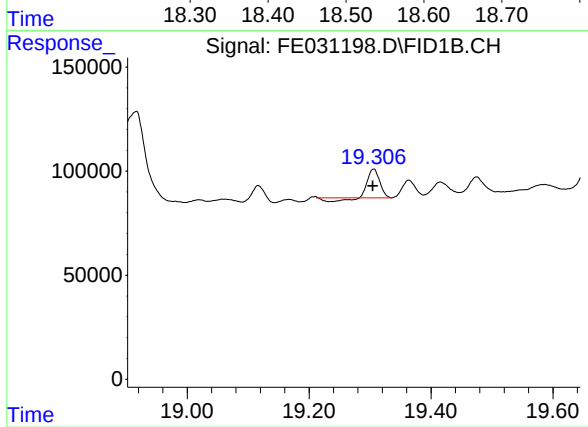

#15 N-TETRATRIACONTANE

R.T.: 19.306 min
Delta R.T.: 0.002 min
Response: 156574
Conc: 0.47 ug/ml