

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012420\
 Data File : FE031206.D
 Signal(s) : FID1B.CH
 Acq On : 24 Jan 2020 9:23
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 25 00:12:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
 Quant Title :
 QLast Update : Mon Jan 06 08:13:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	17851793	53.499 ug/ml
Target Compounds			
2) N-DECANE	4.360	21451276	57.092 ug/ml
3) N-DODECANE	6.370	21759968	61.655 ug/ml
4) N-TETRADECANE	8.168	21578533	56.433 ug/ml
5) N-HEXADECANE	9.771	21480058	55.484 ug/ml
6) N-OCTADECANE	11.215	21210296	55.131 ug/ml
7) N-EICOSANE	12.528	21148588	54.357 ug/ml
8) N-DOCOSANE	13.730	20811985	53.890 ug/ml
10) N-TETRACOSANE	14.835	20580209	53.657 ug/ml
11) N-HEXACOSANE	15.859	20131685	52.633 ug/ml
12) N-OCTACOSANE	16.810	19898050	51.760 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012420\
Data File : FE031206.D
Signal(s) : FID1B.CH
Acq On : 24 Jan 2020 9:23
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 25 00:12:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE010420.M
Quant Title :
QLast Update : Mon Jan 06 08:13:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

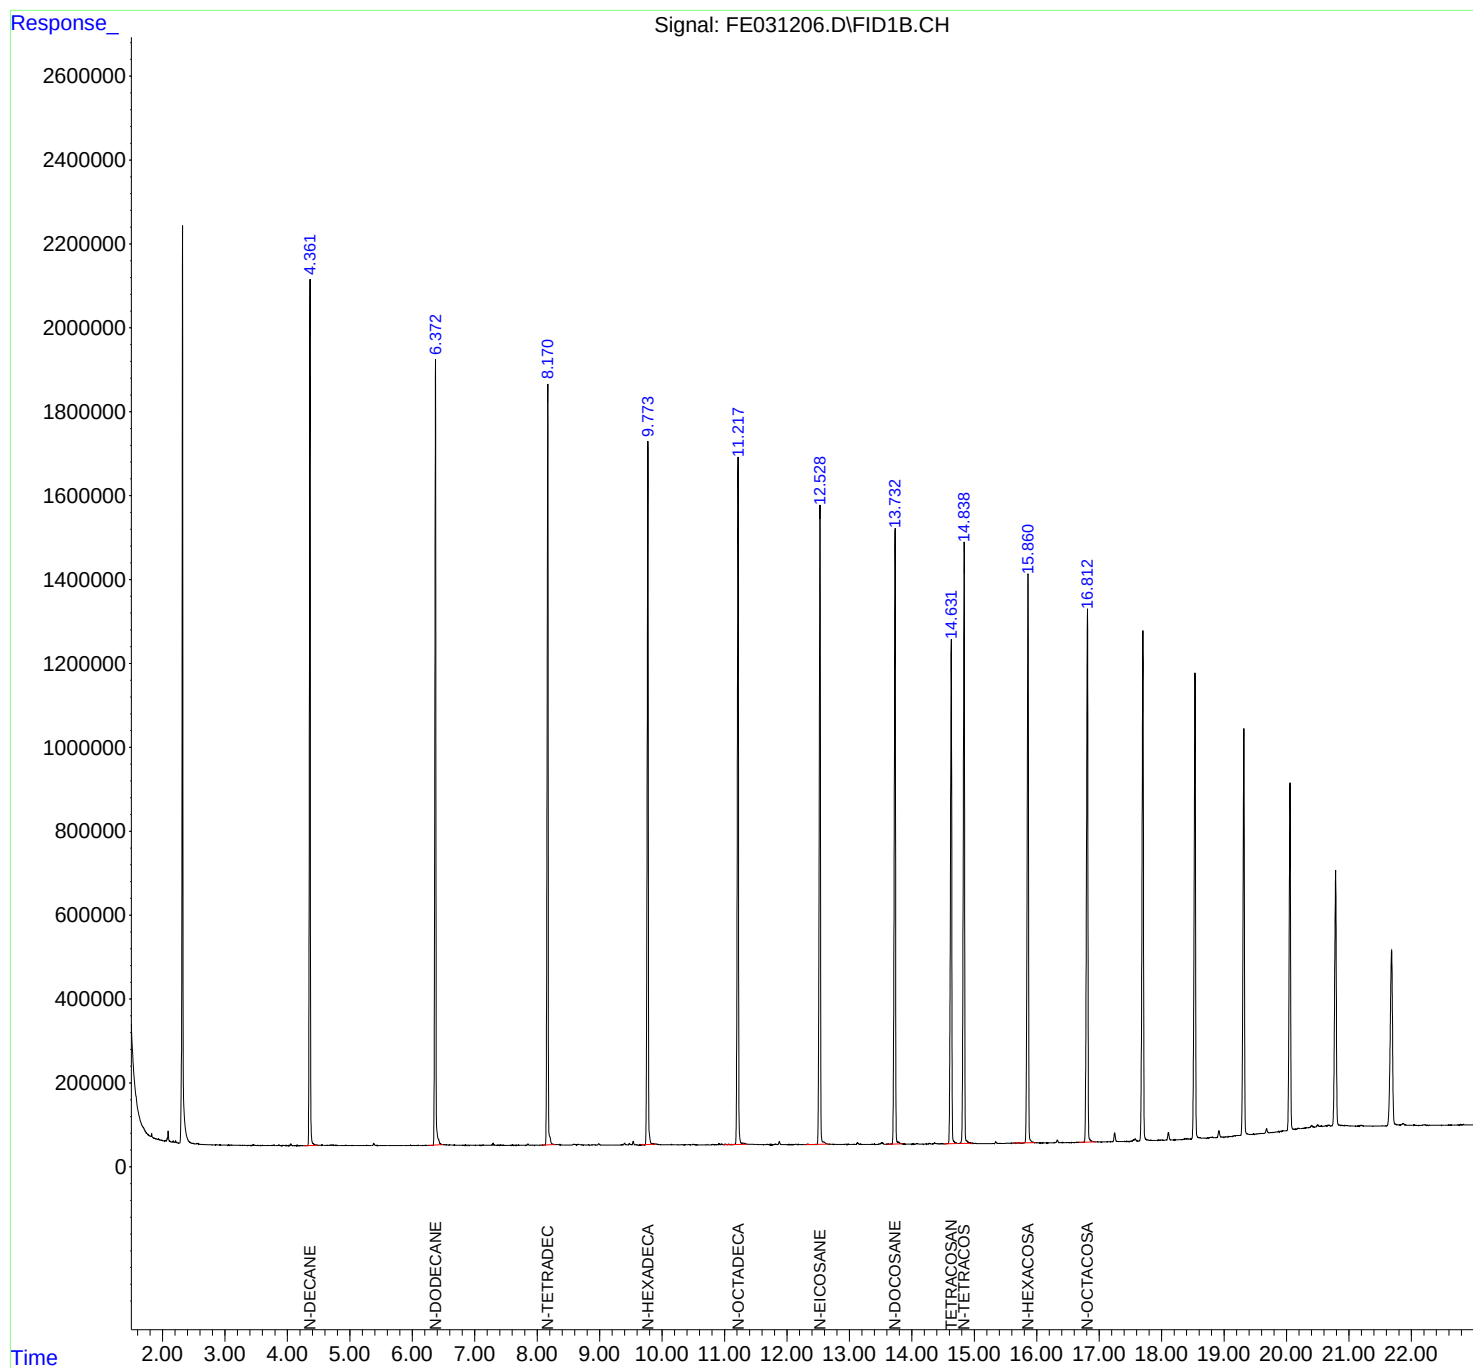

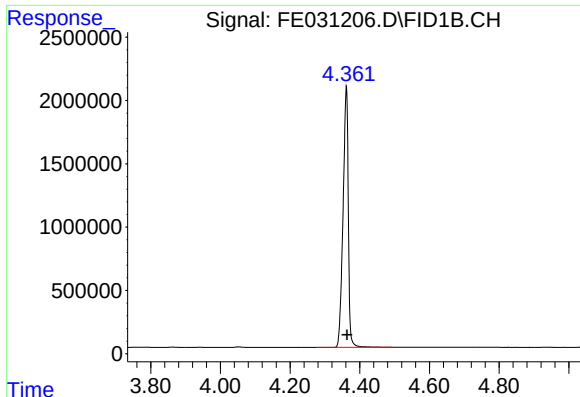


#2 N-DECANE

R.T.: 4.360 min
Delta R.T.: -0.003 min
Response: 21451276
Conc: 57.09 ug/ml

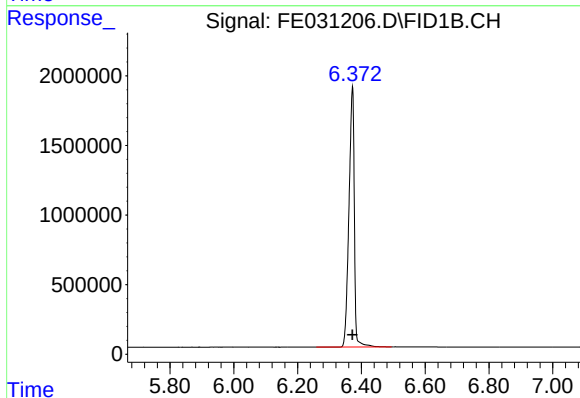


#3 N-DODECANE

R.T.: 6.370 min
Delta R.T.: -0.001 min
Response: 21759968
Conc: 61.65 ug/ml

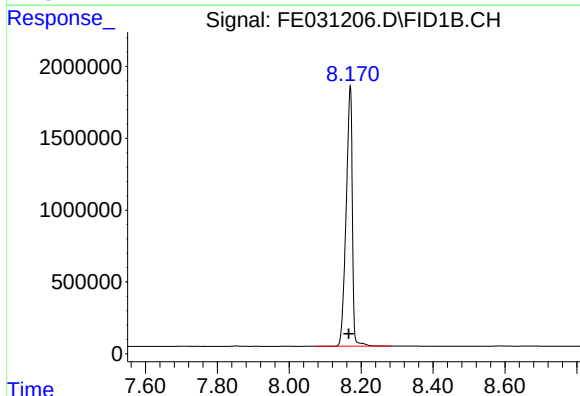


#4 N-TETRADECANE

R.T.: 8.168 min
Delta R.T.: 0.002 min
Response: 21578533
Conc: 56.43 ug/ml

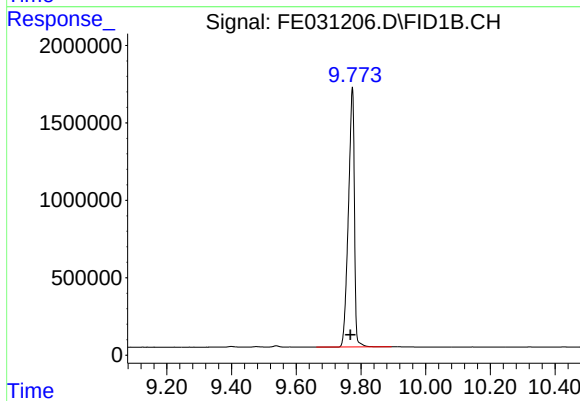


#5 N-HEXADECANE

R.T.: 9.771 min
Delta R.T.: 0.004 min
Response: 21480058
Conc: 55.48 ug/ml

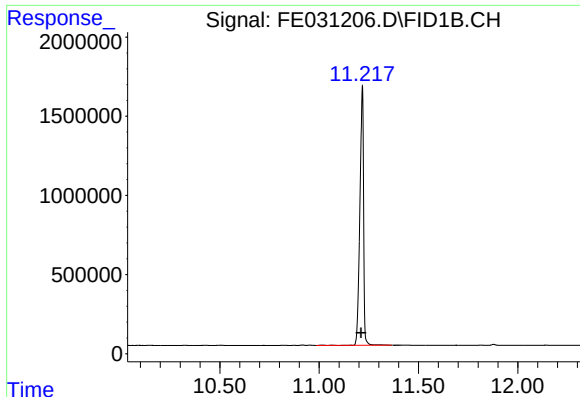


#6 N-OCTADECANE

R.T.: 11.215 min
Delta R.T.: 0.005 min
Response: 21210296
Conc: 55.13 ug/ml

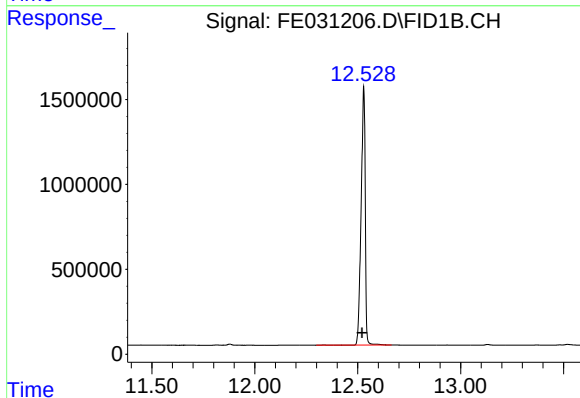


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: 0.006 min
Response: 21148588
Conc: 54.36 ug/ml

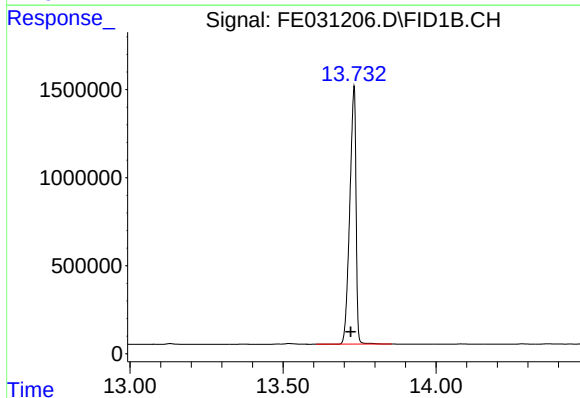


#8 N-DOCOSANE

R.T.: 13.730 min
Delta R.T.: 0.008 min
Response: 20811985
Conc: 53.89 ug/ml

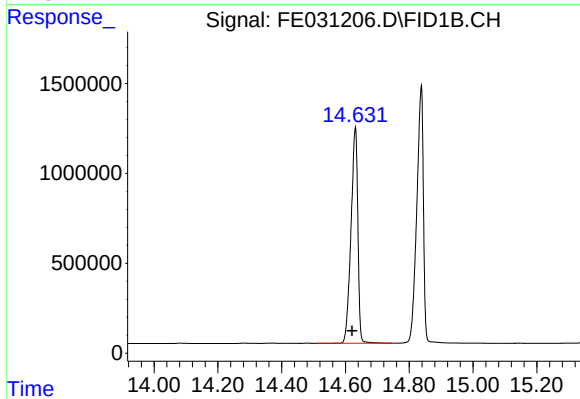


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: 0.009 min
Response: 17851793
Conc: 53.50 ug/ml

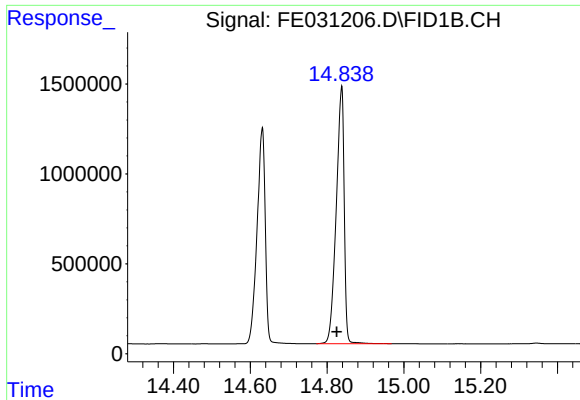


#10 N-TETRACOSANE

R.T.: 14.835 min
Delta R.T.: 0.010 min
Response: 20580209
Conc: 53.66 ug/ml

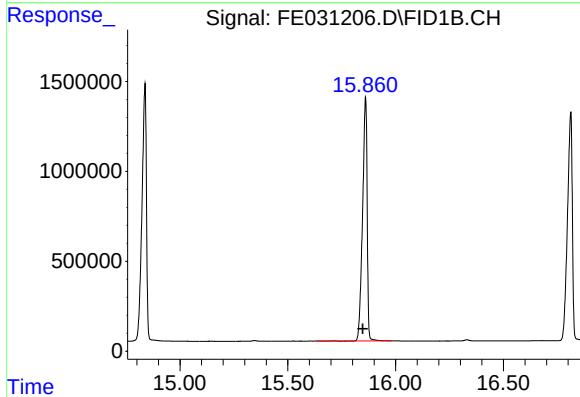

#11 N-HEXACOSANE

R.T.: 15.859 min
Delta R.T.: 0.011 min
Response: 20131685
Conc: 52.63 ug/ml

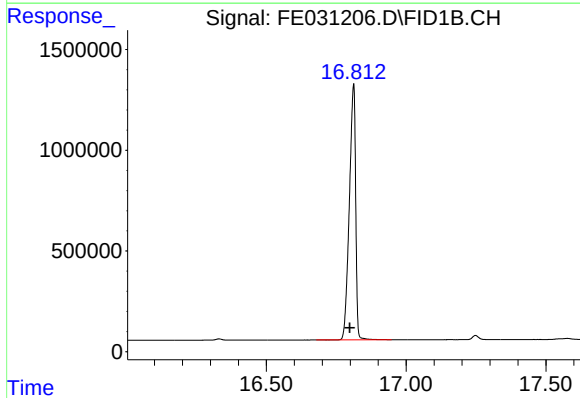

#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: 0.011 min
Response: 19898050
Conc: 51.76 ug/ml