

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012424AL\
 Data File : FE046369.D
 Signal(s) : FID1B.ch
 Acq On : 24 Jan 2024 09:57
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 25 00:16:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:49:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	15.124	70479	0.486 ug/ml
15) T n-Hexacosane (C26)	16.146	84592	0.590 ug/ml
16) T n-Octacosane (C28)	17.097	115882	0.808 ug/ml
17) T n-Tricontane (C30)	17.987	135940	0.915 ug/ml
18) T n-Dotriacontane (C32)	18.821	120969	0.809 ug/ml
19) T n-Tetratriacontane (C34)	19.606	72328	0.505 ug/ml
20) T n-Hexatriacontane (C36)	20.355	35865	0.246 ug/ml
22) T n-Tetracontane (C40)	21.958f	172566	1.102 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012424AL\
Data File : FE046369.D
Signal(s) : FID1B.ch
Acq On : 24 Jan 2024 09:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 25 00:16:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 122923.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:49:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

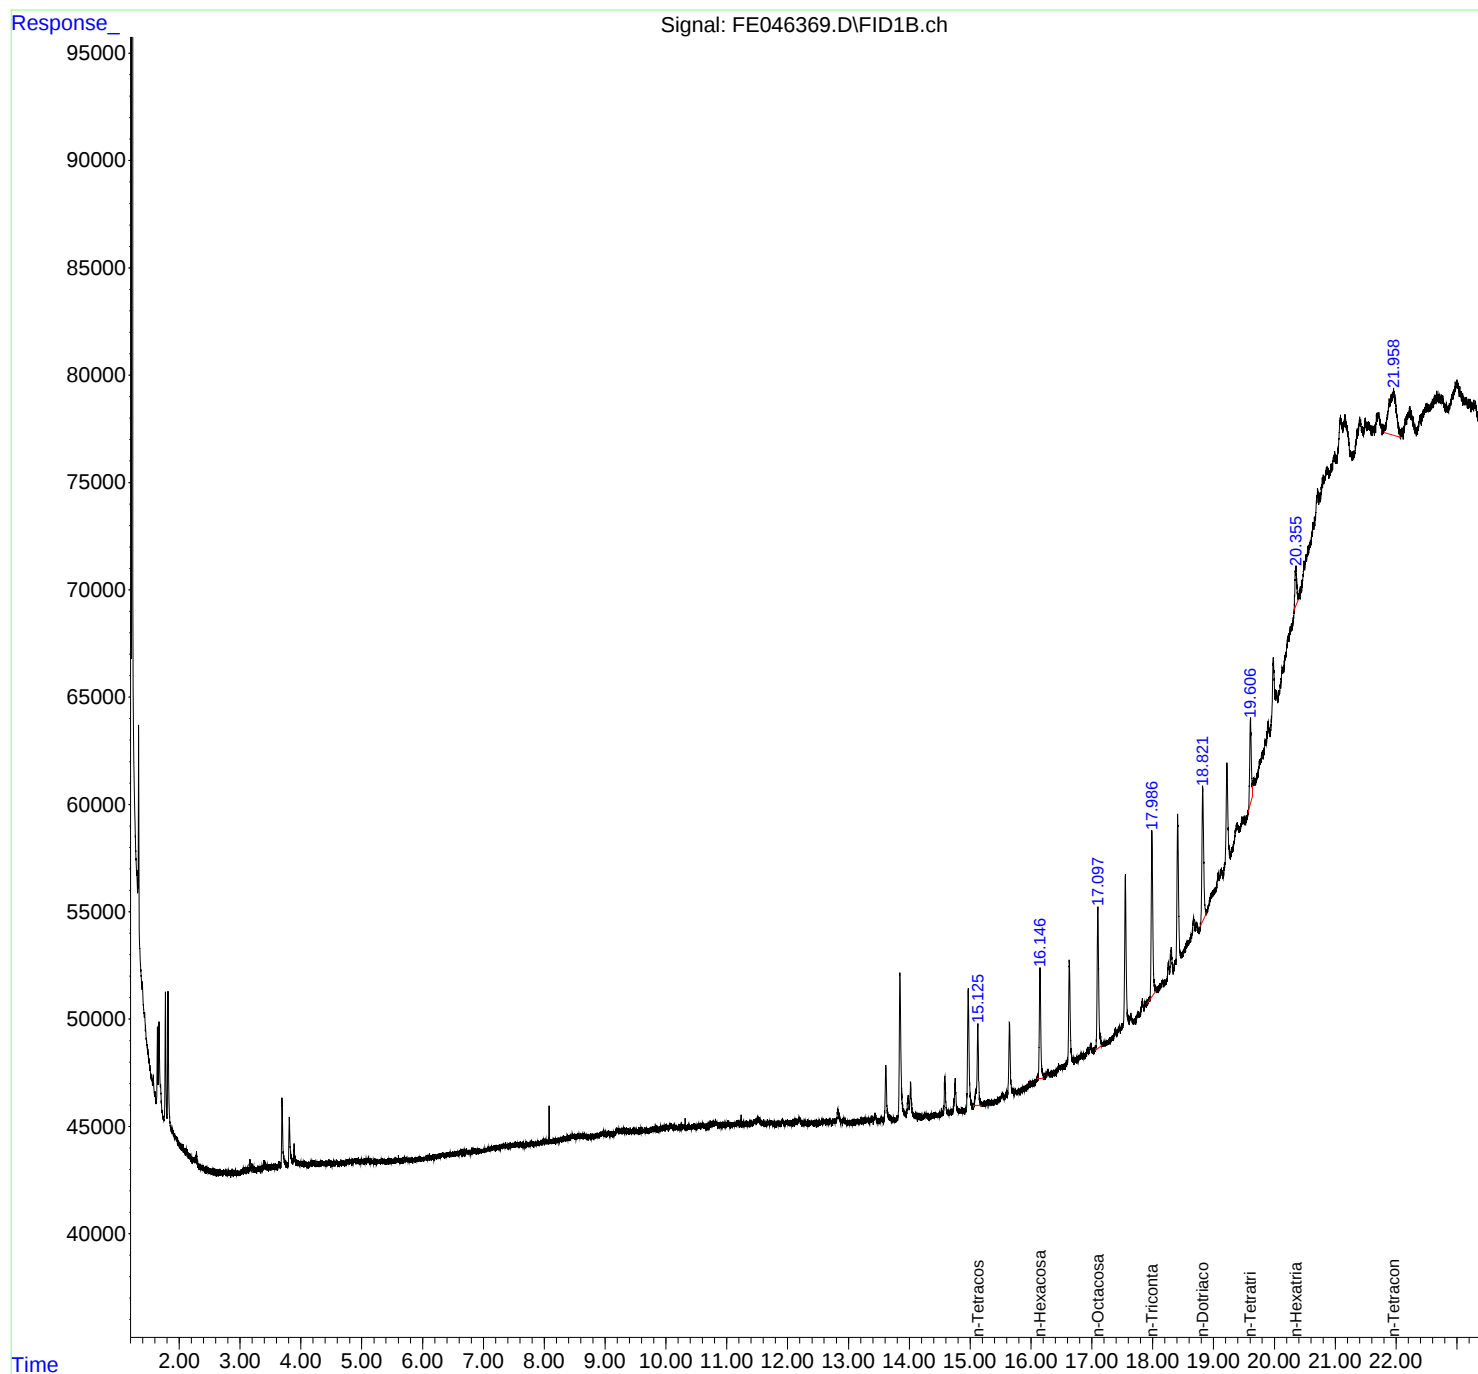

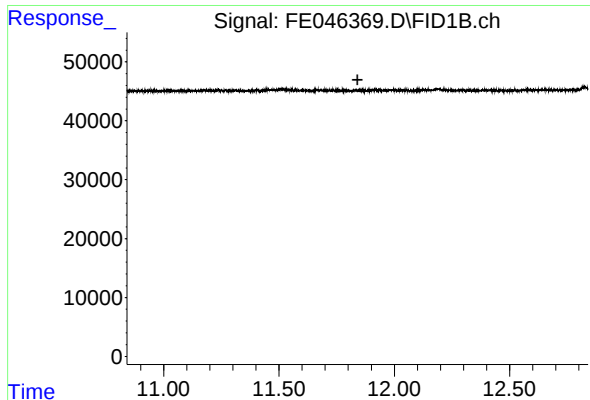


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.840 min
Response: 0
Conc: N.D.

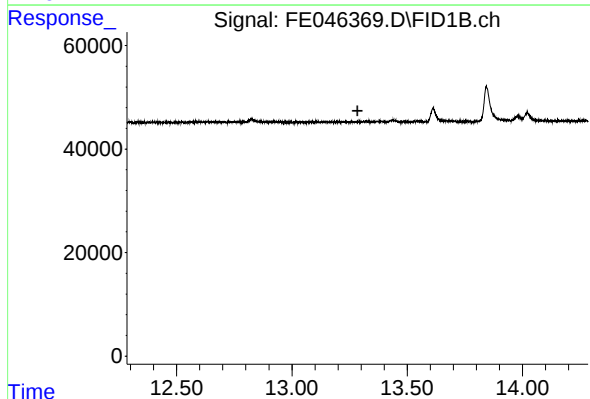


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.284 min
Response: 0
Conc: N.D.

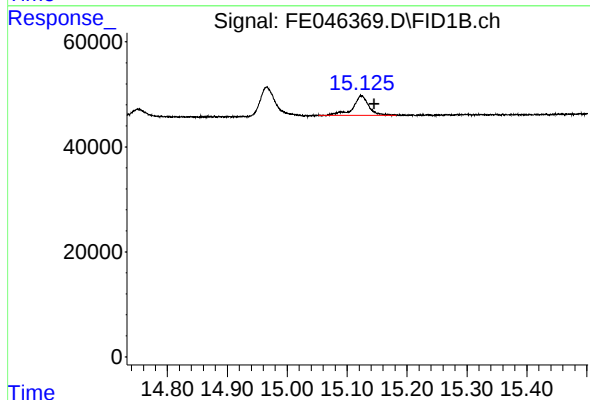


#14 n-Tetracosane (C24)

R.T.: 15.124 min
Delta R.T.: -0.021 min
Response: 70479
Conc: 0.49 ug/ml

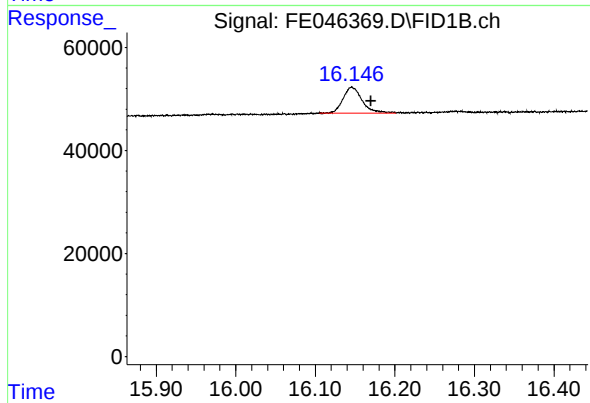


#15 n-Hexacosane (C26)

R.T.: 16.146 min
Delta R.T.: -0.024 min
Response: 84592
Conc: 0.59 ug/ml

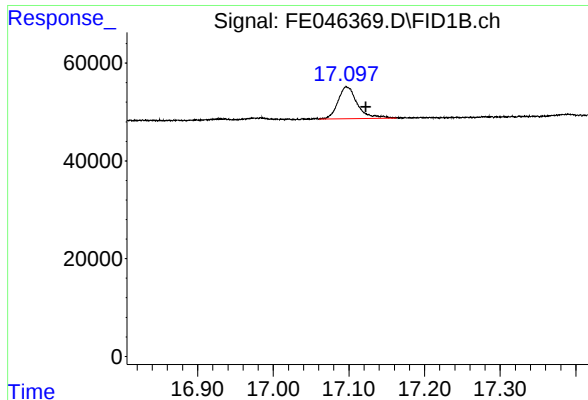


#16 n-Octacosane (C28)

R.T.: 17.097 min
Delta R.T.: -0.026 min
Response: 115882
Conc: 0.81 ug/ml

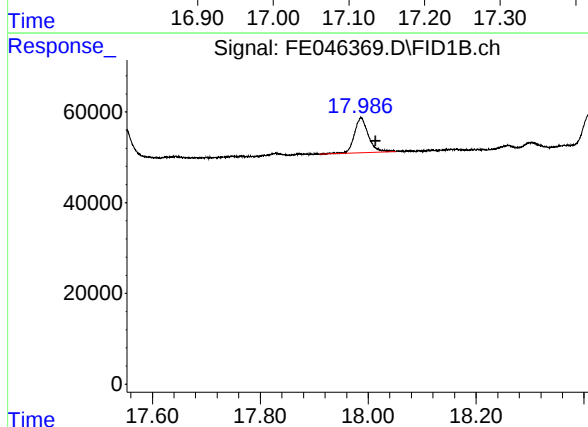


#17 n-Tricontane (C30)

R.T.: 17.987 min
Delta R.T.: -0.027 min
Response: 135940
Conc: 0.91 ug/ml

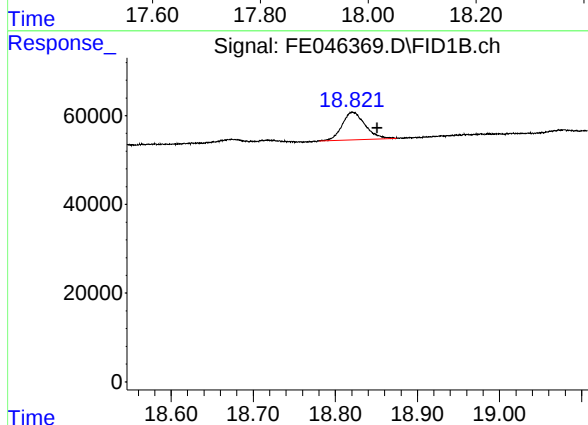


#18 n-Dotriacontane (C32)

R.T.: 18.821 min
Delta R.T.: -0.031 min
Response: 120969
Conc: 0.81 ug/ml

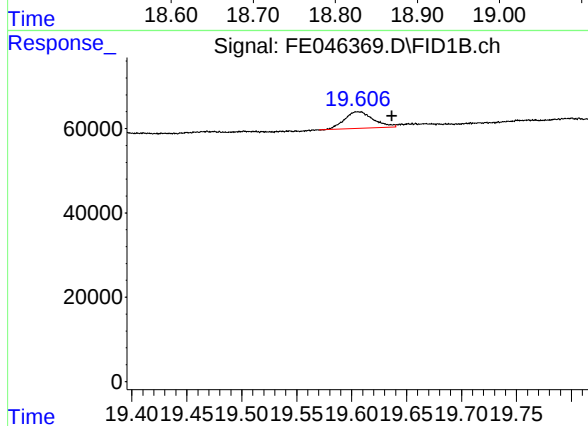


#19 n-Tetratriacontane (C34)

R.T.: 19.606 min
Delta R.T.: -0.031 min
Response: 72328
Conc: 0.50 ug/ml

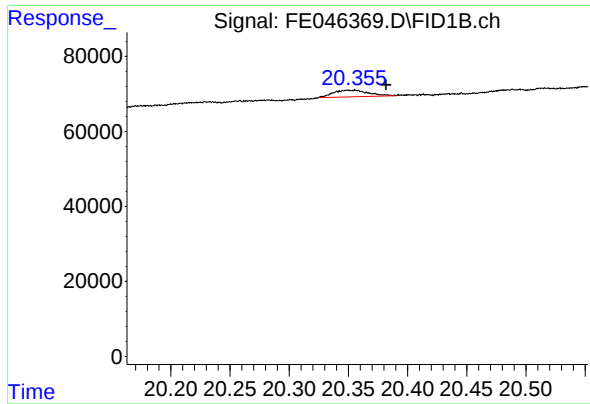

#20 n-Hexatriacontane (C36)

R.T.: 20.355 min
Delta R.T.: -0.027 min
Response: 35865
Conc: 0.25 ug/ml

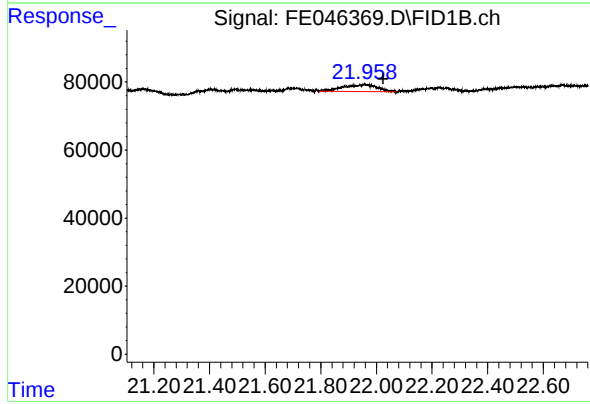

#22 n-Tetracontane (C40)

R.T.: 21.958 min
Delta R.T.: -0.068 min
Response: 172566
Conc: 1.10 ug/ml