

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE012523AL\  
Data File : FE040025.D  
Signal(s) : FID1B.ch  
Acq On : 25 Jan 2023 08:10  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jan 26 02:45:59 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 011023.M  
Quant Title : GC Extractables  
QLast Update : Tue Jan 10 04:24:52 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|       |                         |        |       |             |
|-------|-------------------------|--------|-------|-------------|
| 20) T | n-Hexatriacontane (C36) | 20.416 | 57594 | 0.489 ug/ml |
|-------|-------------------------|--------|-------|-------------|


-----  
(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE012523AL\  
Data File : FE040025.D  
Signal(s) : FID1B.ch  
Acq On : 25 Jan 2023 08:10  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jan 26 02:45:59 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 011023.M  
Quant Title : GC Extractables  
QLast Update : Tue Jan 10 04:24:52 2023  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

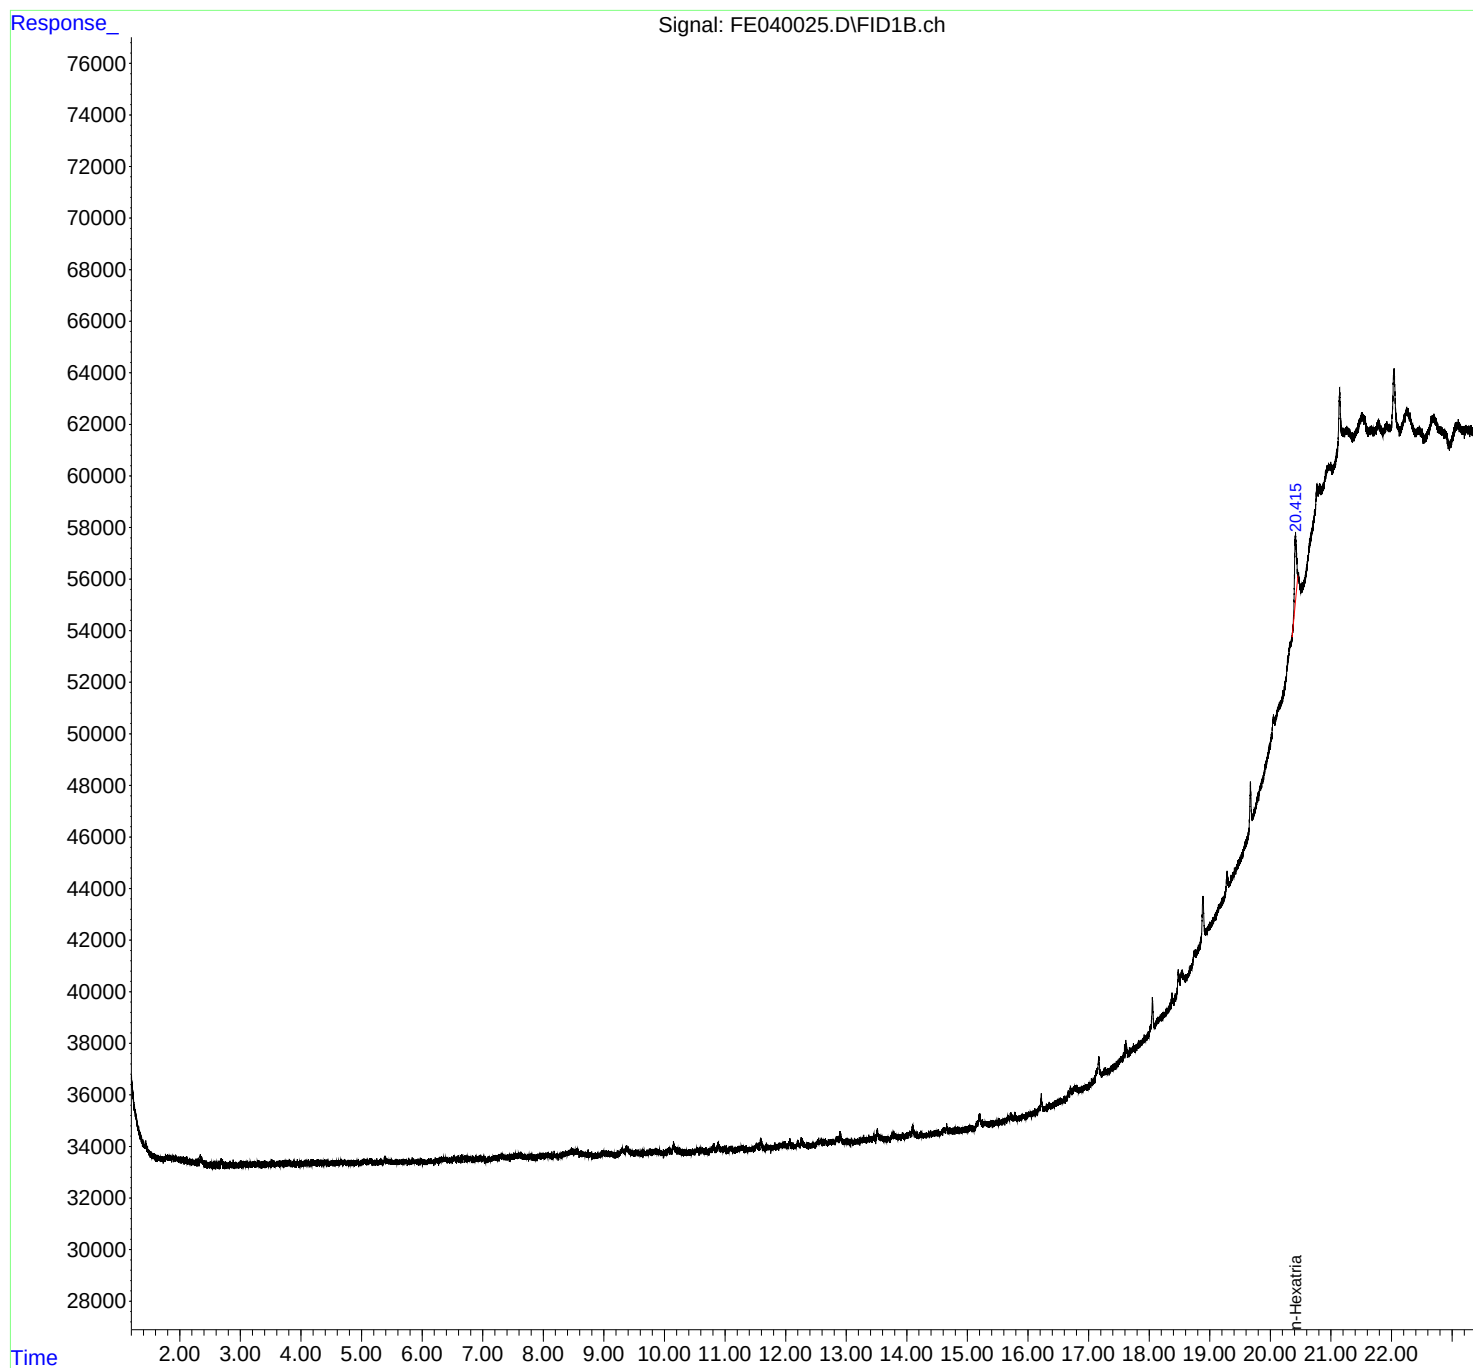

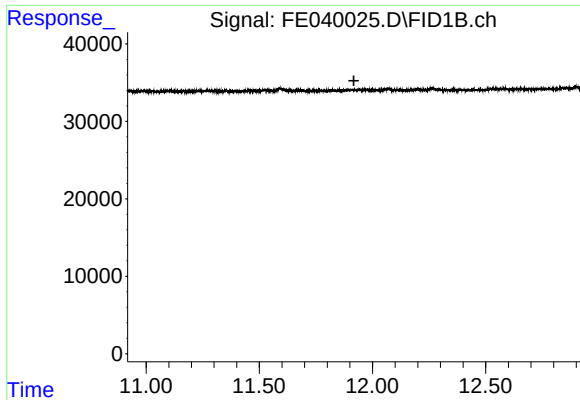


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min  
Exp R.T. : 11.918 min  
Response: 0  
Conc: N.D.

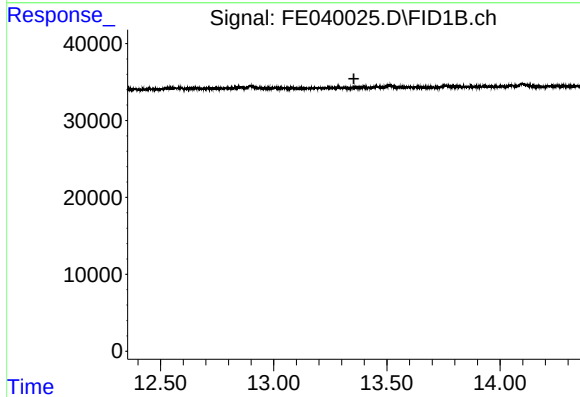

#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T. : 13.354 min  
Response: 0  
Conc: N.D.

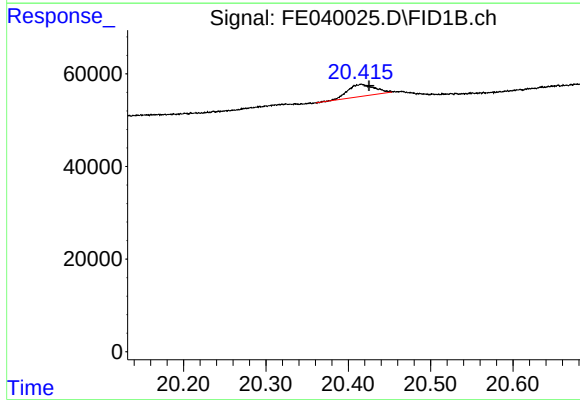

#20 n-Hexatriacontane (C36)

R.T.: 20.416 min  
Delta R.T.: -0.009 min  
Response: 57594  
Conc: 0.49 ug/ml