

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012525\
Data File : FE052082.D
Signal(s) : FID1B.ch
Acq On : 25 Jan 2025 08:29
Operator : YP\AJ
Sample : PB166207BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB166207BL

Integration File: autoint1.e
Quant Time: Jan 27 02:37:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.246	1825337	18.327 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012525\
Data File : FE052082.D
Signal(s) : FID1B.ch
Acq On : 25 Jan 2025 08:29
Operator : YP\AJ
Sample : PB166207BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB166207BL

Integration File: autoint1.e
Quant Time: Jan 27 02:37:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

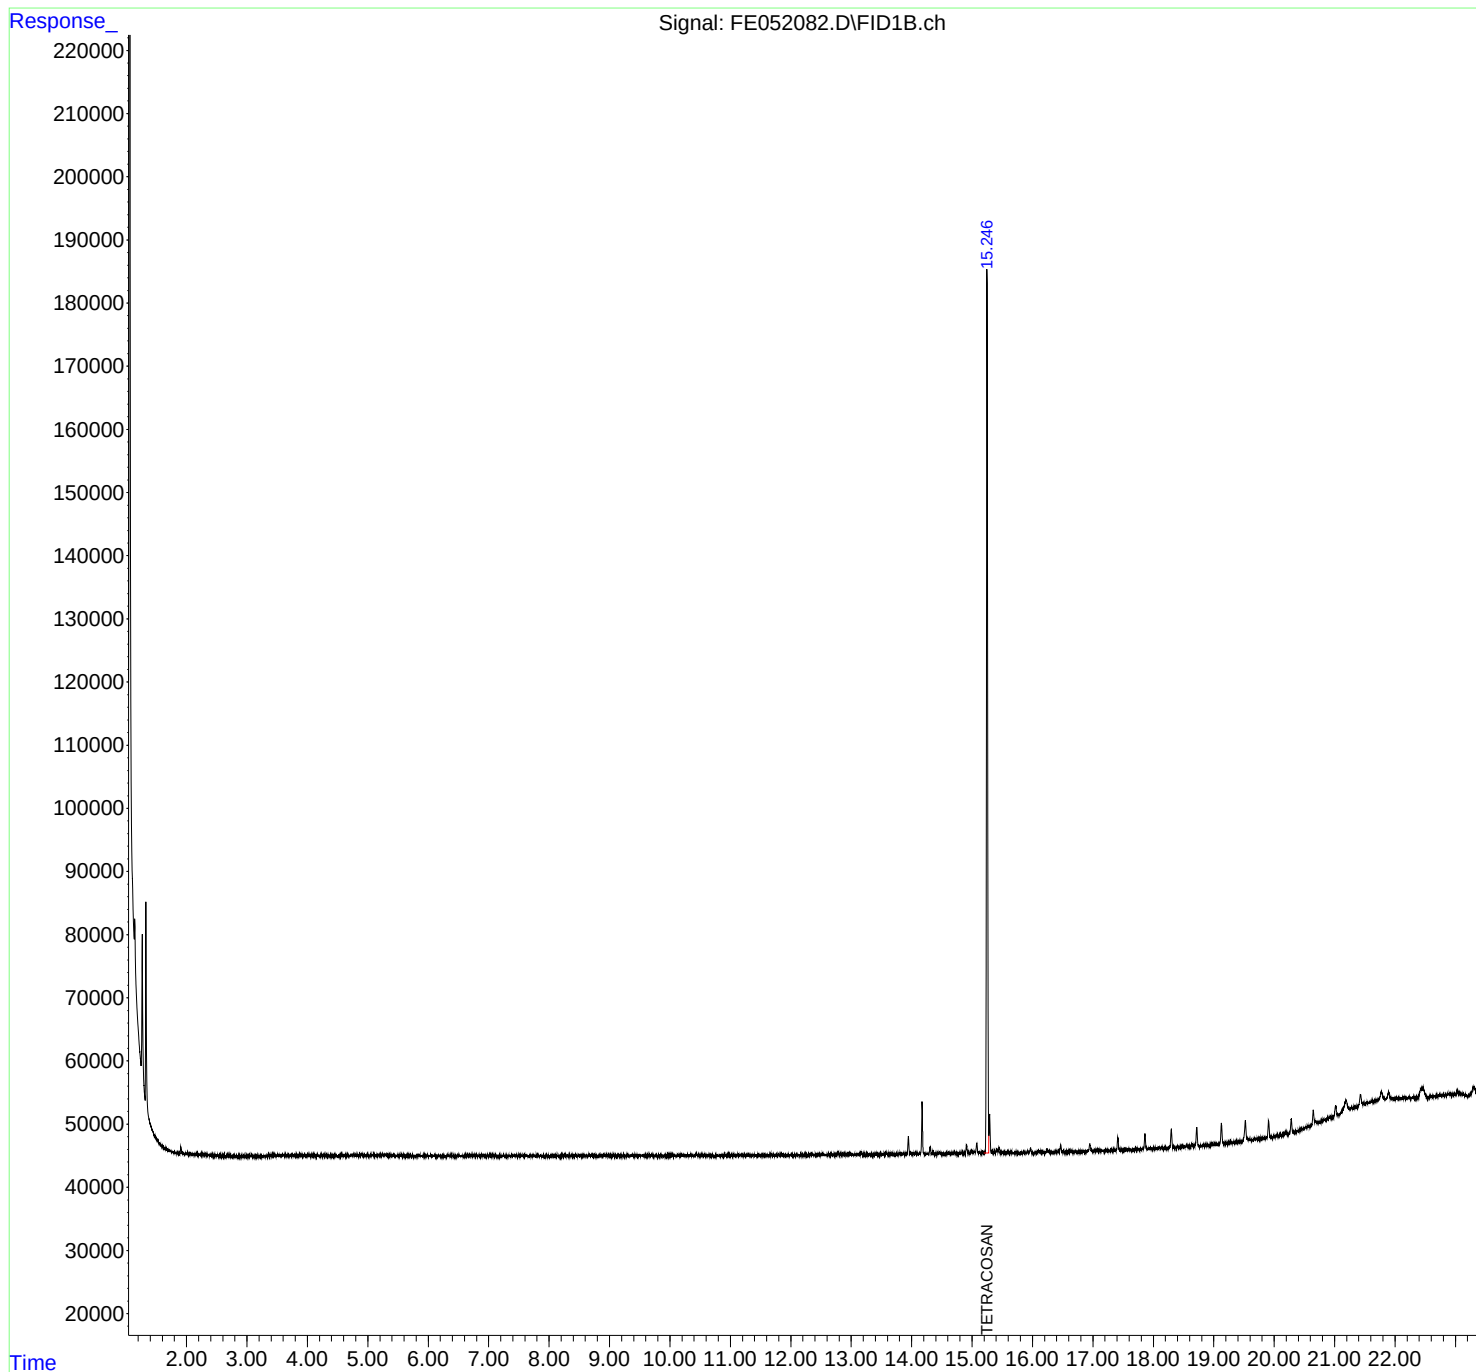

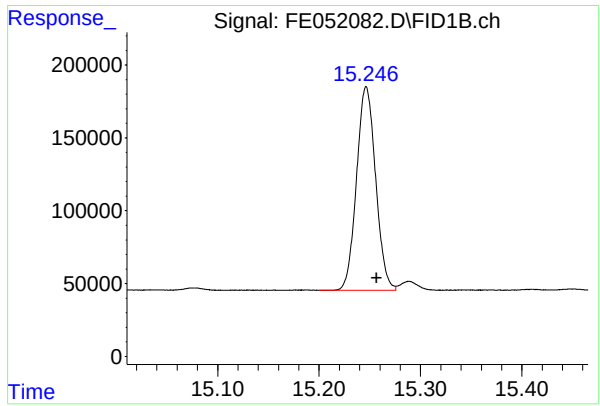

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.246 min
Delta R.T.: -0.010 min
Response: 1825337
Conc: 18.33 ug/ml

Instrument :
FID_E
ClientSampleId :
PB166207BL