

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012925\
Data File : FE052145.D
Signal(s) : FID1B.ch
Acq On : 30 Jan 2025 06:28
Operator : YP\AJ
Sample : Q1206-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-16.3-012725

Integration File: autoint1.e
Quant Time: Jan 30 06:59:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.260	1406969	14.126 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012925\
Data File : FE052145.D
Signal(s) : FID1B.ch
Acq On : 30 Jan 2025 06:28
Operator : YP\AJ
Sample : Q1206-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-16.3-012725

Integration File: autoint1.e
Quant Time: Jan 30 06:59:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

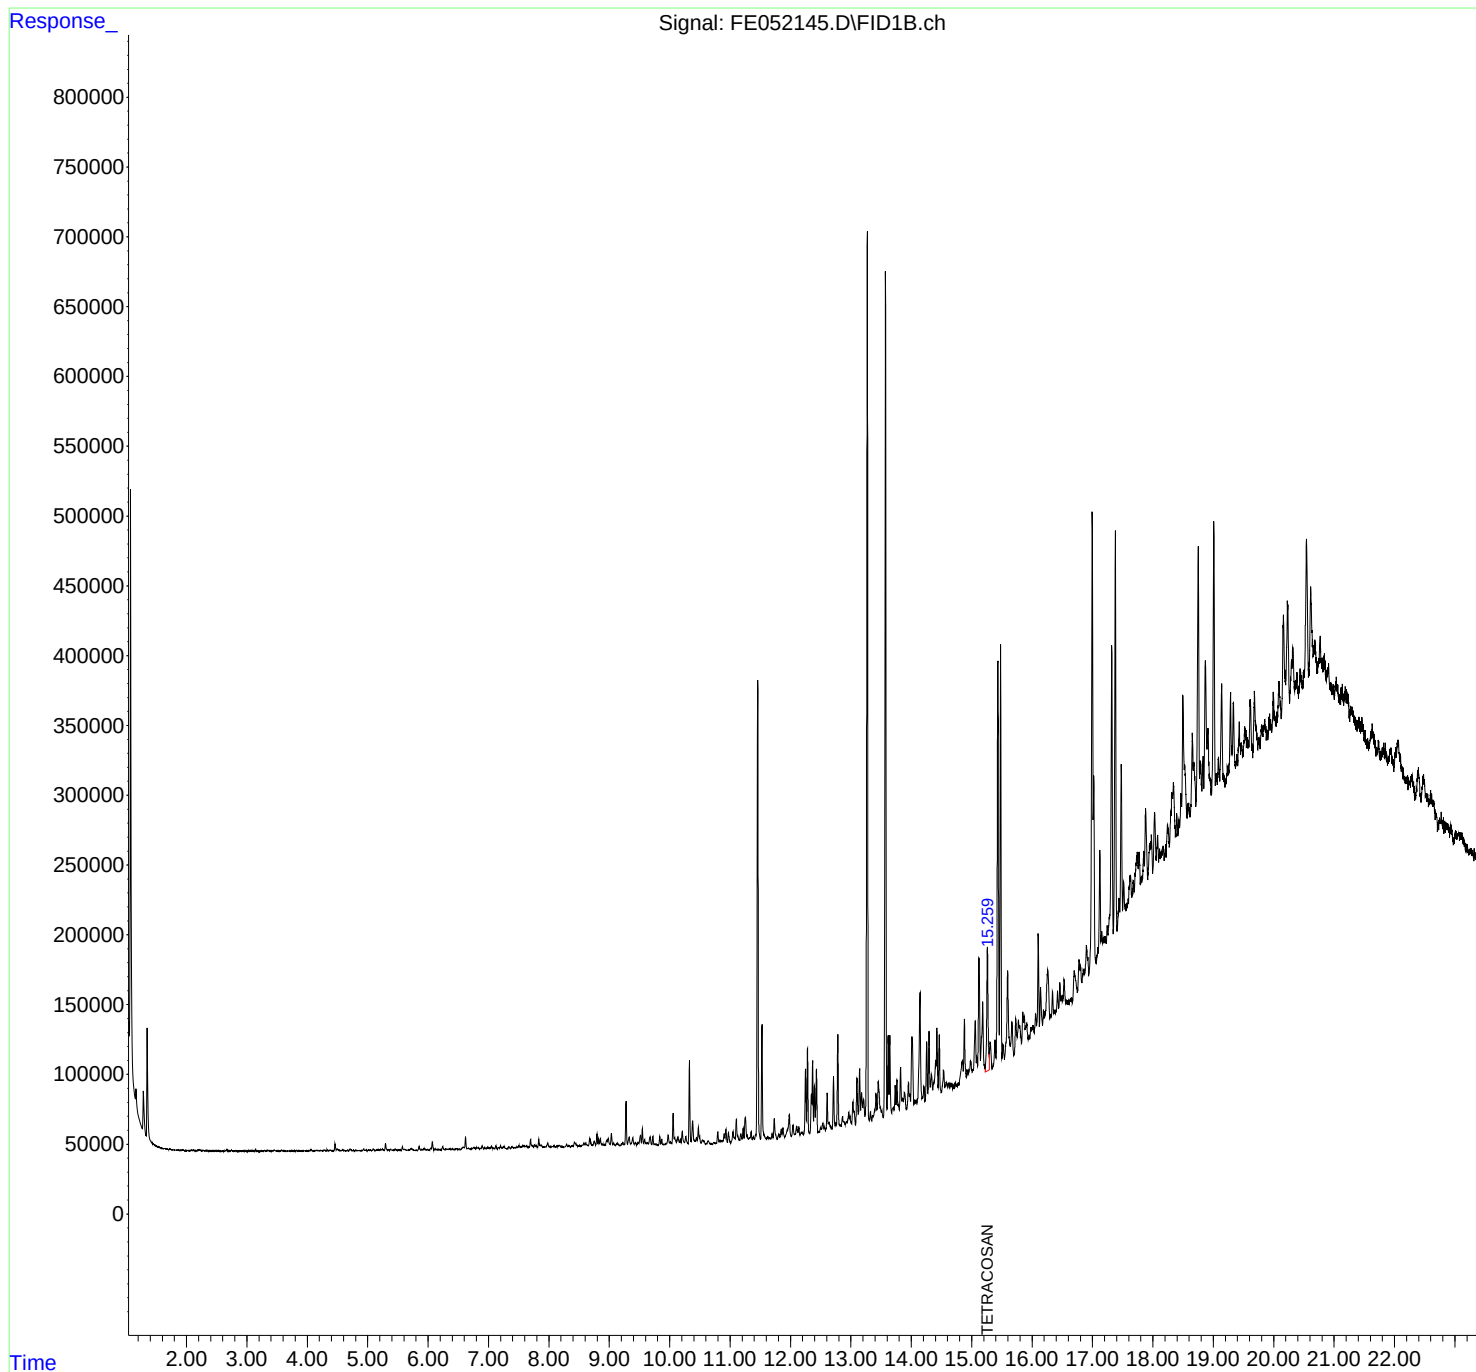

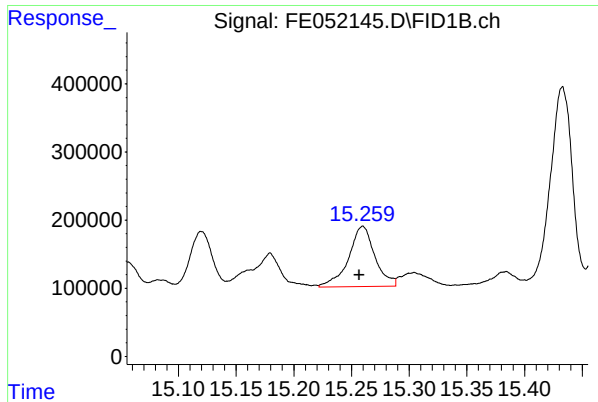

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.260 min
Delta R.T.: 0.003 min
Response: 1406969
Conc: 14.13 ug/ml

Instrument :
FID_E
ClientSampleId :
JPP-16.3-012725