

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012925\
Data File : FE052155.D
Signal(s) : FID1B.ch
Acq On : 30 Jan 2025 12:30
Operator : YP\AJ
Sample : Q1207-09RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-4.5-012725RE

Integration File: autoint1.e
Quant Time: Jan 31 02:02:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.273	518675	5.208 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012925\
Data File : FE052155.D
Signal(s) : FID1B.ch
Acq On : 30 Jan 2025 12:30
Operator : YP\AJ
Sample : Q1207-09RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JPP-4.5-012725RE

Integration File: autoint1.e
Quant Time: Jan 31 02:02:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

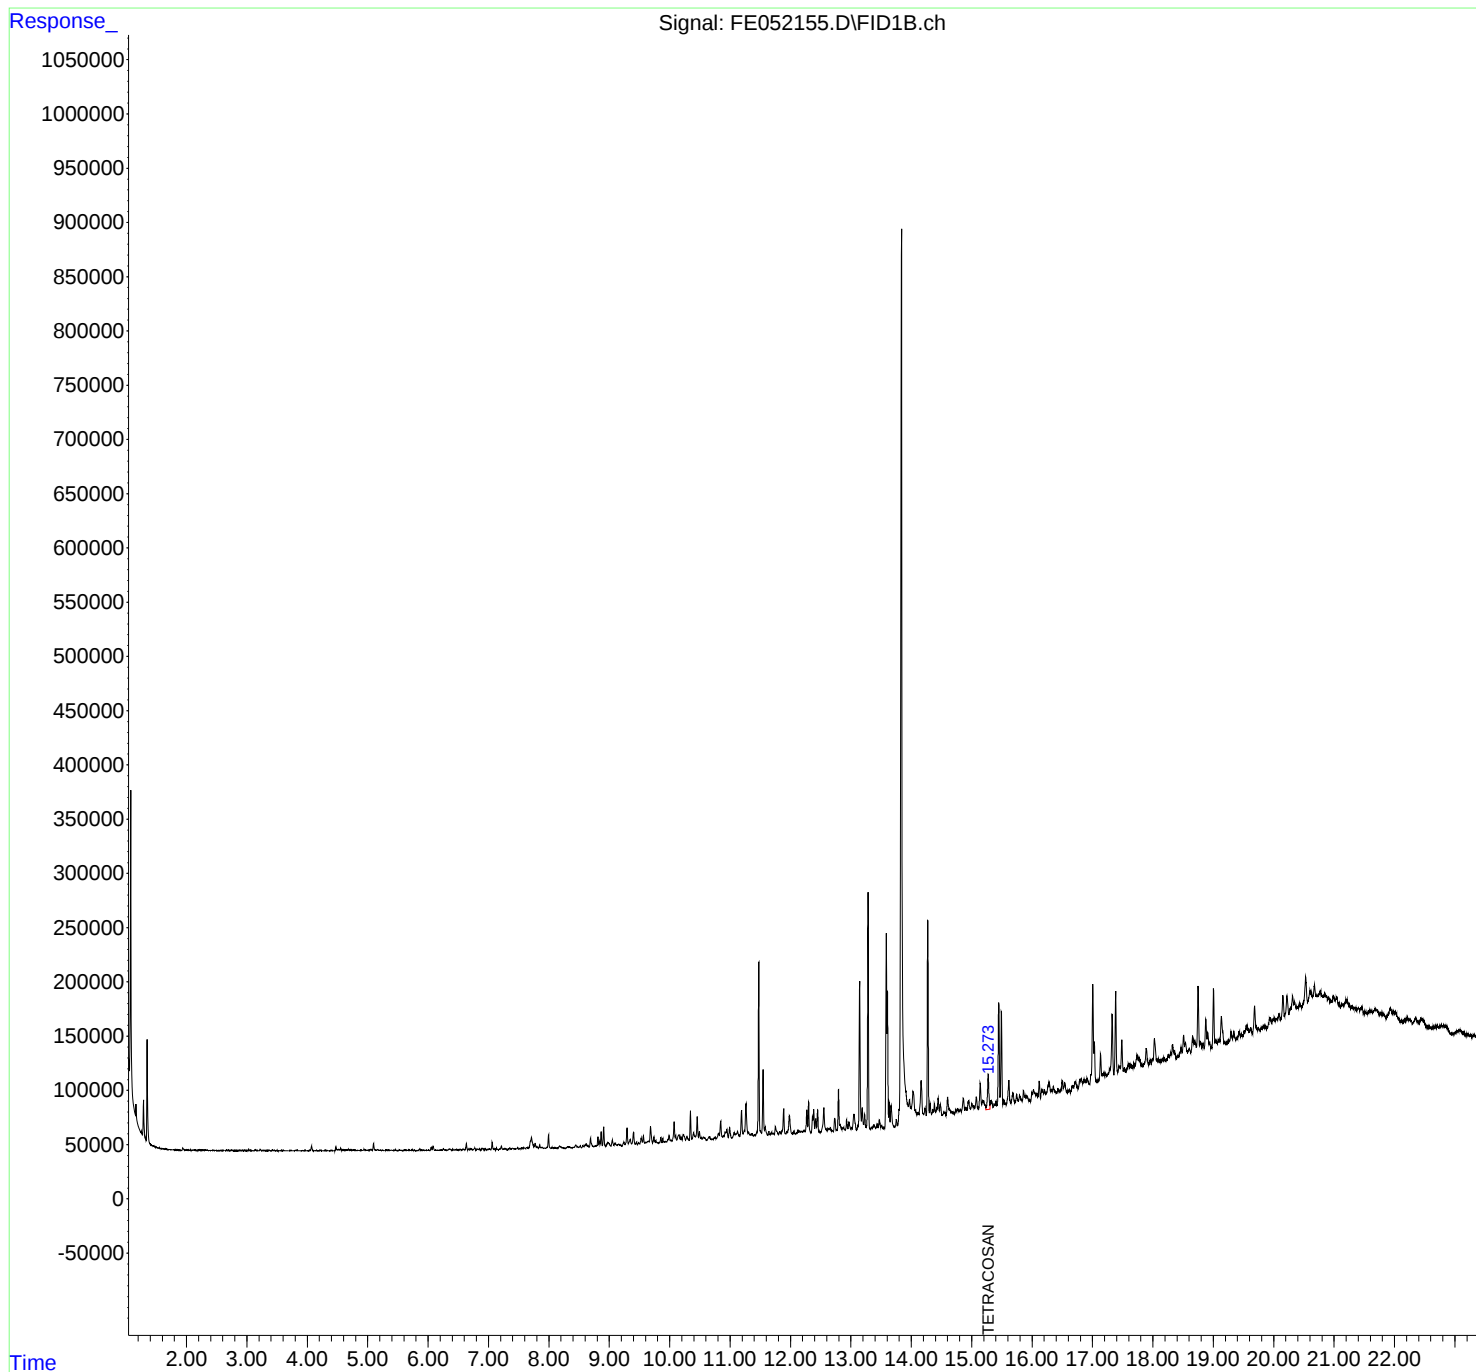

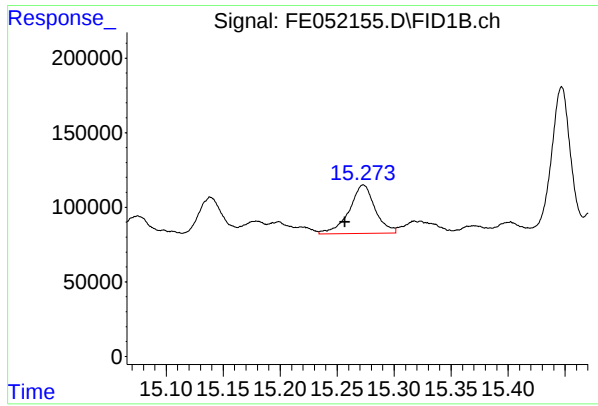

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.273 min
Delta R.T.: 0.016 min
Response: 518675
Conc: 5.21 ug/ml

Instrument :
FID_E
ClientSampleId :
JPP-4.5-012725RE